

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB042319\  
Data File : FB020819.D  
Signal(s) : FID2B.CH  
Acq On : 23 Apr 2019 20:01  
Operator : MJ/SJ  
Sample : K2532-21  
Misc : 5.05g/5.00ml DI WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Apr 24 07:30:40 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB040419.M  
Quant Title :  
QLast Update : Thu Apr 04 17:27:15 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 8.999  | 327803   | 17.773 ng/ml |
| Target Compounds            |        |          |              |
| 2) t 2,2,4-Trimethylpentane | 7.622  | 41643    | 1.397 ng/ml  |
| 4) t Benzene                | 8.109  | 5683     | 0.138 ng/ml  |
| 6) t Toluene                | 10.854 | 8227     | 0.272 ng/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB042319\  
Data File : FB020819.D  
Signal(s) : FID2B.CH  
Acq On : 23 Apr 2019 20:01  
Operator : MJ/SJ  
Sample : K2532-21  
Misc : 5.05g/5.00ml DI WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Apr 24 07:30:40 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB040419.M  
Quant Title :  
QLast Update : Thu Apr 04 17:27:15 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

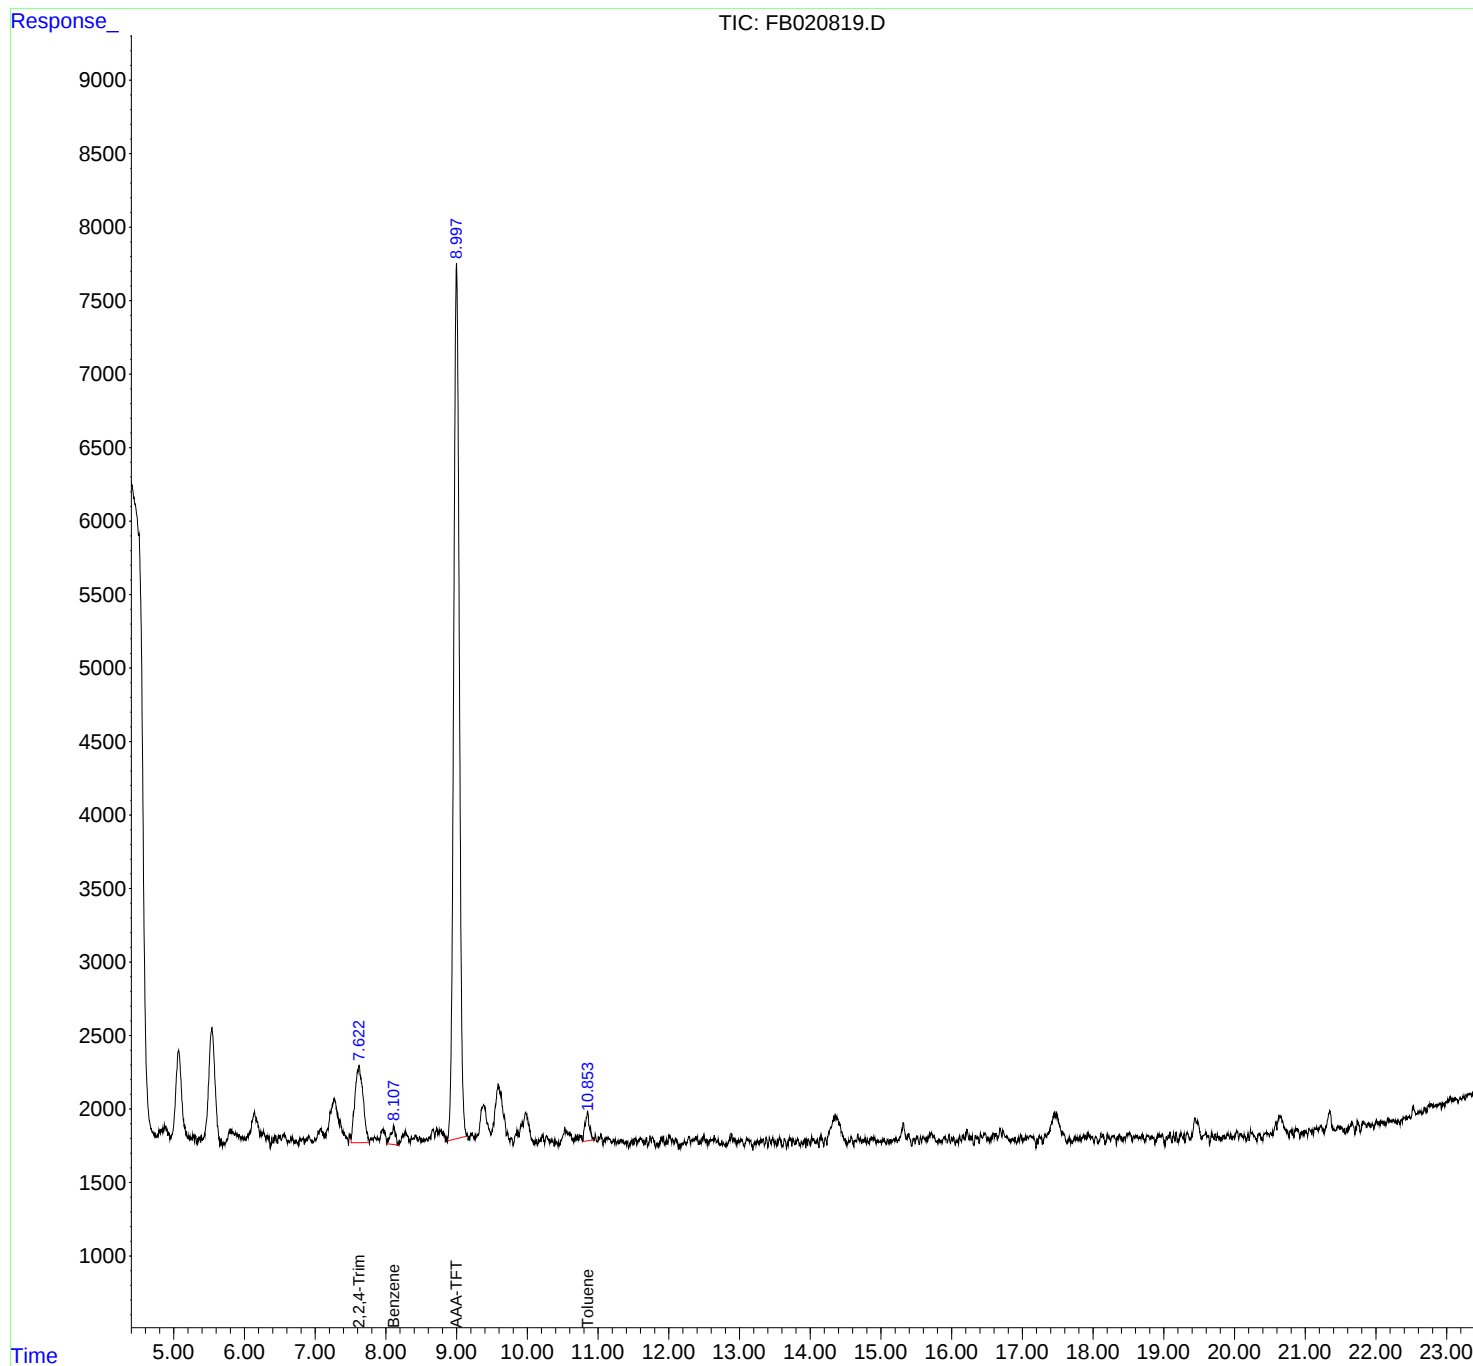


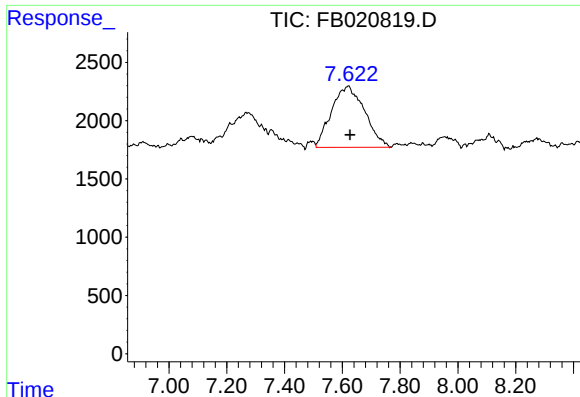

#2 2,2,4-Trimethylpentane


R.T.: 7.622 min  
Delta R.T.: -0.004 min  
Response: 41643  
Conc: 1.40 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

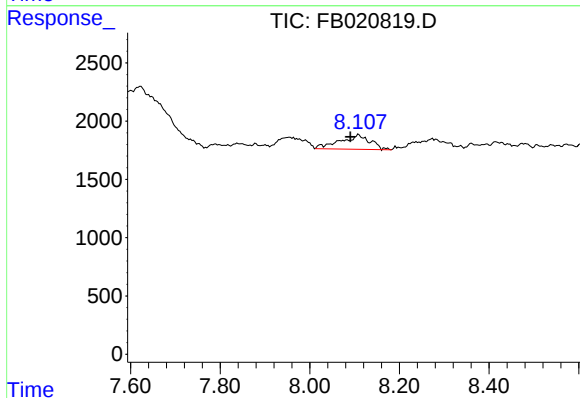


#4 Benzene

R.T.: 8.109 min  
Delta R.T.: 0.018 min  
Response: 5683  
Conc: 0.14 ng/ml

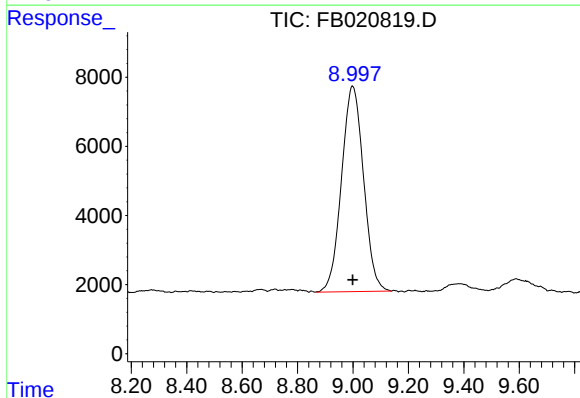

#5 AAA-TFT

R.T.: 8.999 min  
Delta R.T.: 0.000 min  
Response: 327803  
Conc: 17.77 ng/ml

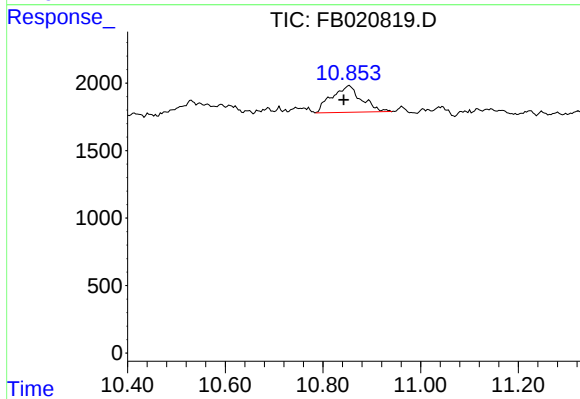

#6 Toluene

R.T.: 10.854 min  
Delta R.T.: 0.012 min  
Response: 8227  
Conc: 0.27 ng/ml