

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042321\
Data File : FB025631.D
Signal(s) : FID2B.CH
Acq On : 23 Apr 2021 10:41
Operator : DD/AJ
Sample : M2090-03
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1

Integration File: Calibration.e
Quant Time: Apr 23 13:08:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.242	417694	21.240 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042321\
Data File : FB025631.D
Signal(s) : FID2B.CH
Acq On : 23 Apr 2021 10:41
Operator : DD/AJ
Sample : M2090-03
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1

Integration File: Calibration.e
Quant Time: Apr 23 13:08:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

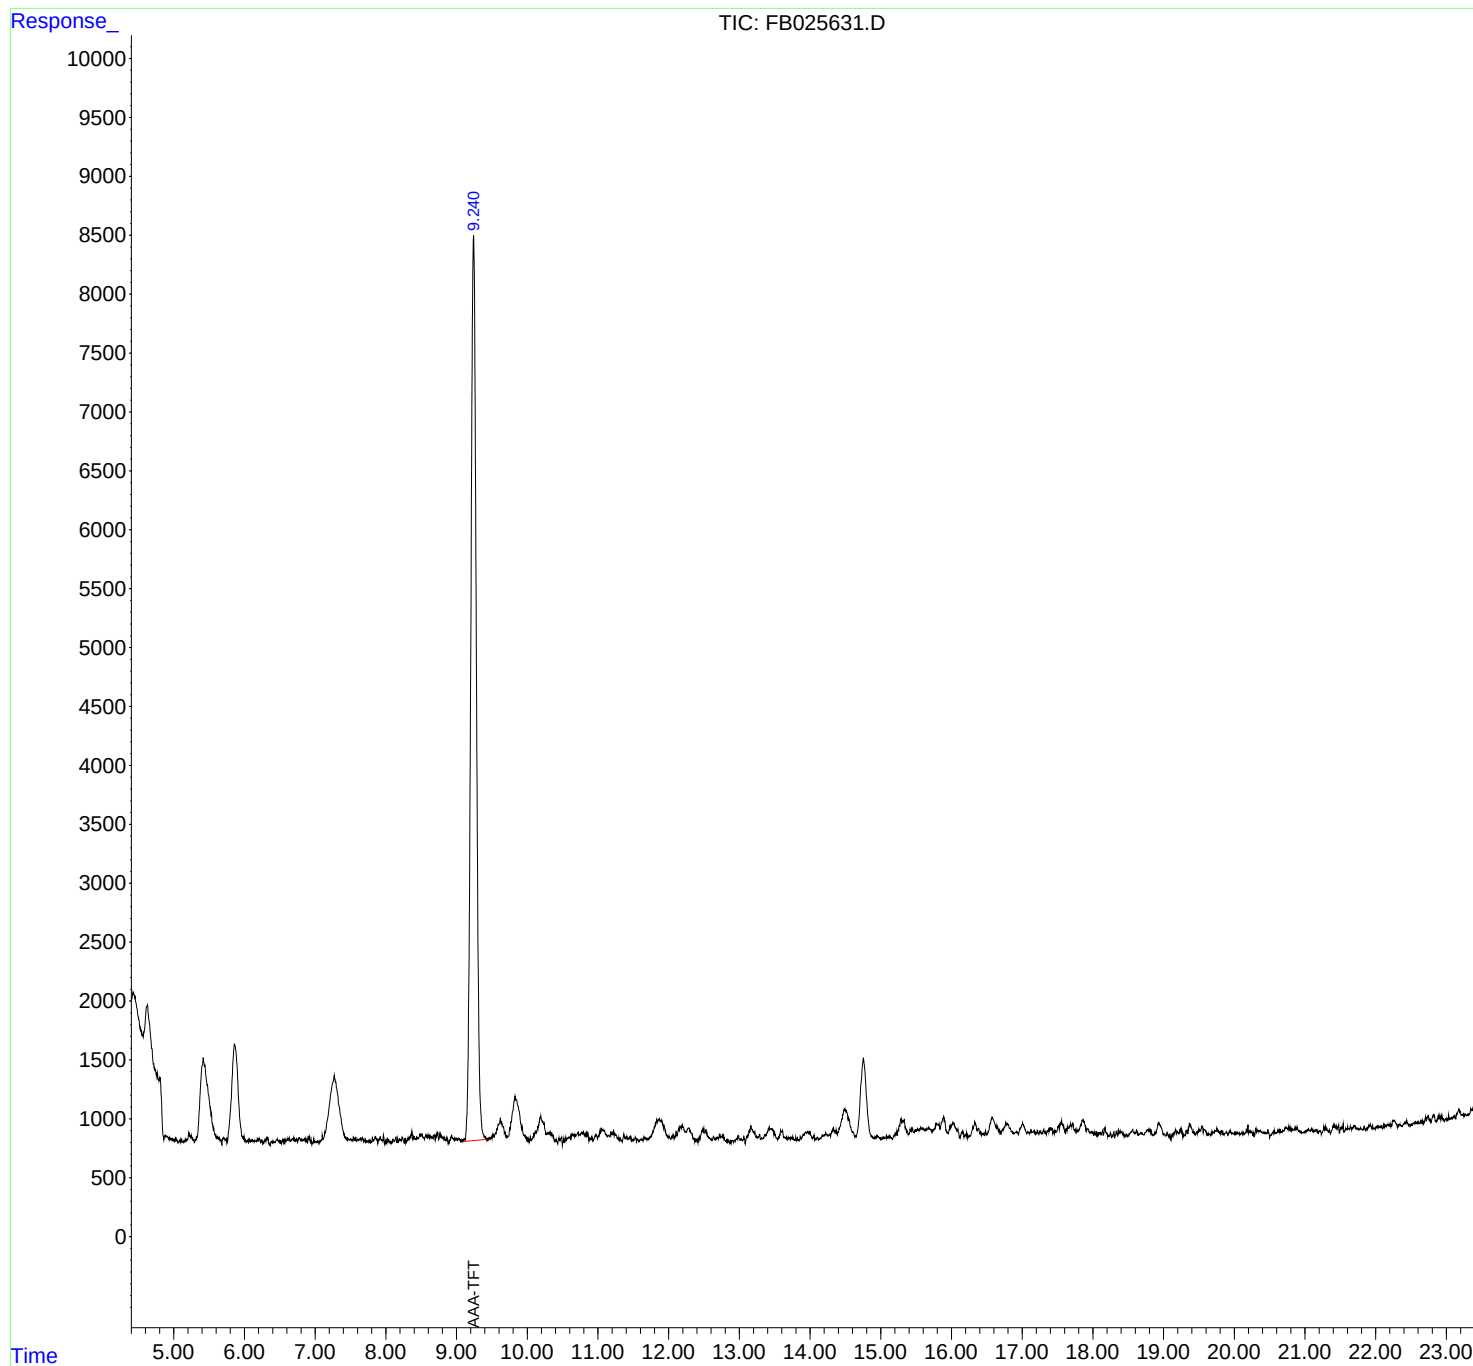

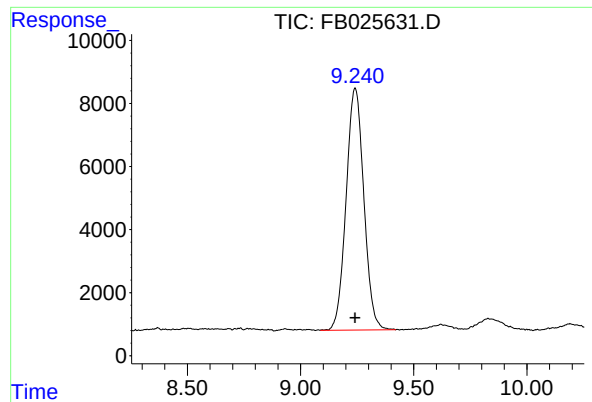

#5 AAA-TFT

R.T.: 9.242 min
Delta R.T.: 0.000 min
Response: 417694
Conc: 21.24 ng/ml

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1