

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042321\
 Data File : FB025636.D
 Signal(s) : FID2B.CH
 Acq On : 23 Apr 2021 13:37
 Operator : DD/AJ
 Sample : M2090-03MS
 Misc : 4.99g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SEDGWICK-COMP-1MS

Integration File: Calibration.e
 Quant Time: Apr 23 14:44:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.242	389650	19.814 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.210	649004	26.827 ng/ml
2) t 2,2,4-Trimethylpentane	7.899	586928	31.558 ng/ml
3) t n-Heptane	8.220	264772	9.037 ng/ml
4) t Benzene	8.371	368362	9.534 ng/ml
6) t Toluene	11.061	1049562	29.079 ng/ml
7) t Ethylbenzene	13.468	339113	9.891 ng/ml
8) t m-Xylene	13.599	672304	19.778 ng/ml
9) t O-Xylene	14.322	633394	19.442 ng/ml
10) t 1,2,4-Trimethylbenzene	16.575	508043	19.326 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042321\
Data File : FB025636.D
Signal(s) : FID2B.CH
Acq On : 23 Apr 2021 13:37
Operator : DD/AJ
Sample : M2090-03MS
Misc : 4.99g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1MS

Integration File: Calibration.e
Quant Time: Apr 23 14:44:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

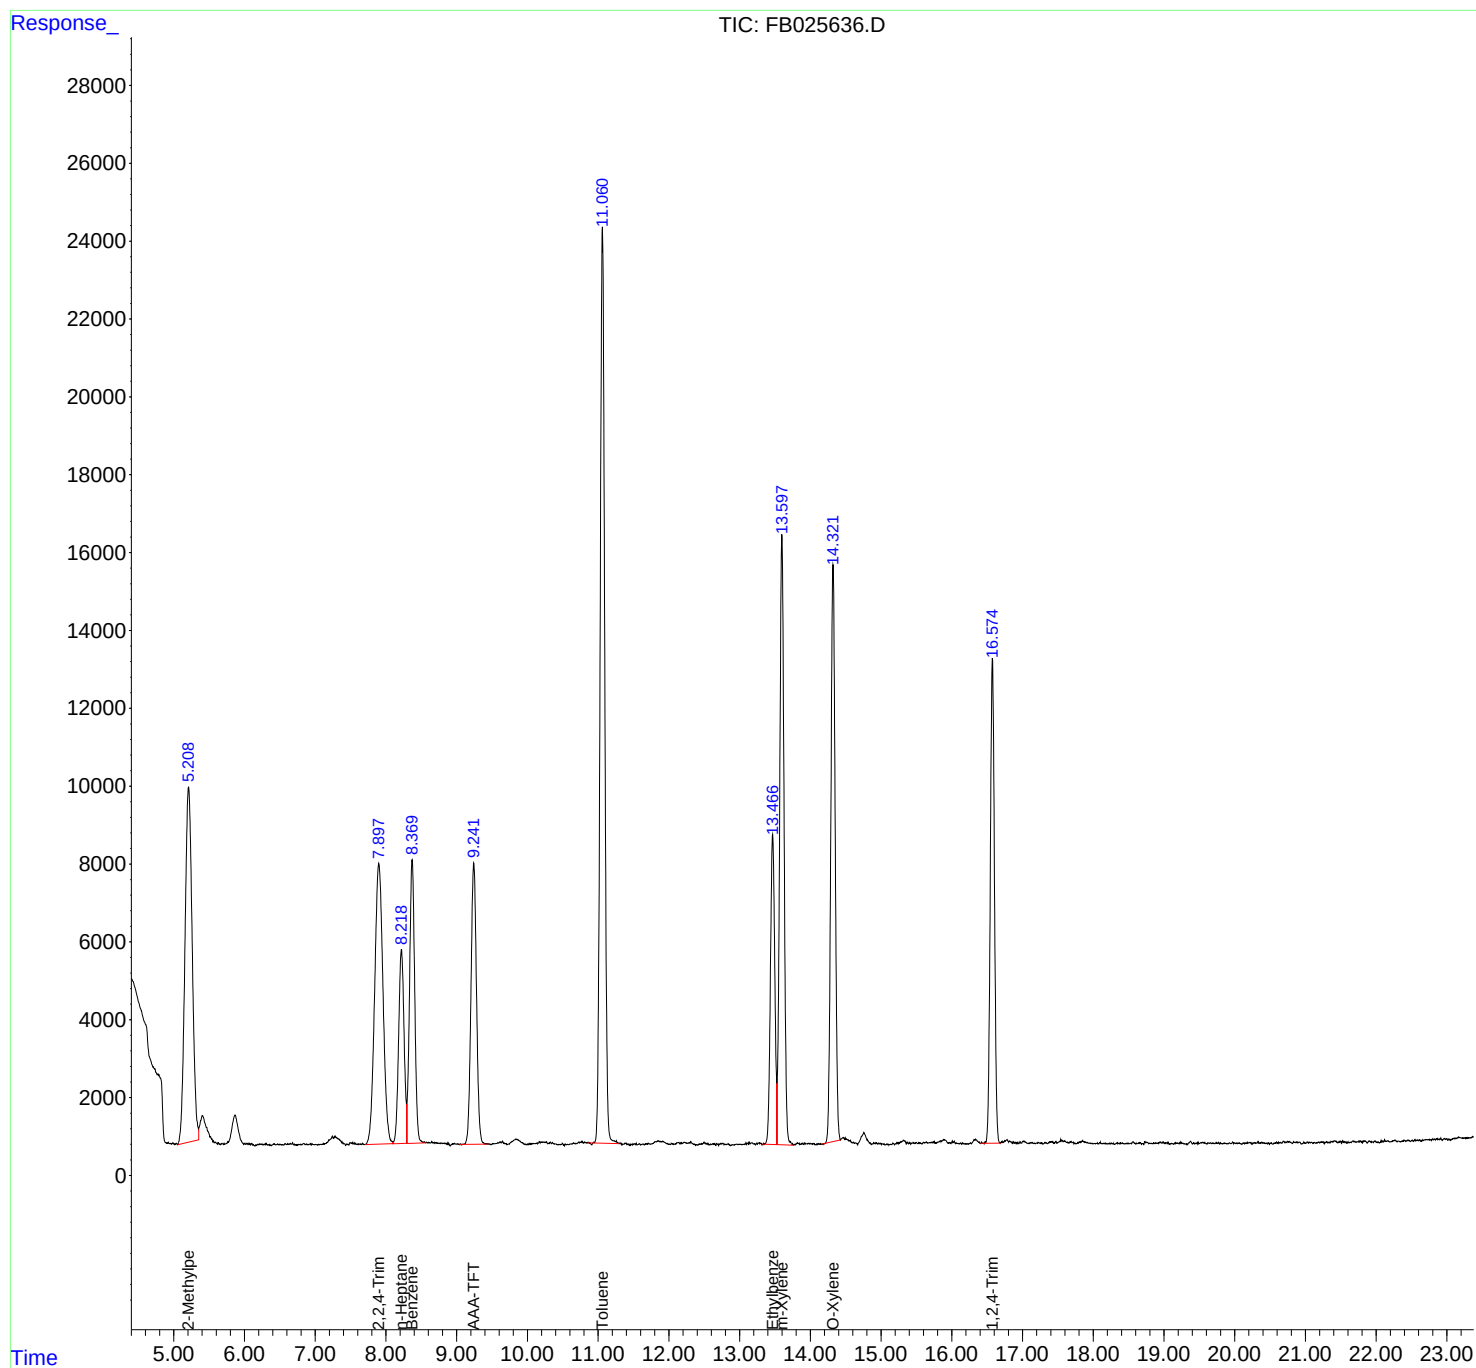


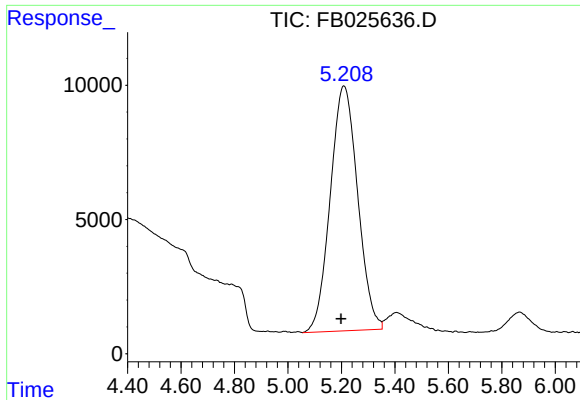

#1 2-Methylpentane


R.T.: 5.210 min
Delta R.T.: 0.012 min
Response: 649004
Conc: 26.83 ng/ml

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1MS

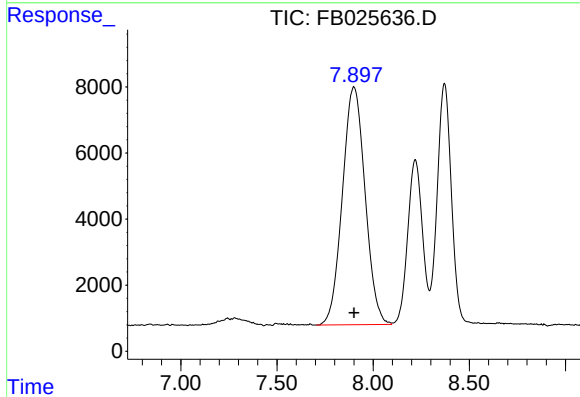


#2 2,2,4-Trimethylpentane

R.T.: 7.899 min
Delta R.T.: -0.003 min
Response: 586928
Conc: 31.56 ng/ml

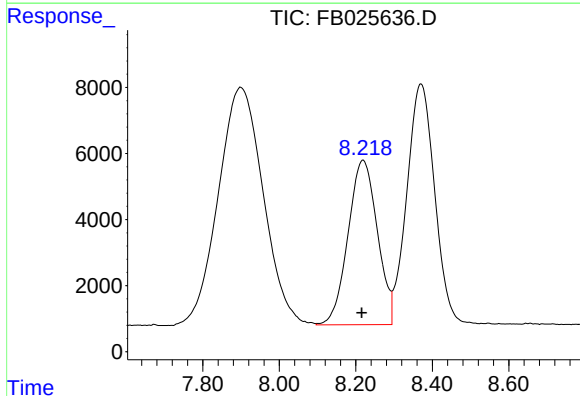


#3 n-Heptane

R.T.: 8.220 min
Delta R.T.: 0.004 min
Response: 264772
Conc: 9.04 ng/ml

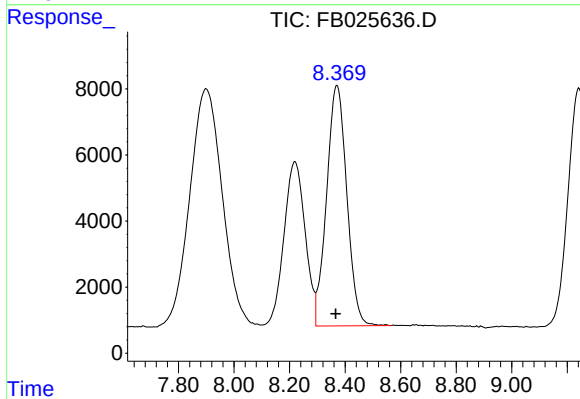

#4 Benzene


R.T.: 8.371 min
Delta R.T.: 0.004 min
Response: 368362
Conc: 9.53 ng/ml

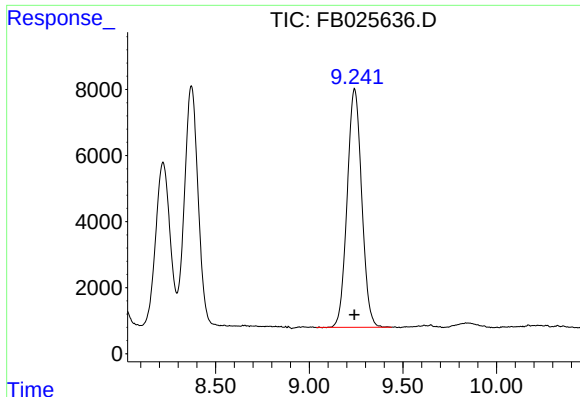

#5 AAA-TFT


R.T.: 9.242 min
Delta R.T.: 0.001 min
Response: 389650
Conc: 19.81 ng/ml

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1MS

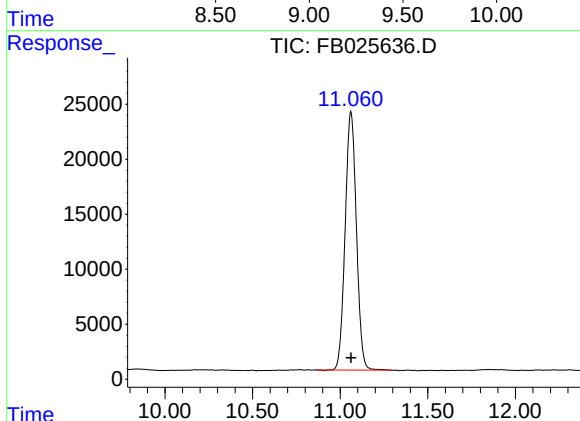


#6 Toluene

R.T.: 11.061 min
Delta R.T.: 0.000 min
Response: 1049562
Conc: 29.08 ng/ml

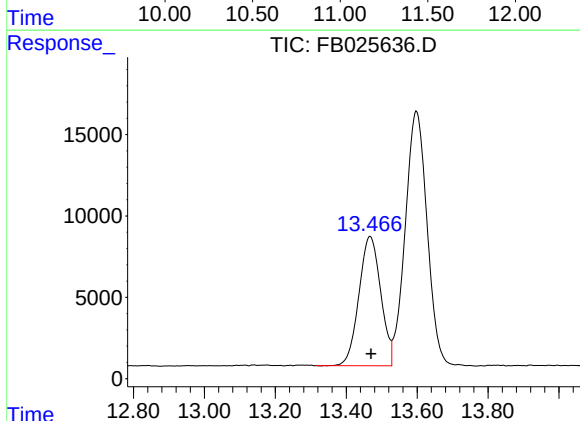


#7 Ethylbenzene

R.T.: 13.468 min
Delta R.T.: -0.003 min
Response: 339113
Conc: 9.89 ng/ml

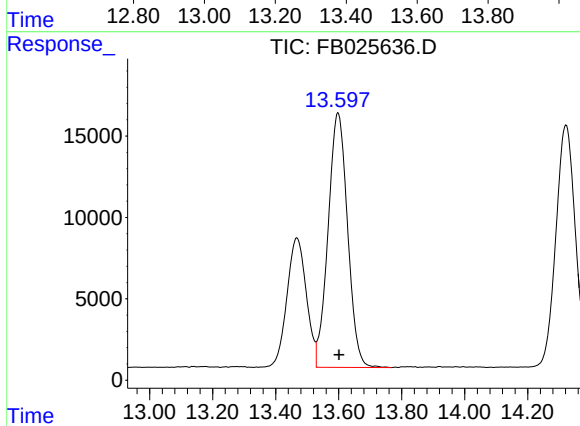

#8 m-Xylene


R.T.: 13.599 min
Delta R.T.: -0.002 min
Response: 672304
Conc: 19.78 ng/ml

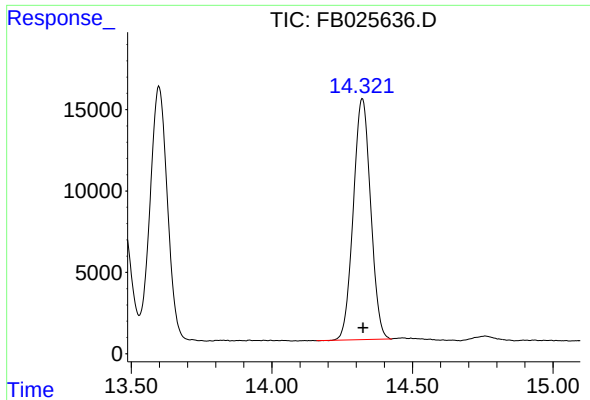

#9 O-Xylene

R.T.: 14.322 min
Delta R.T.: -0.003 min
Response: 633394
Conc: 19.44 ng/ml

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1MS

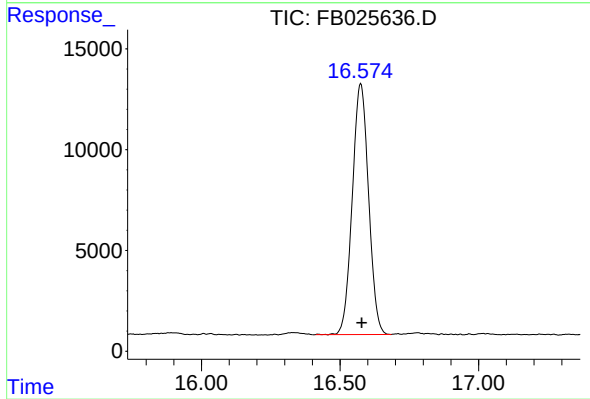

#10 1,2,4-Trimethylbenzene

R.T.: 16.575 min
Delta R.T.: -0.003 min
Response: 508043
Conc: 19.33 ng/ml