

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042321\
 Data File : FB025637.D
 Signal(s) : FID2B.CH
 Acq On : 23 Apr 2021 14:11
 Operator : DD/AJ
 Sample : M2090-03MSD
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SEDGWICK-COMP-1MSD

Integration File: Calibration.e
 Quant Time: Apr 23 14:44:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.234	387291	19.694 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.185	624951	25.833 ng/ml
2) t 2,2,4-Trimethylpentane	7.889	557911	29.998 ng/ml
3) t n-Heptane	8.207	261899	8.939 ng/ml
4) t Benzene	8.360	369285	9.558 ng/ml
6) t Toluene	11.056	1055414	29.241 ng/ml
7) t Ethylbenzene	13.465	339671	9.908 ng/ml
8) t m-Xylene	13.596	673617	19.817 ng/ml
9) t O-Xylene	14.319	635465	19.506 ng/ml
10) t 1,2,4-Trimethylbenzene	16.574	514685	19.579 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042321\
Data File : FB025637.D
Signal(s) : FID2B.CH
Acq On : 23 Apr 2021 14:11
Operator : DD/AJ
Sample : M2090-03MSD
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1MSD

Integration File: Calibration.e
Quant Time: Apr 23 14:44:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

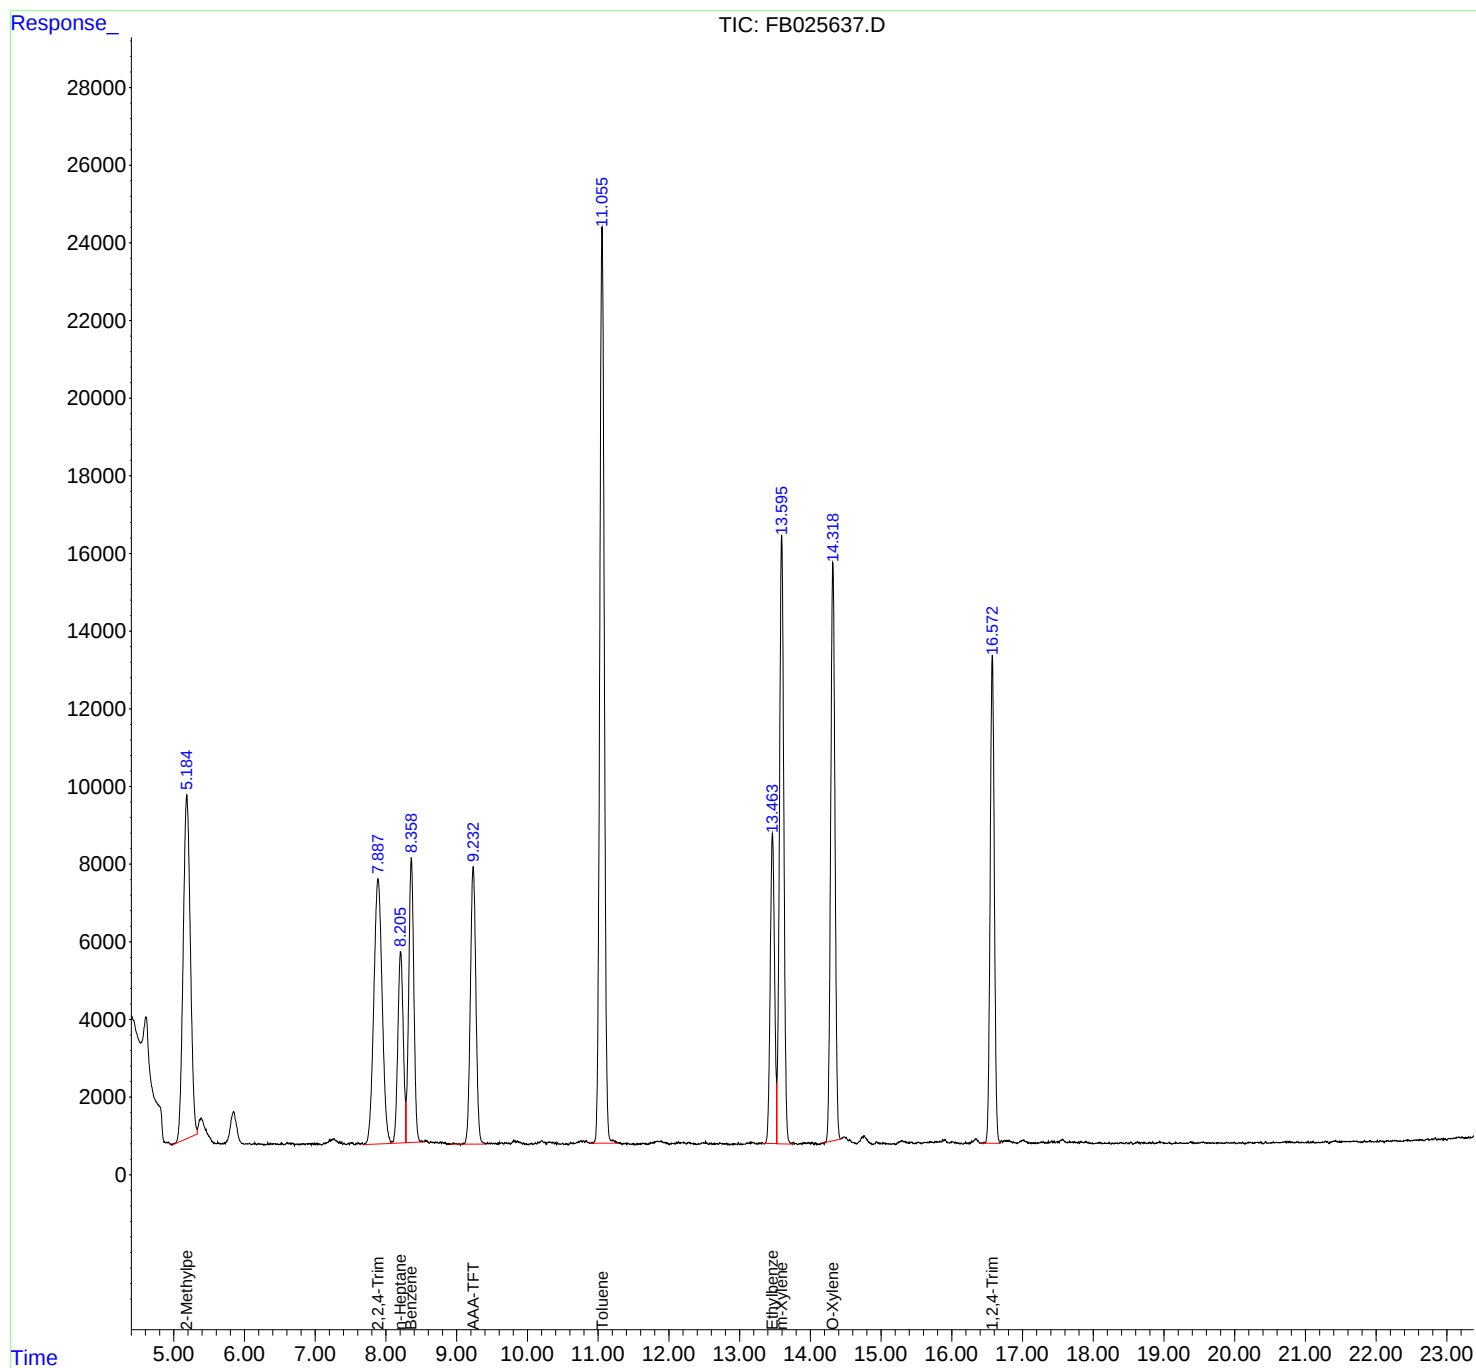


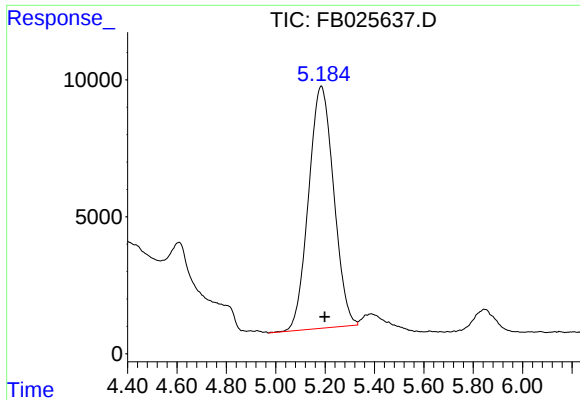

#1 2-Methylpentane


R.T.: 5.185 min
Delta R.T.: -0.013 min
Response: 624951
Conc: 25.83 ng/ml

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1MSD

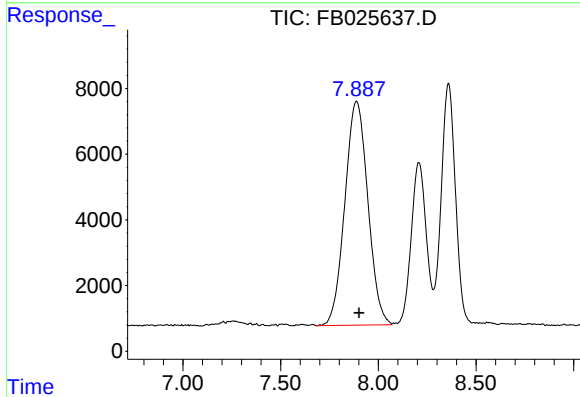


#2 2,2,4-Trimethylpentane

R.T.: 7.889 min
Delta R.T.: -0.013 min
Response: 557911
Conc: 30.00 ng/ml

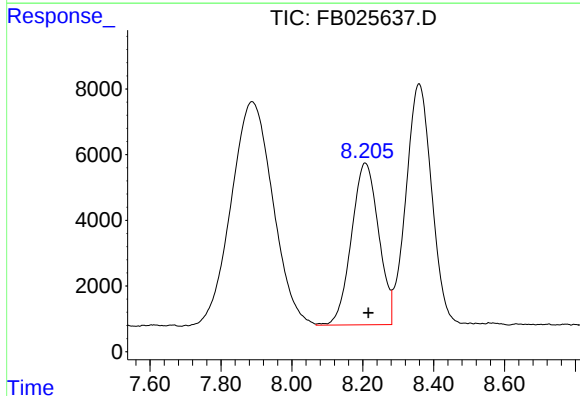


#3 n-Heptane

R.T.: 8.207 min
Delta R.T.: -0.009 min
Response: 261899
Conc: 8.94 ng/ml

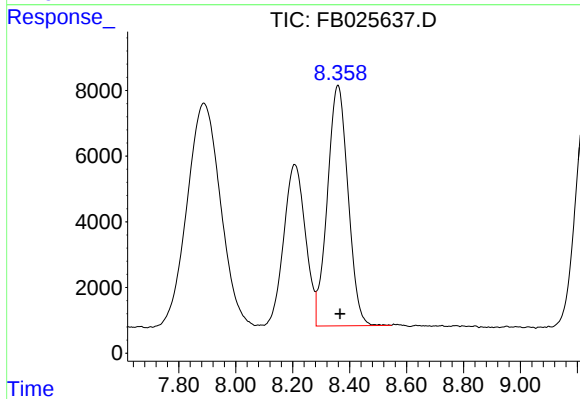

#4 Benzene


R.T.: 8.360 min
Delta R.T.: -0.007 min
Response: 369285
Conc: 9.56 ng/ml

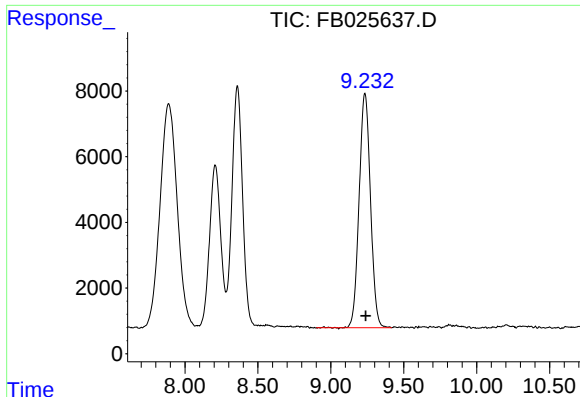

#5 AAA-TFT


R.T.: 9.234 min
Delta R.T.: -0.007 min
Response: 387291
Conc: 19.69 ng/ml

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1MSD

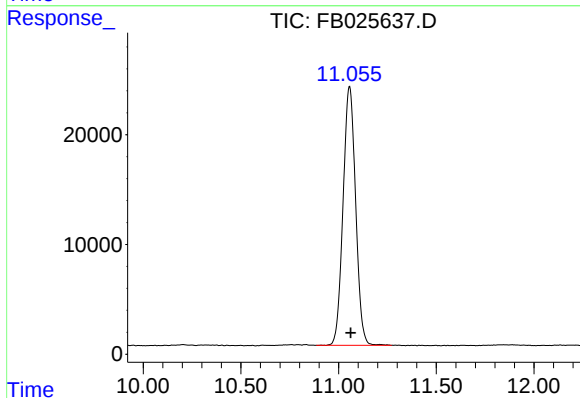


#6 Toluene

R.T.: 11.056 min
Delta R.T.: -0.006 min
Response: 1055414
Conc: 29.24 ng/ml

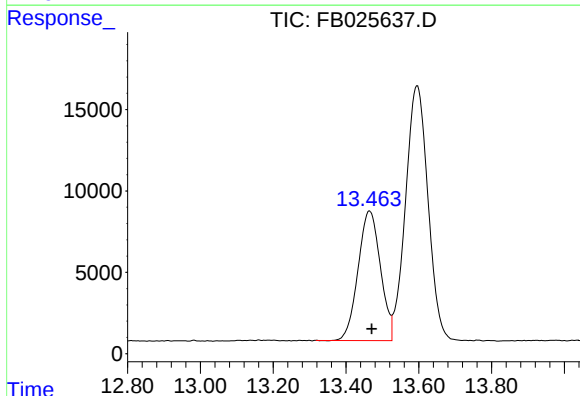


#7 Ethylbenzene

R.T.: 13.465 min
Delta R.T.: -0.005 min
Response: 339671
Conc: 9.91 ng/ml

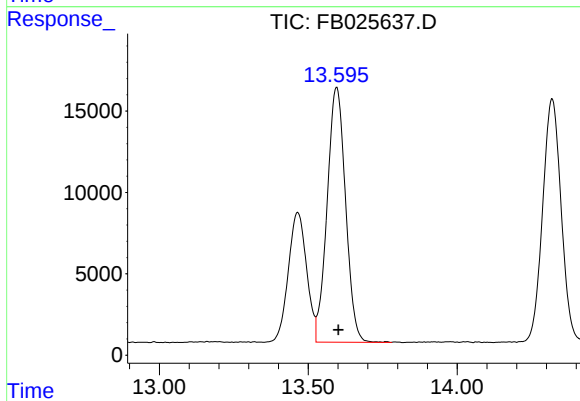

#8 m-Xylene


R.T.: 13.596 min
Delta R.T.: -0.005 min
Response: 673617
Conc: 19.82 ng/ml

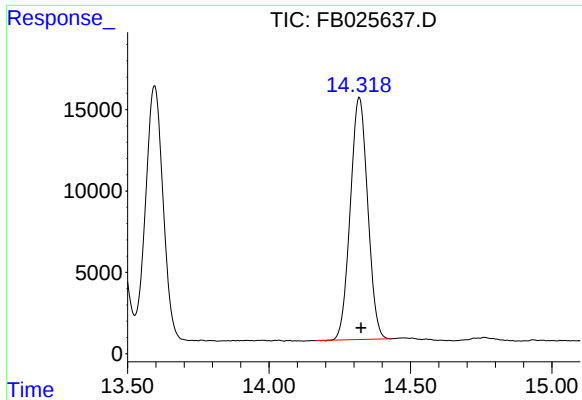

#9 O-Xylene

R.T.: 14.319 min
Delta R.T.: -0.006 min
Response: 635465
Conc: 19.51 ng/ml

Instrument :
FID_B
ClientSampleId :
SEDGWICK-COMP-1MSD

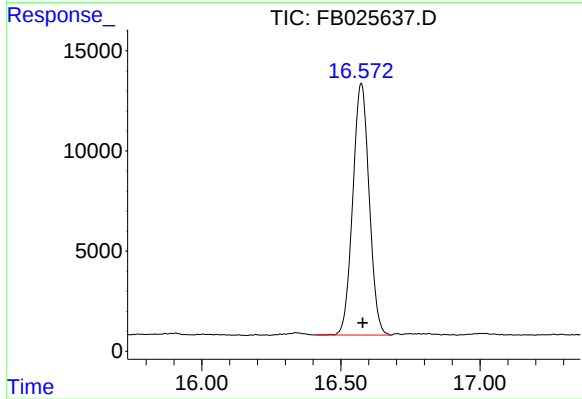

#10 1,2,4-Trimethylbenzene

R.T.: 16.574 min
Delta R.T.: -0.005 min
Response: 514685
Conc: 19.58 ng/ml