

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042321\
 Data File : FB025638.D
 Signal(s) : FID2B.CH
 Acq On : 23 Apr 2021 14:48
 Operator : DD/AJ
 Sample : BSF0423S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0423S1

Integration File: Calibration.e
 Quant Time: Apr 23 15:45:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.235	398973	20.288 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.192	689882	28.517 ng/ml
2) t 2,2,4-Trimethylpentane	7.892	638452	34.329 ng/ml
3) t n-Heptane	8.211	302711	10.332 ng/ml
4) t Benzene	8.362	372751	9.648 ng/ml
6) t Toluene	11.057	1083795	30.028 ng/ml
7) t Ethylbenzene	13.466	351402	10.250 ng/ml
8) t m-Xylene	13.597	700949	20.621 ng/ml
9) t O-Xylene	14.320	650084	19.954 ng/ml
10) t 1,2,4-Trimethylbenzene	16.574	542883	20.651 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042321\
Data File : FB025638.D
Signal(s) : FID2B.CH
Acq On : 23 Apr 2021 14:48
Operator : DD/AJ
Sample : BSF0423S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0423S1

Integration File: Calibration.e
Quant Time: Apr 23 15:45:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

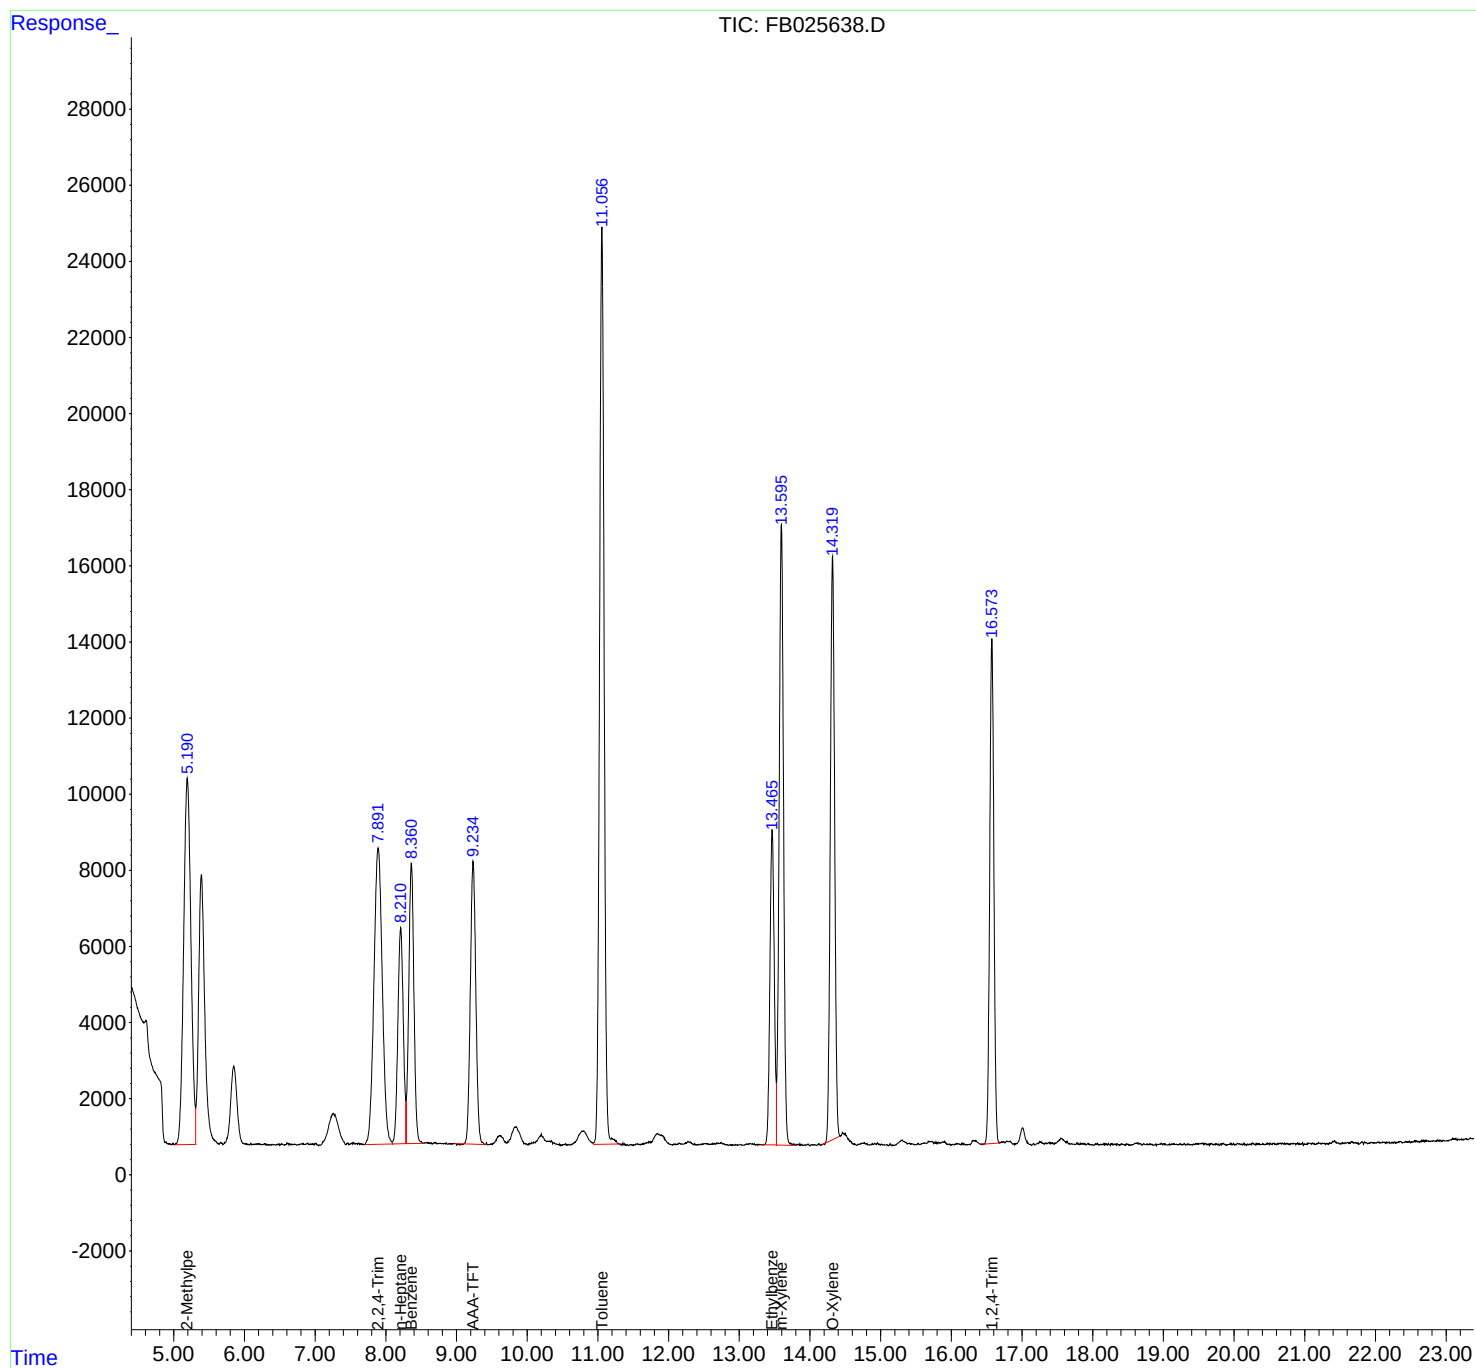


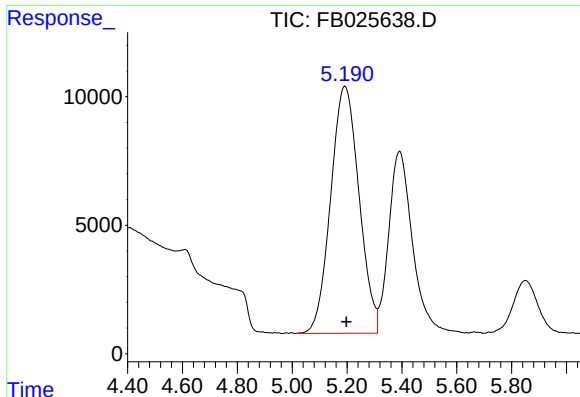

#1 2-Methylpentane


R.T.: 5.192 min
Delta R.T.: -0.006 min
Response: 689882
Conc: 28.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0423S1

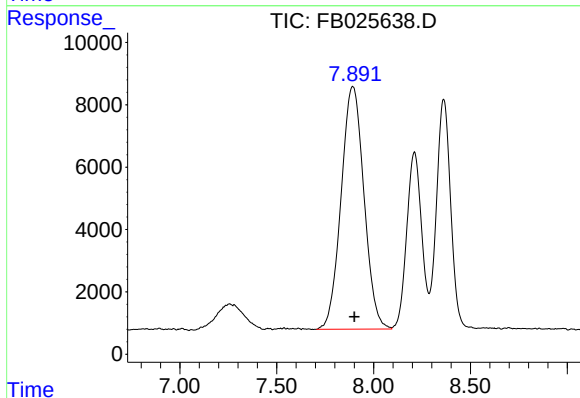


#2 2,2,4-Trimethylpentane

R.T.: 7.892 min
Delta R.T.: -0.009 min
Response: 638452
Conc: 34.33 ng/ml

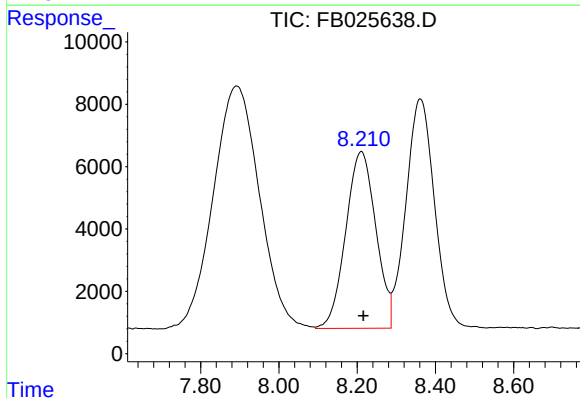


#3 n-Heptane

R.T.: 8.211 min
Delta R.T.: -0.005 min
Response: 302711
Conc: 10.33 ng/ml

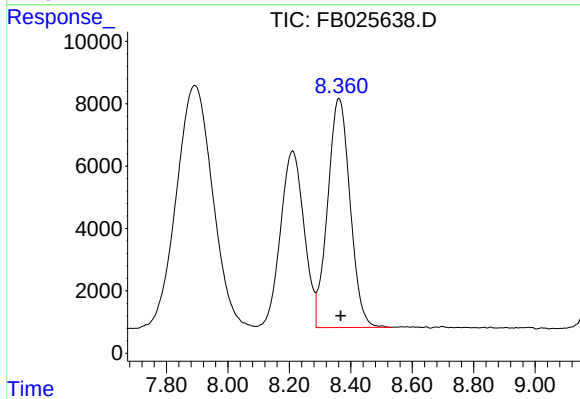

#4 Benzene


R.T.: 8.362 min
Delta R.T.: -0.005 min
Response: 372751
Conc: 9.65 ng/ml

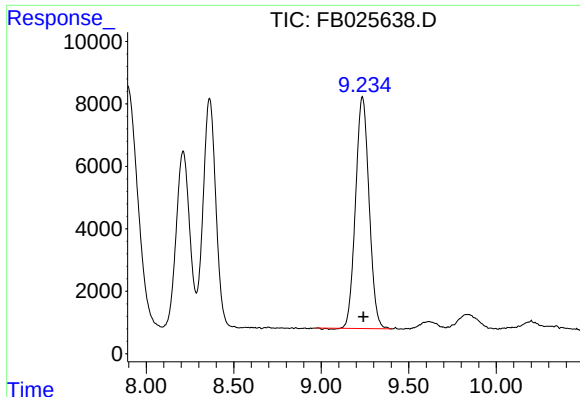

#5 AAA-TFT


R.T.: 9.235 min
Delta R.T.: -0.006 min
Response: 398973
Conc: 20.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0423S1

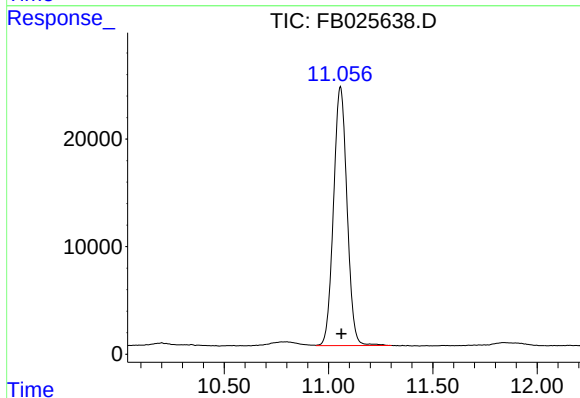


#6 Toluene

R.T.: 11.057 min
Delta R.T.: -0.005 min
Response: 1083795
Conc: 30.03 ng/ml

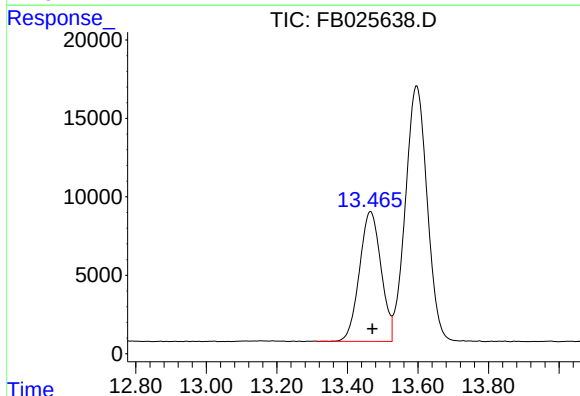


#7 Ethylbenzene

R.T.: 13.466 min
Delta R.T.: -0.005 min
Response: 351402
Conc: 10.25 ng/ml

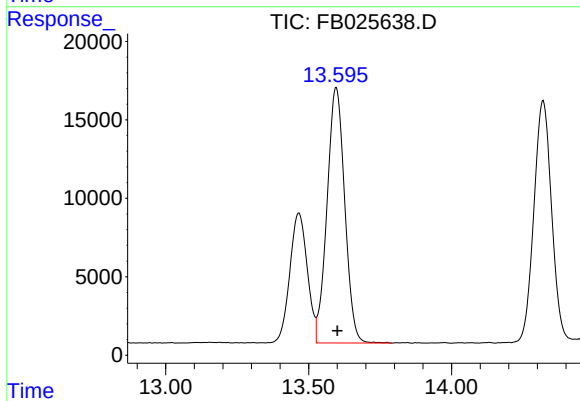

#8 m-Xylene


R.T.: 13.597 min
Delta R.T.: -0.004 min
Response: 700949
Conc: 20.62 ng/ml

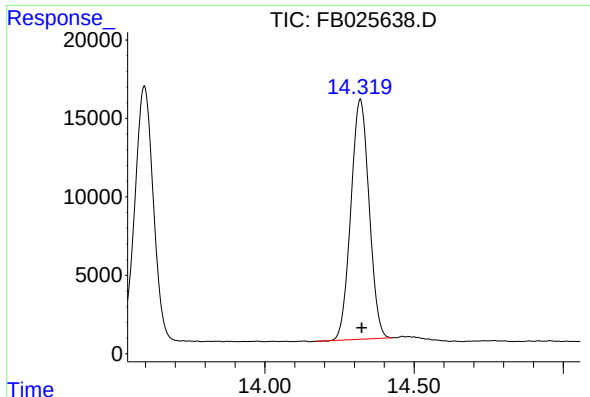

#9 O-Xylene

R.T.: 14.320 min
Delta R.T.: -0.005 min
Response: 650084
Conc: 19.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0423S1

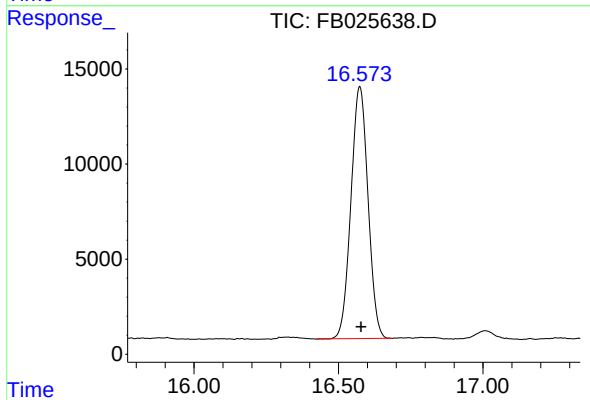

#10 1,2,4-Trimethylbenzene

R.T.: 16.574 min
Delta R.T.: -0.004 min
Response: 542883
Conc: 20.65 ng/ml