

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042419\
 Data File : FB020842.D
 Signal(s) : FID2B.CH
 Acq On : 24 Apr 2019 19:12
 Operator : MJ/SJ
 Sample : K2542-01MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 25 01:45:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.999	429574	23.290 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.868	1090369	30.973 ng/ml
2) t 2,2,4-Trimethylpentane	7.629	1003539	33.660 ng/ml
3) t n-Heptane	7.955	419553	10.688 ng/ml
4) t Benzene	8.091	449560	10.945 ng/ml
6) t Toluene	10.843	1010575	33.445 ng/ml
7) t Ethylbenzene	13.293	282782	11.054 ng/ml
8) t m-Xylene	13.427	584765	22.126 ng/ml
9) t O-Xylene	14.157	600751	22.191 ng/ml
10) t 1,2,4-Trimethylbenzene	16.442	587478	22.485 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042419\
Data File : FB020842.D
Signal(s) : FID2B.CH
Acq On : 24 Apr 2019 19:12
Operator : MJ/SJ
Sample : K2542-01MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 21 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 25 01:45:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

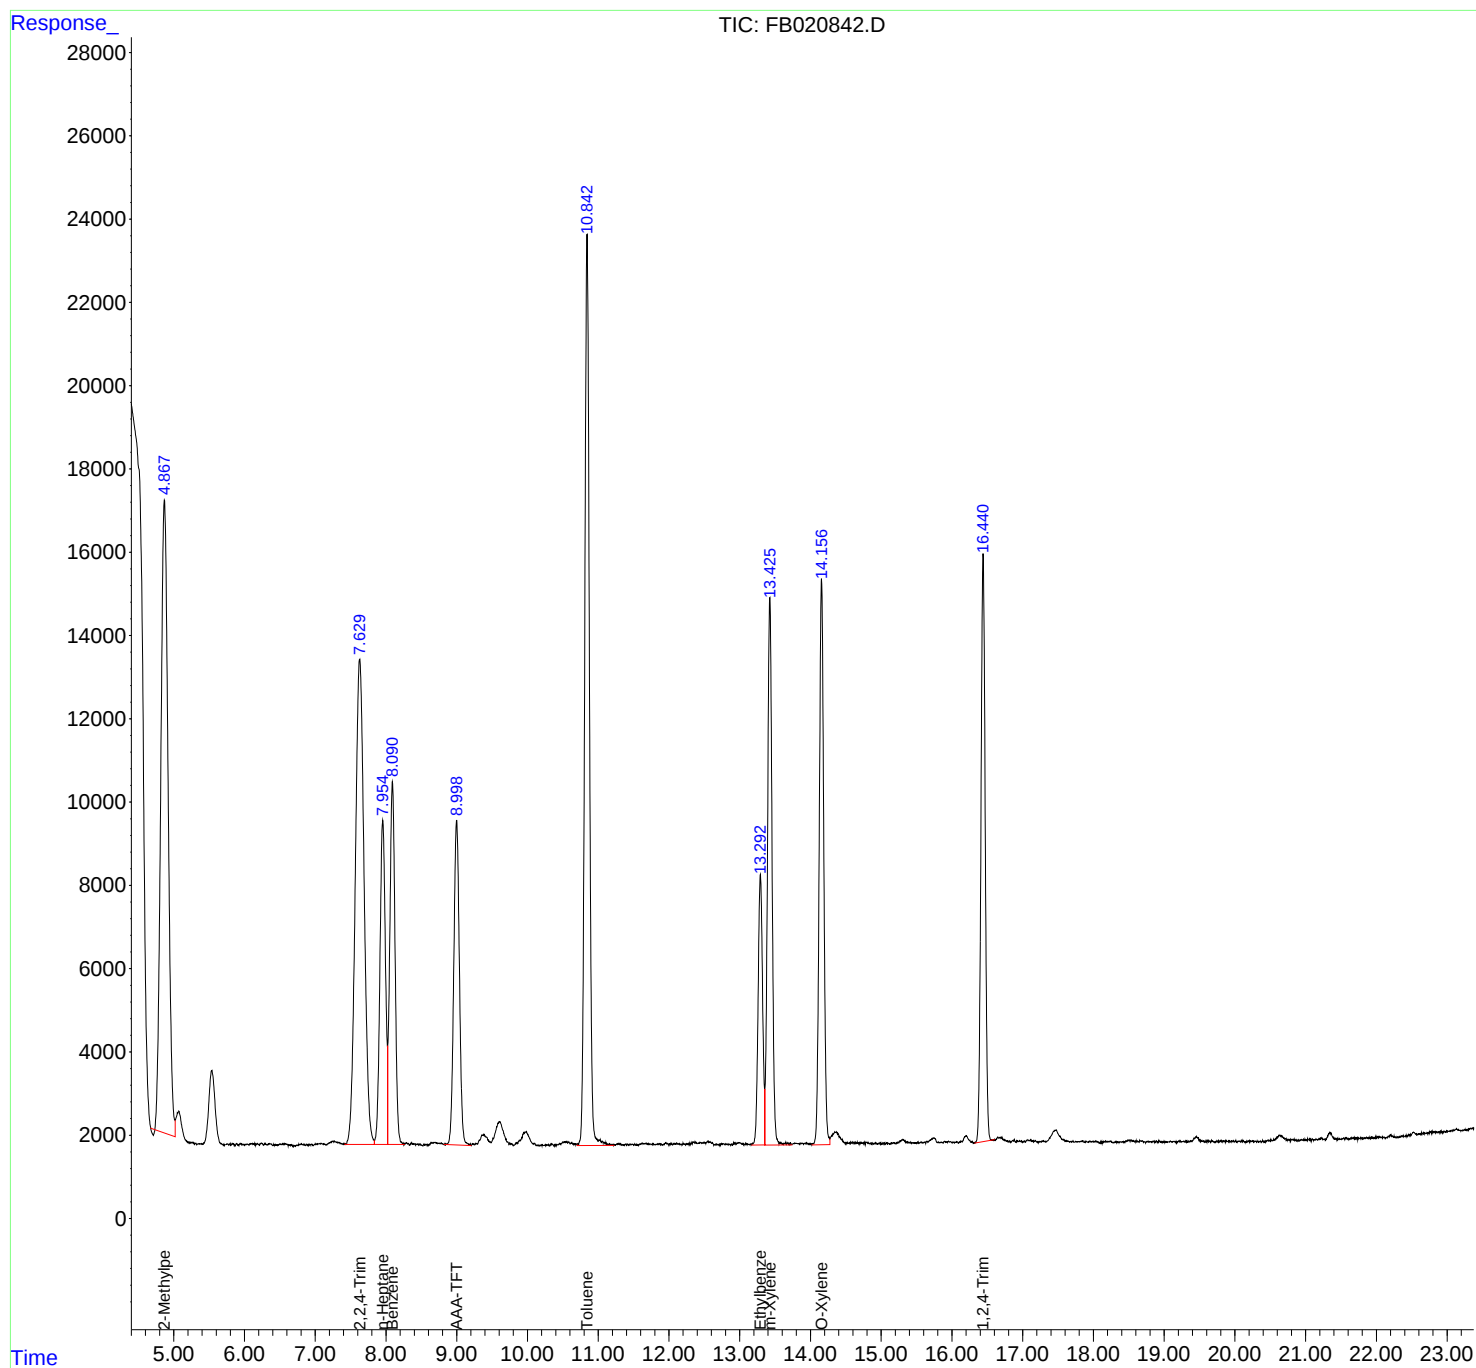

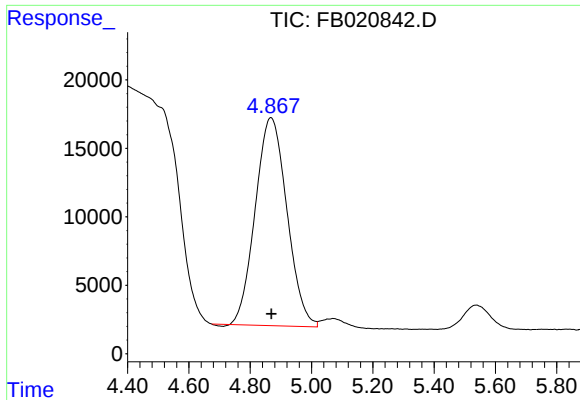


#1 2-Methylpentane

R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 1090369
Conc: 30.97 ng/ml

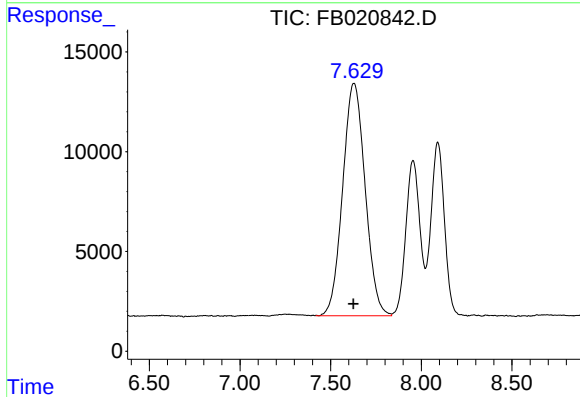


#2 2,2,4-Trimethylpentane

R.T.: 7.629 min
Delta R.T.: 0.002 min
Response: 1003539
Conc: 33.66 ng/ml

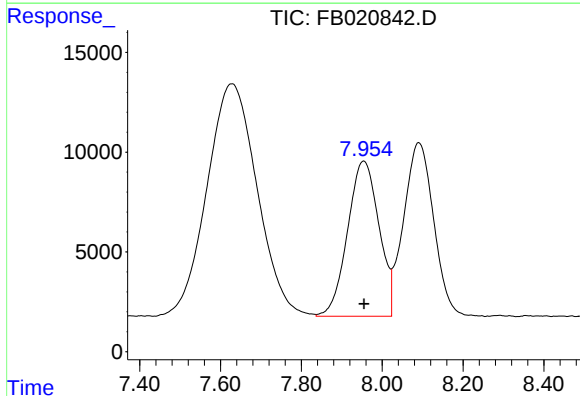


#3 n-Heptane

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 419553
Conc: 10.69 ng/ml

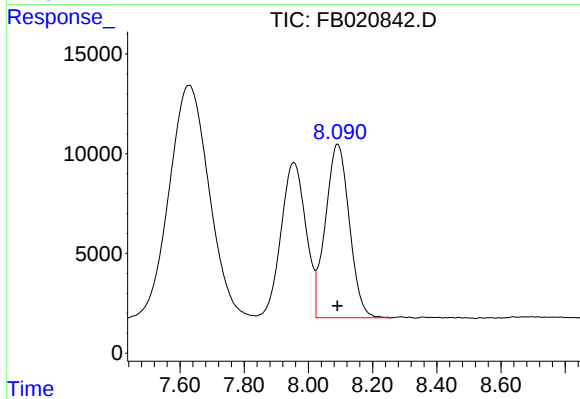


#4 Benzene

R.T.: 8.091 min
Delta R.T.: 0.000 min
Response: 449560
Conc: 10.94 ng/ml

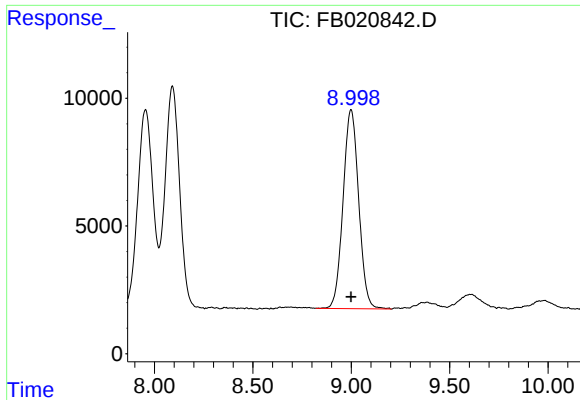


#5 AAA-TFT

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 429574
Conc: 23.29 ng/ml

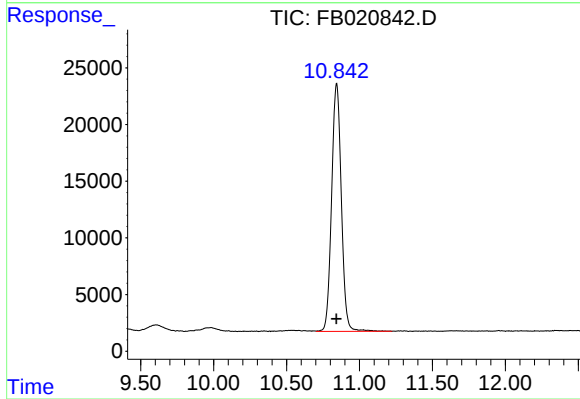


#6 Toluene

R.T.: 10.843 min
Delta R.T.: 0.000 min
Response: 1010575
Conc: 33.44 ng/ml

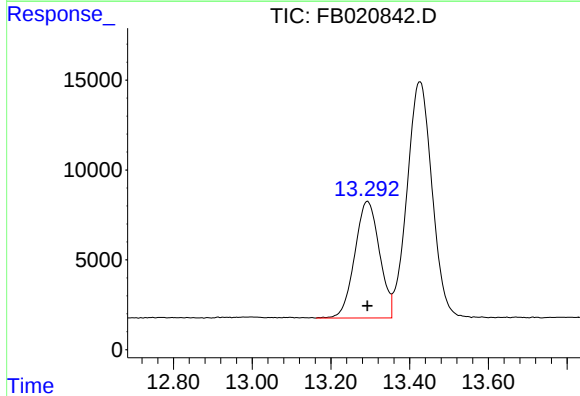


#7 Ethylbenzene

R.T.: 13.293 min
Delta R.T.: 0.000 min
Response: 282782
Conc: 11.05 ng/ml

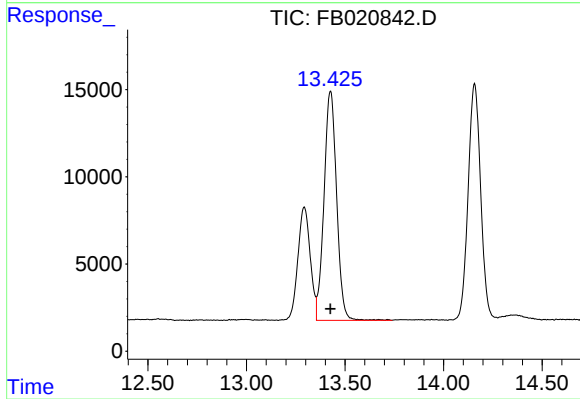

#8 m-Xylene

R.T.: 13.427 min
Delta R.T.: 0.000 min
Response: 584765
Conc: 22.13 ng/ml

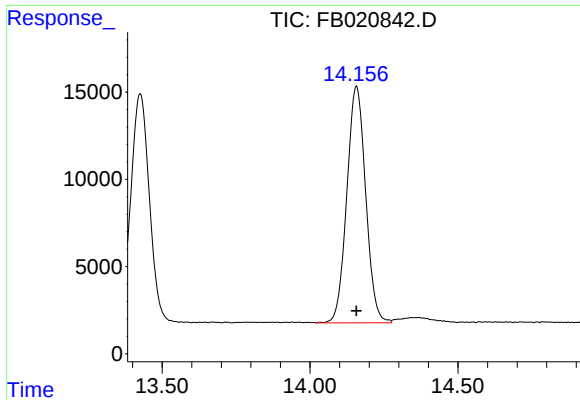


#9 O-Xylene

R.T.: 14.157 min

Delta R.T.: 0.000 min

Response: 600751

Conc: 22.19 ng/ml

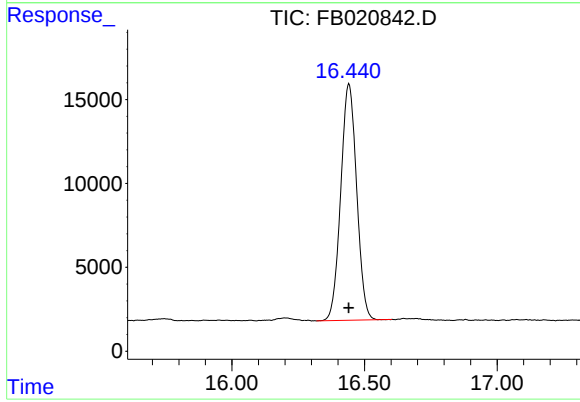

#10 1,2,4-Trimethylbenzene

R.T.: 16.442 min

Delta R.T.: 0.001 min

Response: 587478

Conc: 22.49 ng/ml