

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042419\
 Data File : FB020824.D
 Signal(s) : FID2B.CH
 Acq On : 24 Apr 2019 9:36
 Operator : MJ/SJ
 Sample : BSF0424S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 25 01:41:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.000	461652	25.029 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.869	1145434	32.537 ng/ml
2) t	2,2,4-Trimethylpentane	7.629	1056600	35.440 ng/ml
3) t	n-Heptane	7.956	432841	11.026 ng/ml
4) t	Benzene	8.092	458413	11.160 ng/ml
6) t	Toluene	10.843	1016685	33.647 ng/ml
7) t	Ethylbenzene	13.294	276889	10.824 ng/ml
8) t	m-Xylene	13.426	574431	21.735 ng/ml
9) t	O-Xylene	14.158	588679	21.745 ng/ml
10) t	1,2,4-Trimethylbenzene	16.442	583596	22.337 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042419\
Data File : FB020824.D
Signal(s) : FID2B.CH
Acq On : 24 Apr 2019 9:36
Operator : MJ/SJ
Sample : BSF0424S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 25 01:41:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

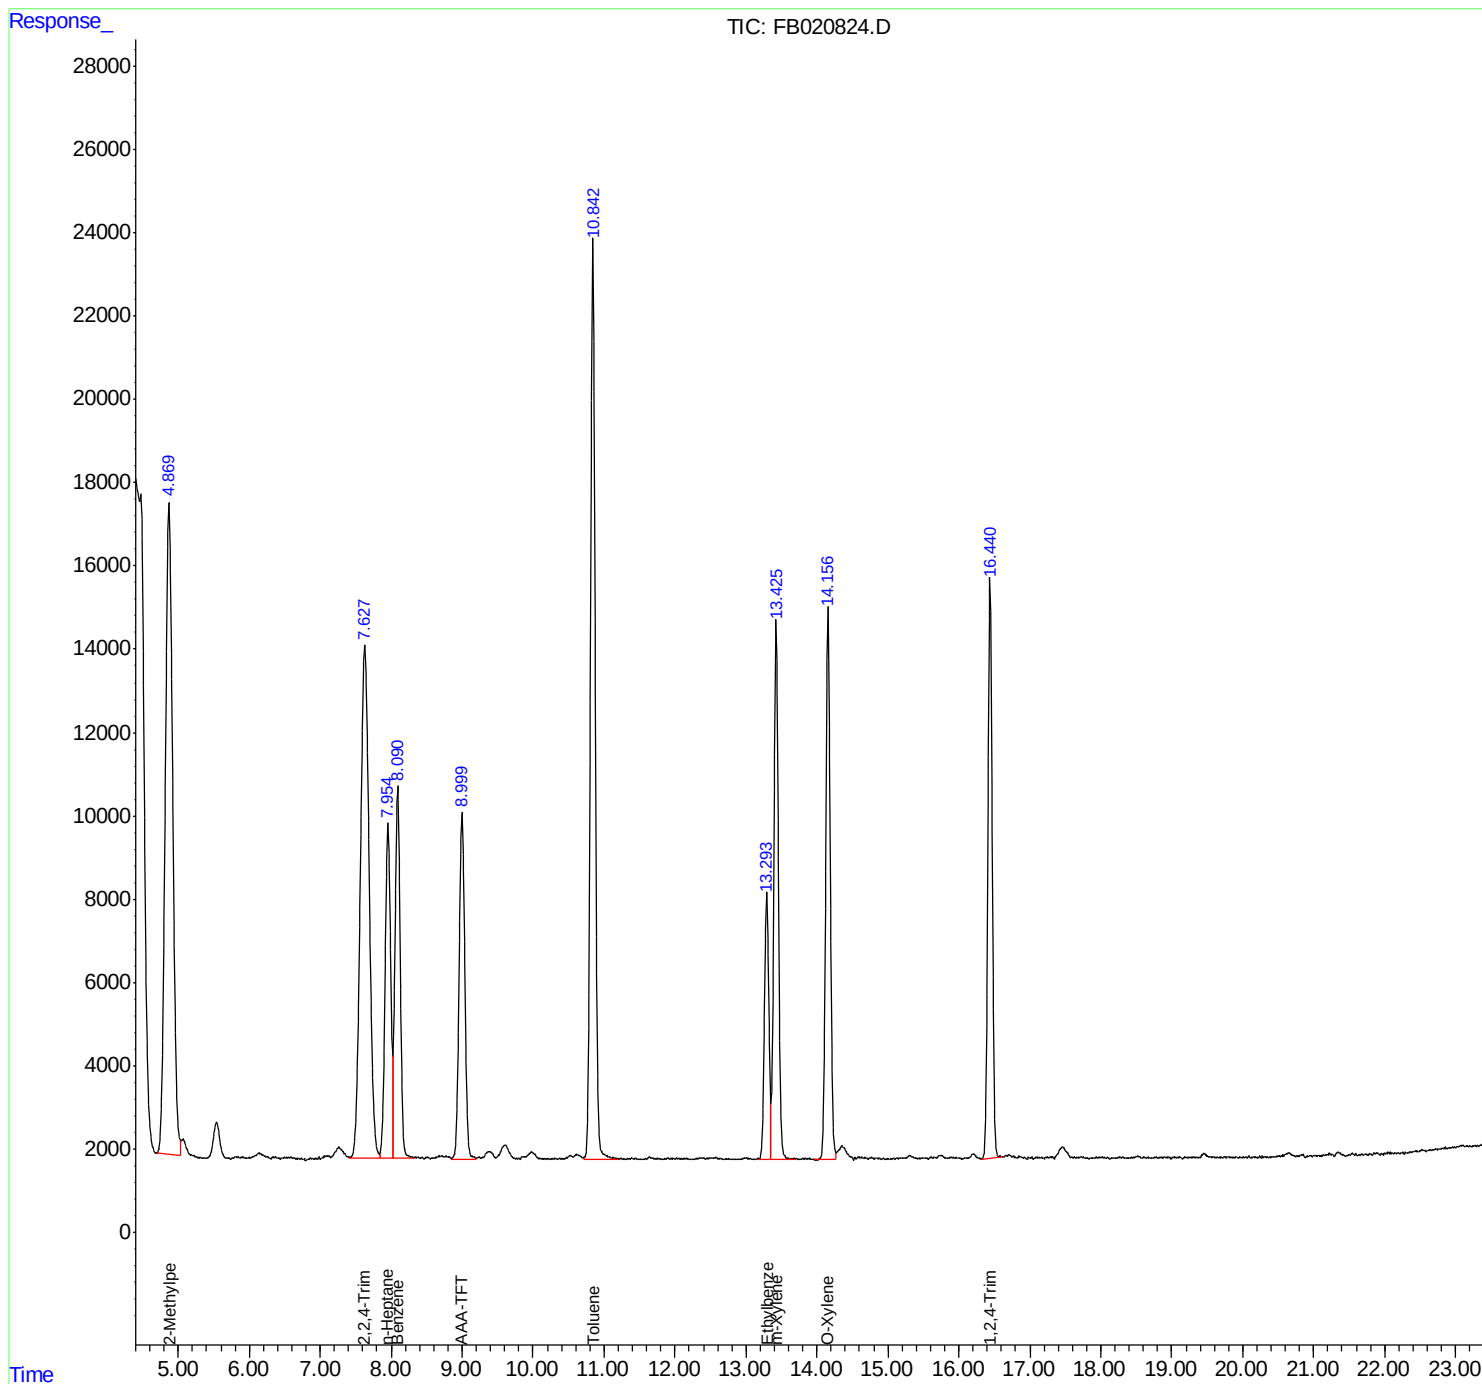

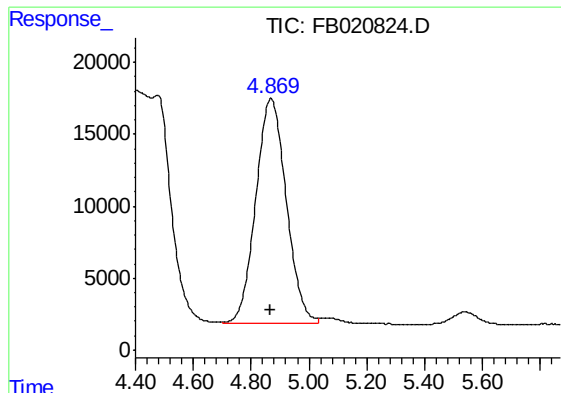


#1 2-Methylpentane

R.T.: 4.869 min
Delta R.T.: 0.000 min
Response: 1145434
Conc: 32.54 ng/ml

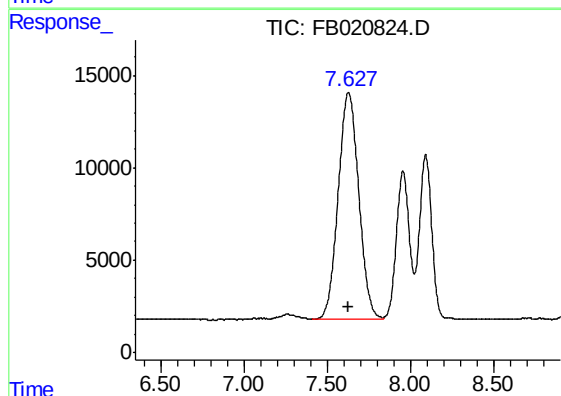


#2 2,2,4-Trimethylpentane

R.T.: 7.629 min
Delta R.T.: 0.002 min
Response: 1056600
Conc: 35.44 ng/ml

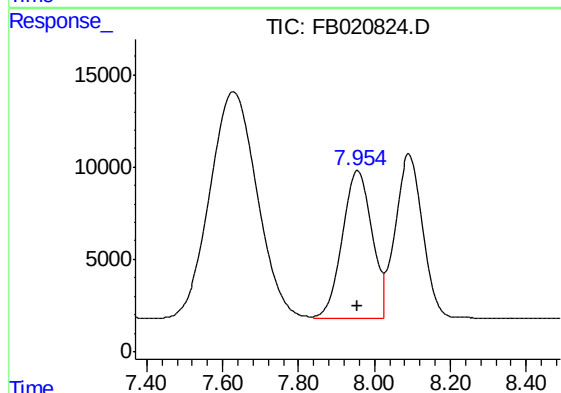


#3 n-Heptane

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 432841
Conc: 11.03 ng/ml

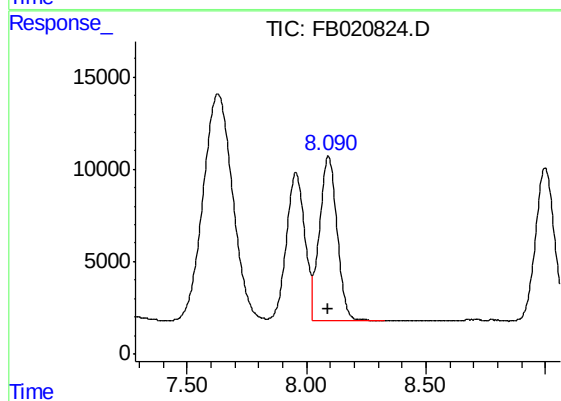


#4 Benzene

R.T.: 8.092 min
Delta R.T.: 0.000 min
Response: 458413
Conc: 11.16 ng/ml

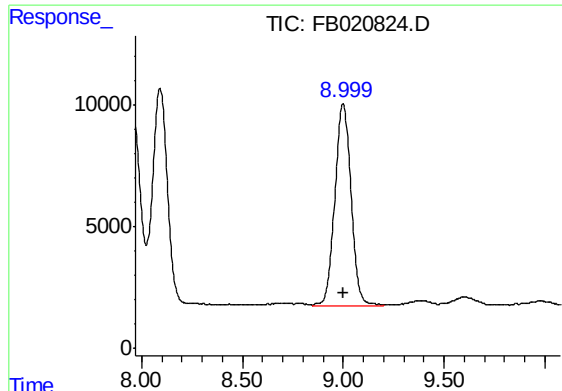


#5 AAA-TFT

R.T.: 9.000 min
Delta R.T.: 0.000 min
Response: 461652
Conc: 25.03 ng/ml

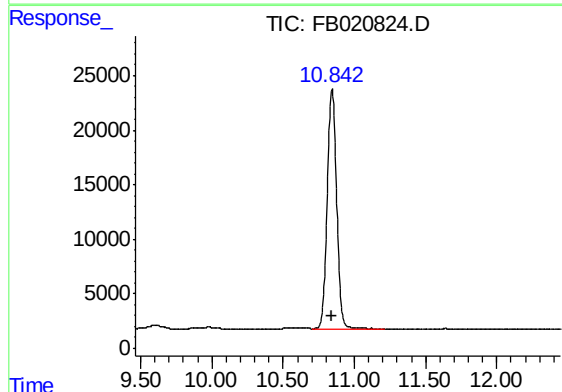


#6 Toluene

R.T.: 10.843 min
Delta R.T.: 0.001 min
Response: 1016685
Conc: 33.65 ng/ml

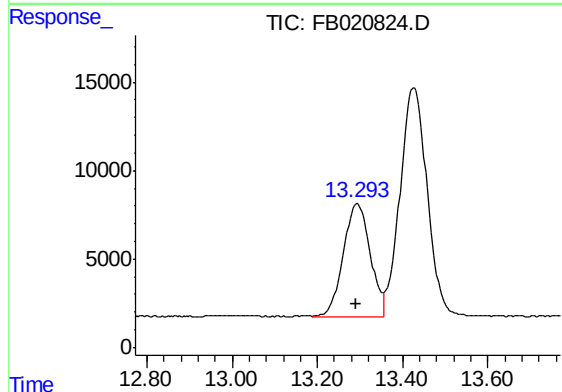


#7 Ethylbenzene

R.T.: 13.294 min
Delta R.T.: 0.001 min
Response: 276889
Conc: 10.82 ng/ml

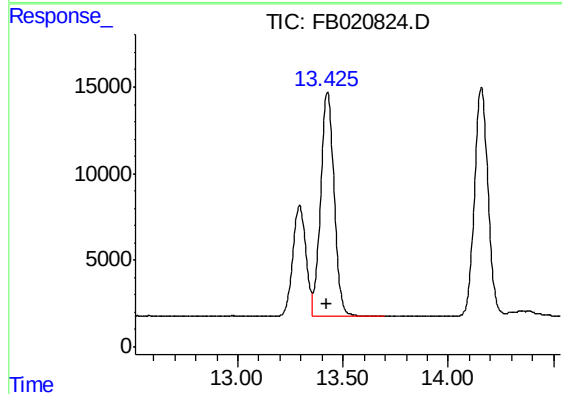


#8 m-Xylene

R.T.: 13.426 min
Delta R.T.: 0.000 min
Response: 574431
Conc: 21.73 ng/ml

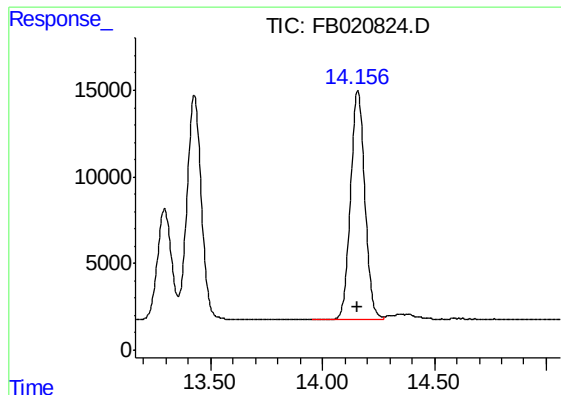

#9 O-Xylene

R.T.: 14.158 min
Delta R.T.: 0.001 min
Response: 588679
Conc: 21.74 ng/ml

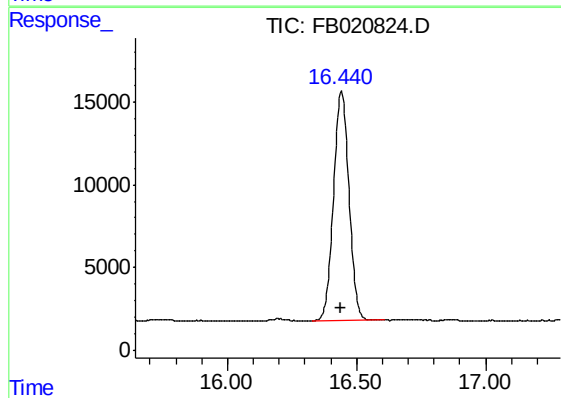

#10 1,2,4-Trimethylbenzene

R.T.: 16.442 min
Delta R.T.: 0.002 min
Response: 583596
Conc: 22.34 ng/ml