

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042420\
 Data File : FB042425.D
 Signal(s) : FID2B.CH
 Acq On : 24 Apr 2020 11:30
 Operator : DD/AJ
 Sample : BSF0424S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 25 02:18:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	487126	19.443 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	920078	28.187 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1013225	29.690 ng/ml
3) t n-Heptane	7.759	322817	9.565 ng/ml
4) t Benzene	7.893	395257	9.793 ng/ml
6) t Toluene	10.631	1132732	28.814 ng/ml
7) t Ethylbenzene	13.071	363479	9.970 ng/ml
8) t m-Xylene	13.205	709640	20.272 ng/ml
9) t O-Xylene	13.933	689352	20.226 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	578133	20.361 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042420\
Data File : FB042425.D
Signal(s) : FID2B.CH
Acq On : 24 Apr 2020 11:30
Operator : DD/AJ
Sample : BSF0424S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 25 02:18:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

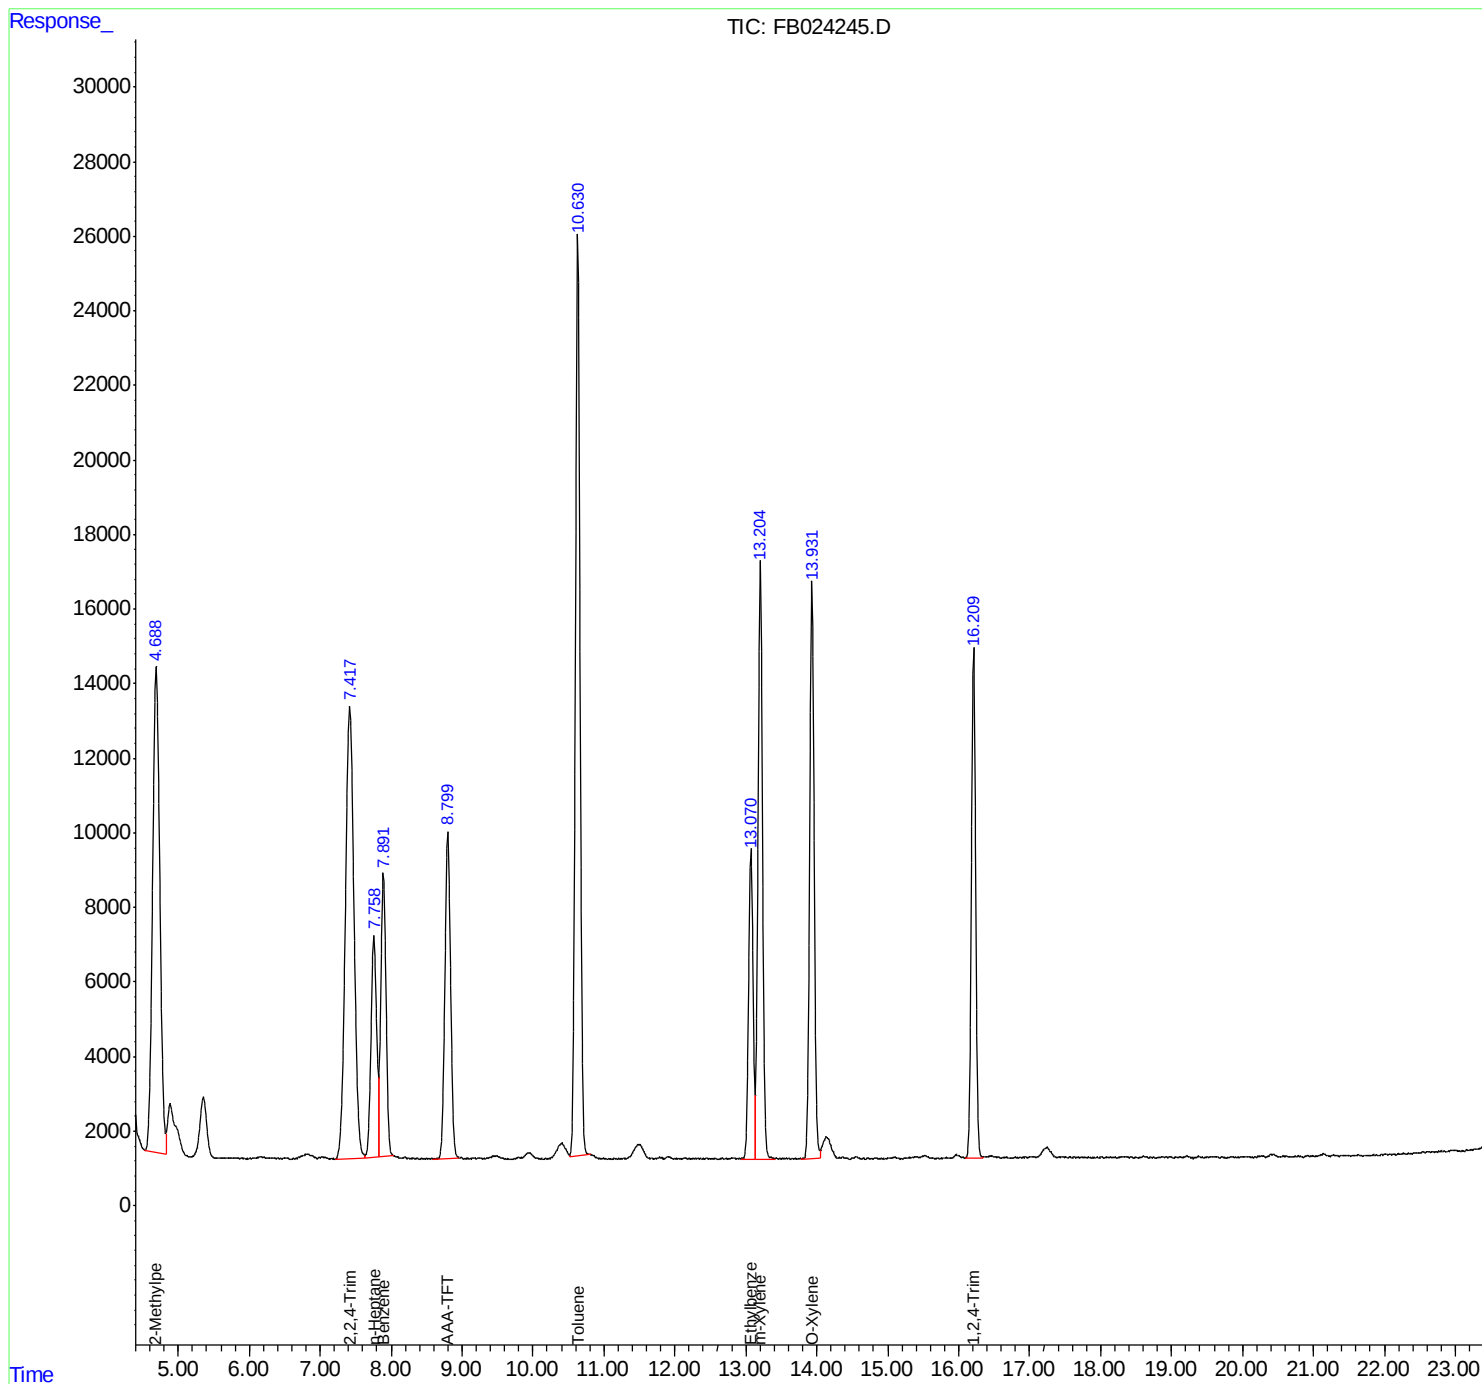

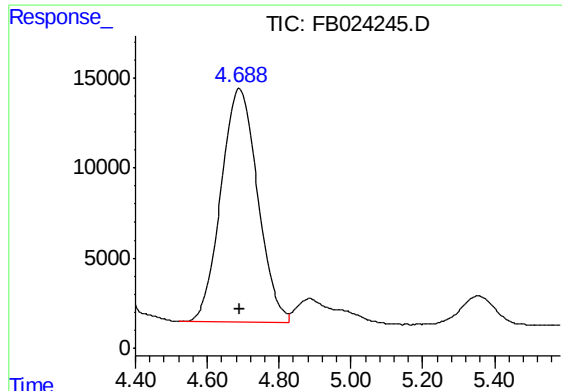


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 920078
Conc: 28.19 ng/ml

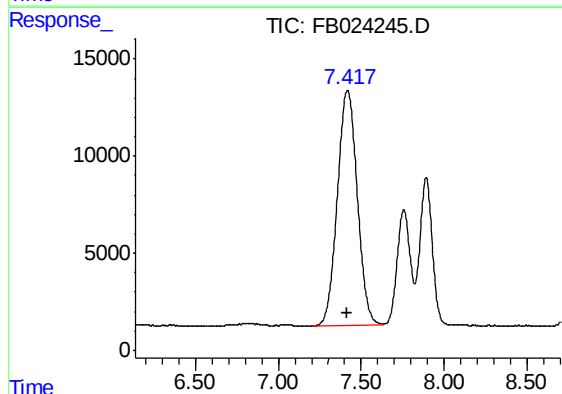


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.001 min
Response: 1013225
Conc: 29.69 ng/ml

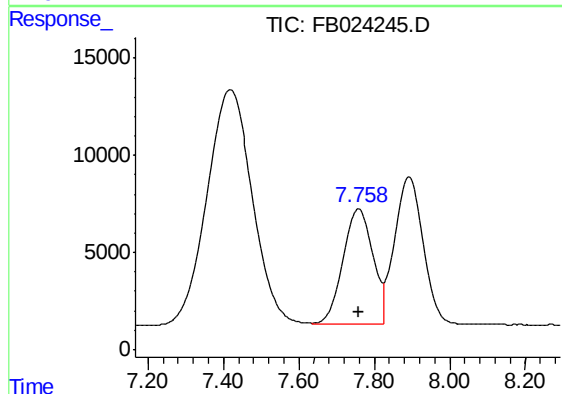


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 322817
Conc: 9.56 ng/ml

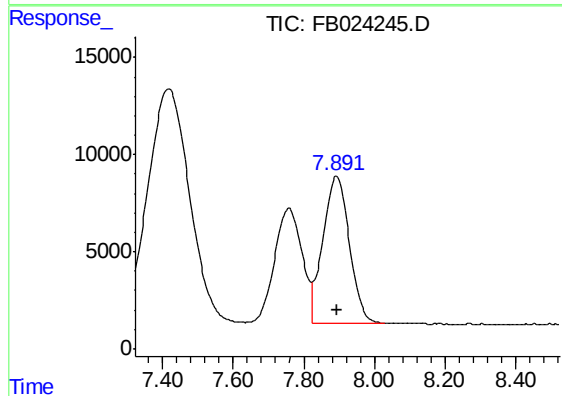


#4 Benzene

R.T.: 7.893 min
Delta R.T.: -0.001 min
Response: 395257
Conc: 9.79 ng/ml

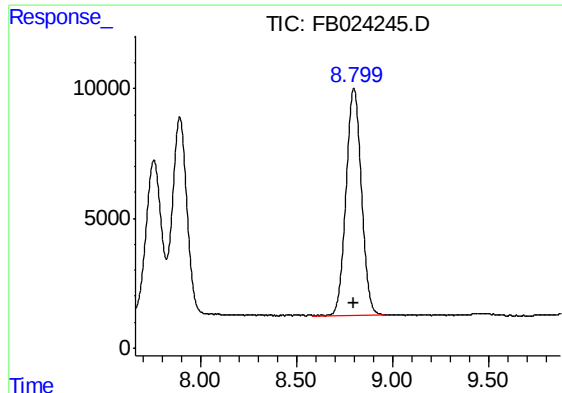


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: -0.001 min
Response: 487126
Conc: 19.44 ng/ml

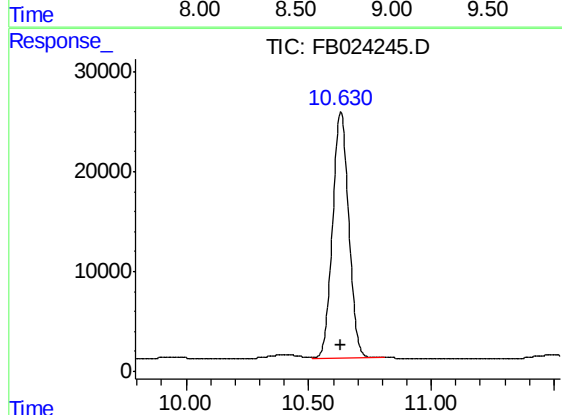


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1132732
Conc: 28.81 ng/ml

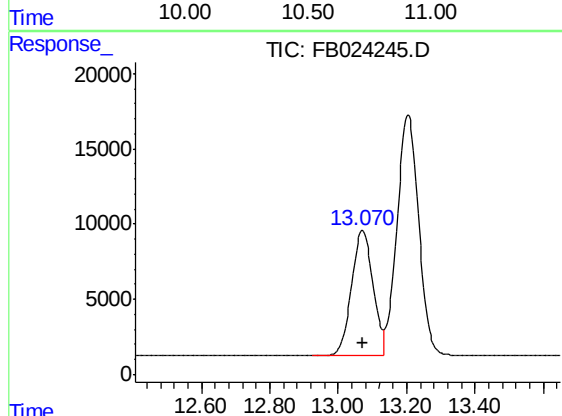


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 363479
Conc: 9.97 ng/ml

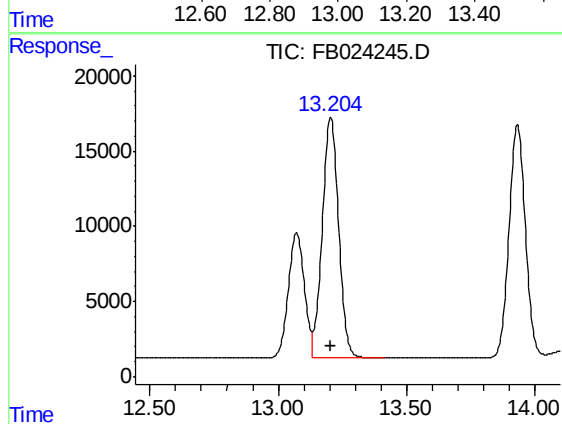


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 709640
Conc: 20.27 ng/ml

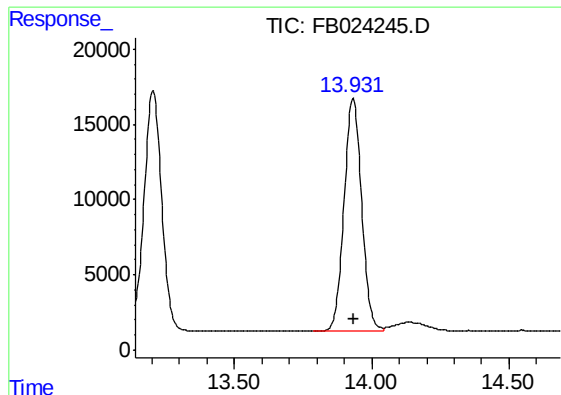

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 689352
Conc: 20.23 ng/ml

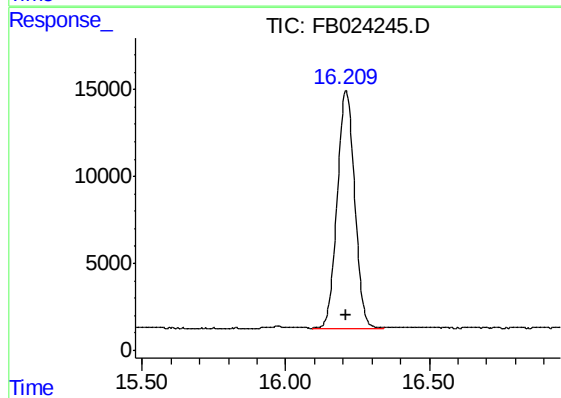

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 578133
Conc: 20.36 ng/ml