

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042420\
 Data File : FB0424251.D
 Signal(s) : FID2B.CH
 Acq On : 24 Apr 2020 14:34
 Operator : DD/AJ
 Sample : L2331-07MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 25 02:19:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	448893	17.917 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.693	793630	24.313 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	839263	24.592 ng/ml
3) t n-Heptane	7.762	269797	7.994 ng/ml
4) t Benzene	7.896	364323	9.027 ng/ml
6) t Toluene	10.634	1039303	26.438 ng/ml
7) t Ethylbenzene	13.073	323350	8.870 ng/ml
8) t m-Xylene	13.206	627033	17.912 ng/ml
9) t O-Xylene	13.934	615475	18.058 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	502194	17.687 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042420\
Data File : FB0424251.D
Signal(s) : FID2B.CH
Acq On : 24 Apr 2020 14:34
Operator : DD/AJ
Sample : L2331-07MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 25 02:19:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

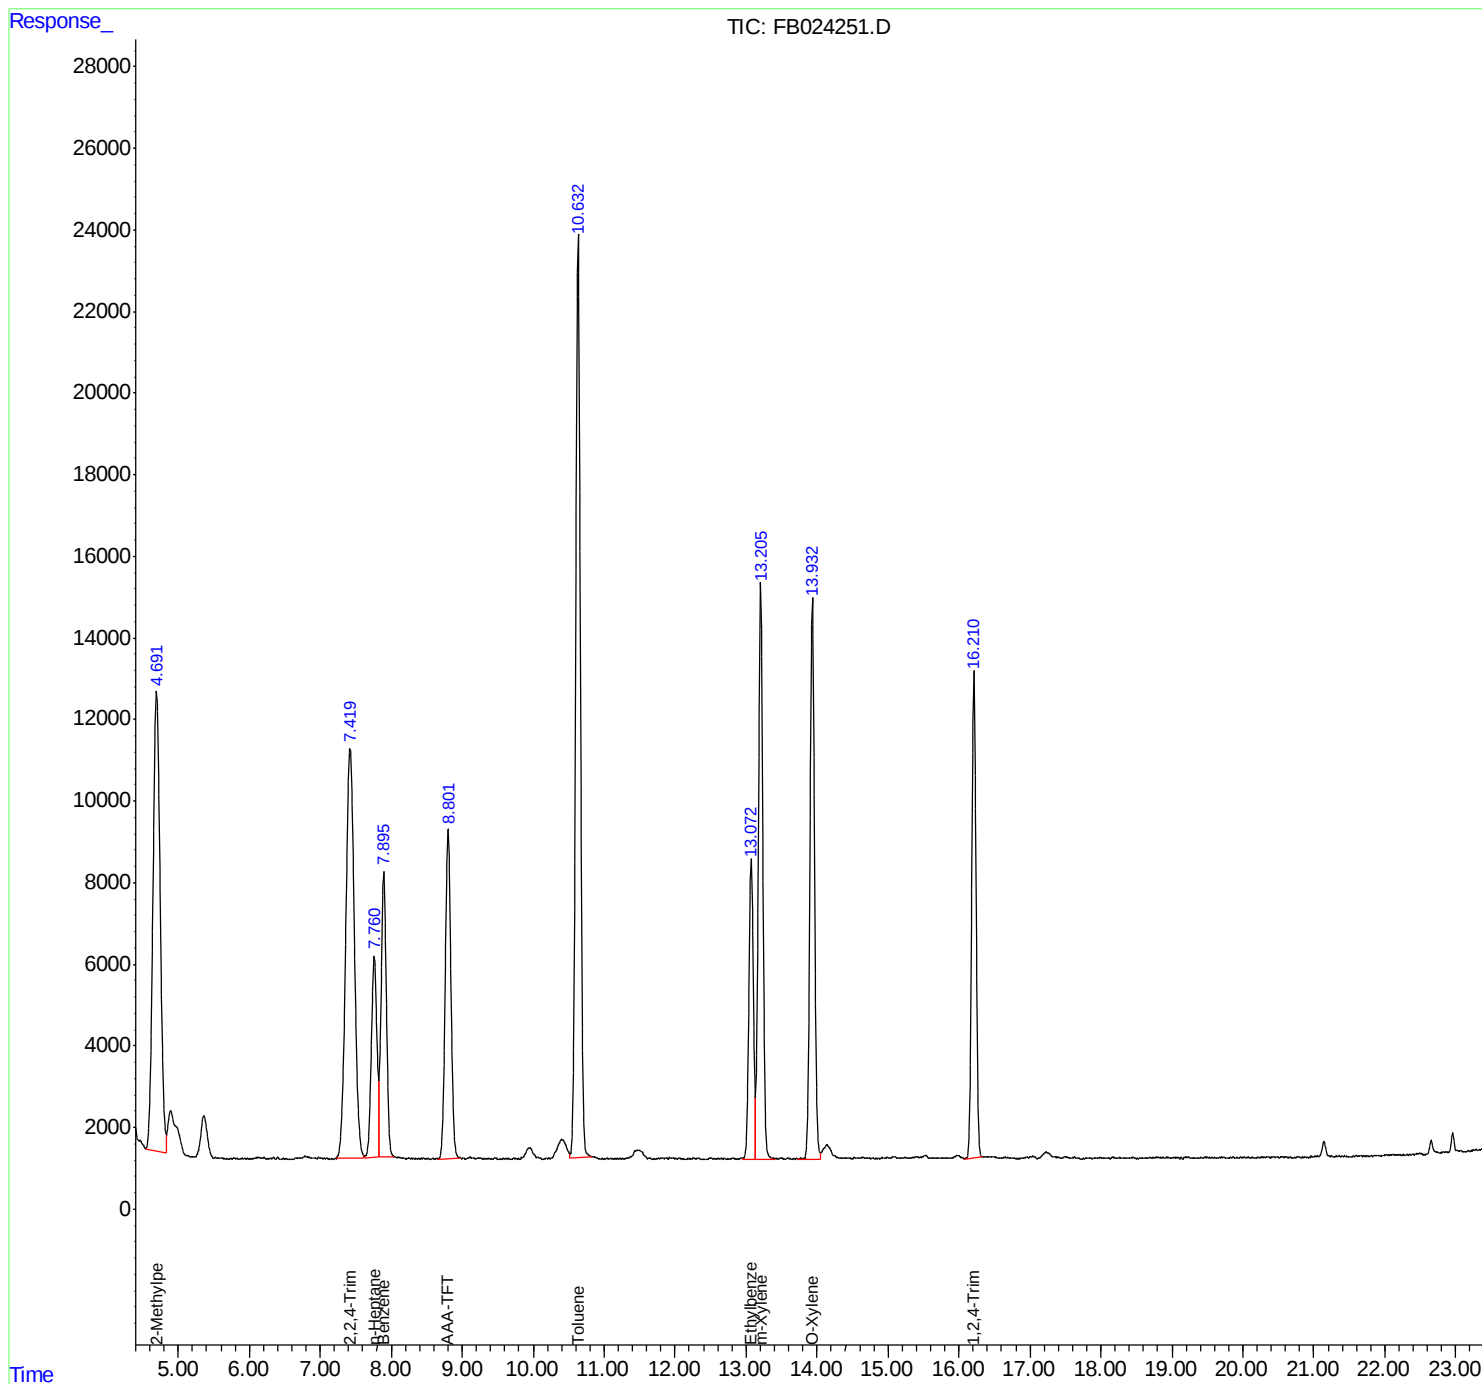

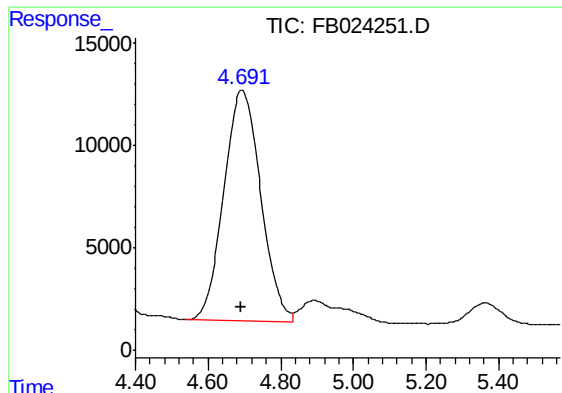


#1 2-Methylpentane

R.T.: 4.693 min
Delta R.T.: 0.002 min
Response: 793630
Conc: 24.31 ng/ml

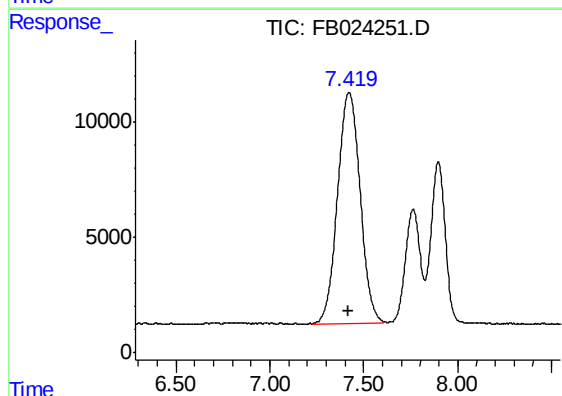


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.002 min
Response: 839263
Conc: 24.59 ng/ml

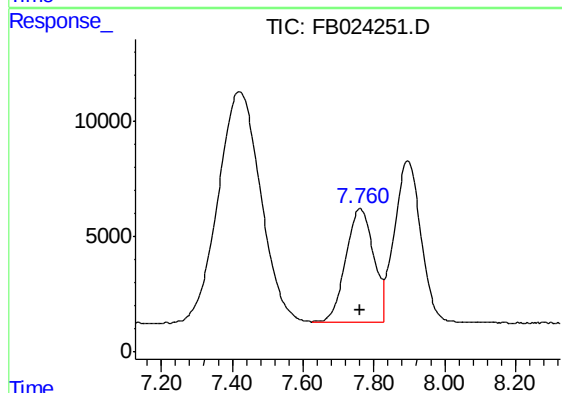


#3 n-Heptane

R.T.: 7.762 min
Delta R.T.: 0.002 min
Response: 269797
Conc: 7.99 ng/ml

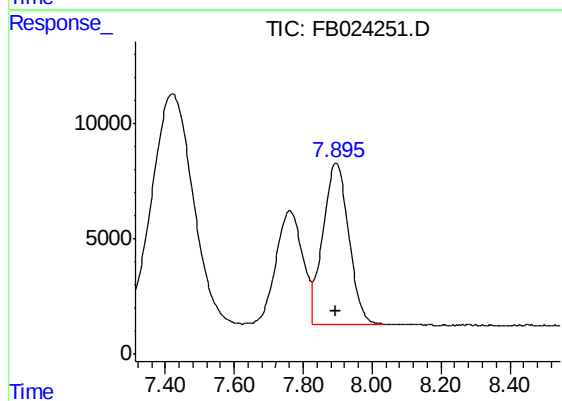


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.002 min
Response: 364323
Conc: 9.03 ng/ml

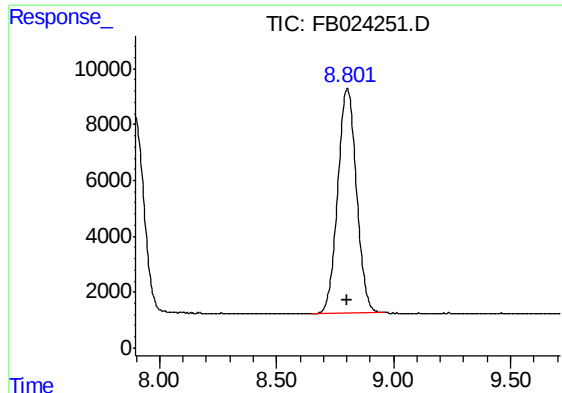


#5 AAA-TFT

R.T.: 8.803 min
Delta R.T.: 0.002 min
Response: 448893
Conc: 17.92 ng/ml

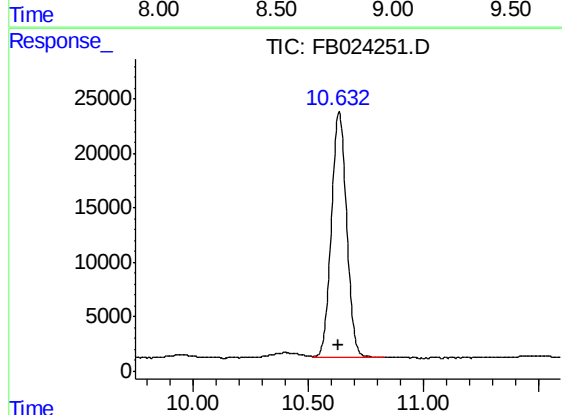


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.002 min
Response: 1039303
Conc: 26.44 ng/ml

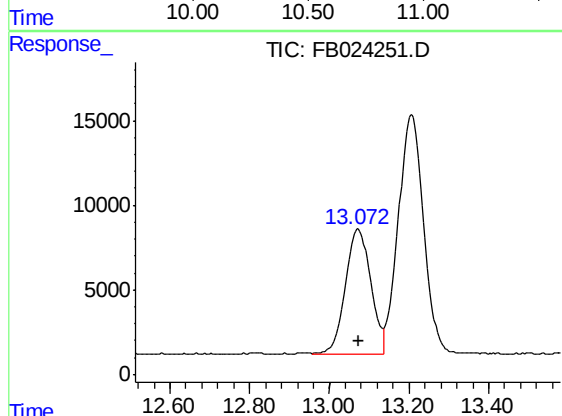


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.000 min
Response: 323350
Conc: 8.87 ng/ml

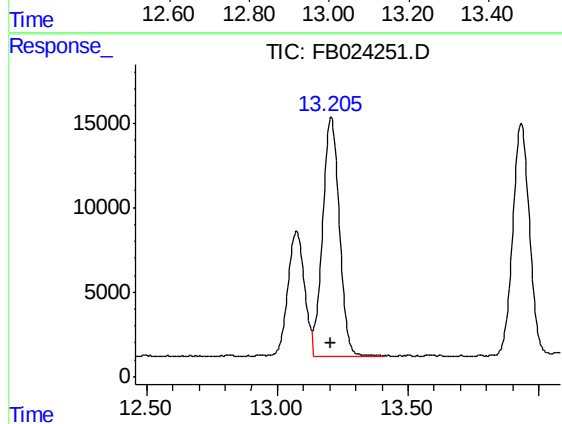


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.000 min
Response: 627033
Conc: 17.91 ng/ml

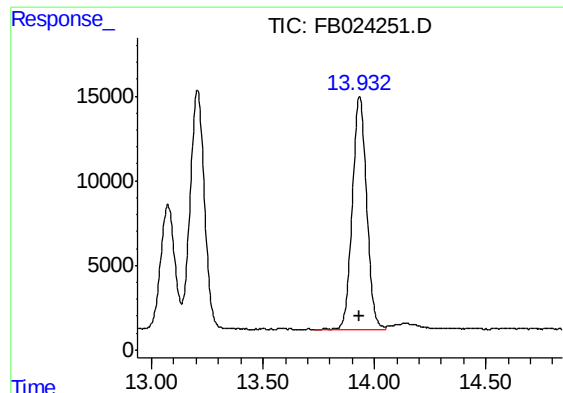

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.000 min
Response: 615475
Conc: 18.06 ng/ml

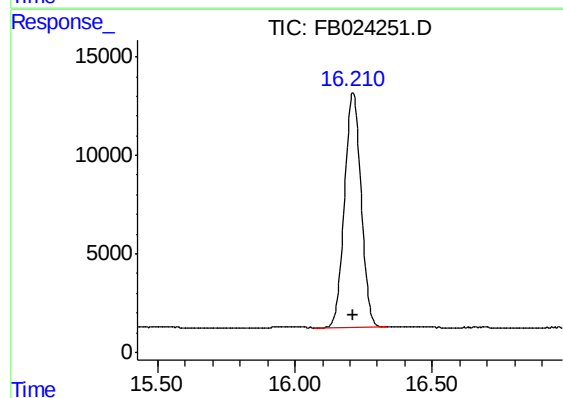

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.000 min
Response: 502194
Conc: 17.69 ng/ml