

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042420\
 Data File : FB024252.D
 Signal(s) : FID2B.CH
 Acq On : 24 Apr 2020 15:04
 Operator : DD/AJ
 Sample : L2331-07MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 25 02:19:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	442684	17.670 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	748760	22.938 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	740796	21.707 ng/ml
3) t n-Heptane	7.761	238919	7.079 ng/ml
4) t Benzene	7.896	369780	9.162 ng/ml
6) t Toluene	10.634	1038783	26.424 ng/ml
7) t Ethylbenzene	13.074	315607	8.657 ng/ml
8) t m-Xylene	13.207	604597	17.271 ng/ml
9) t O-Xylene	13.934	592090	17.372 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	477285	16.810 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042420\
Data File : FB0424252.D
Signal(s) : FID2B.CH
Acq On : 24 Apr 2020 15:04
Operator : DD/AJ
Sample : L2331-07MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 25 02:19:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

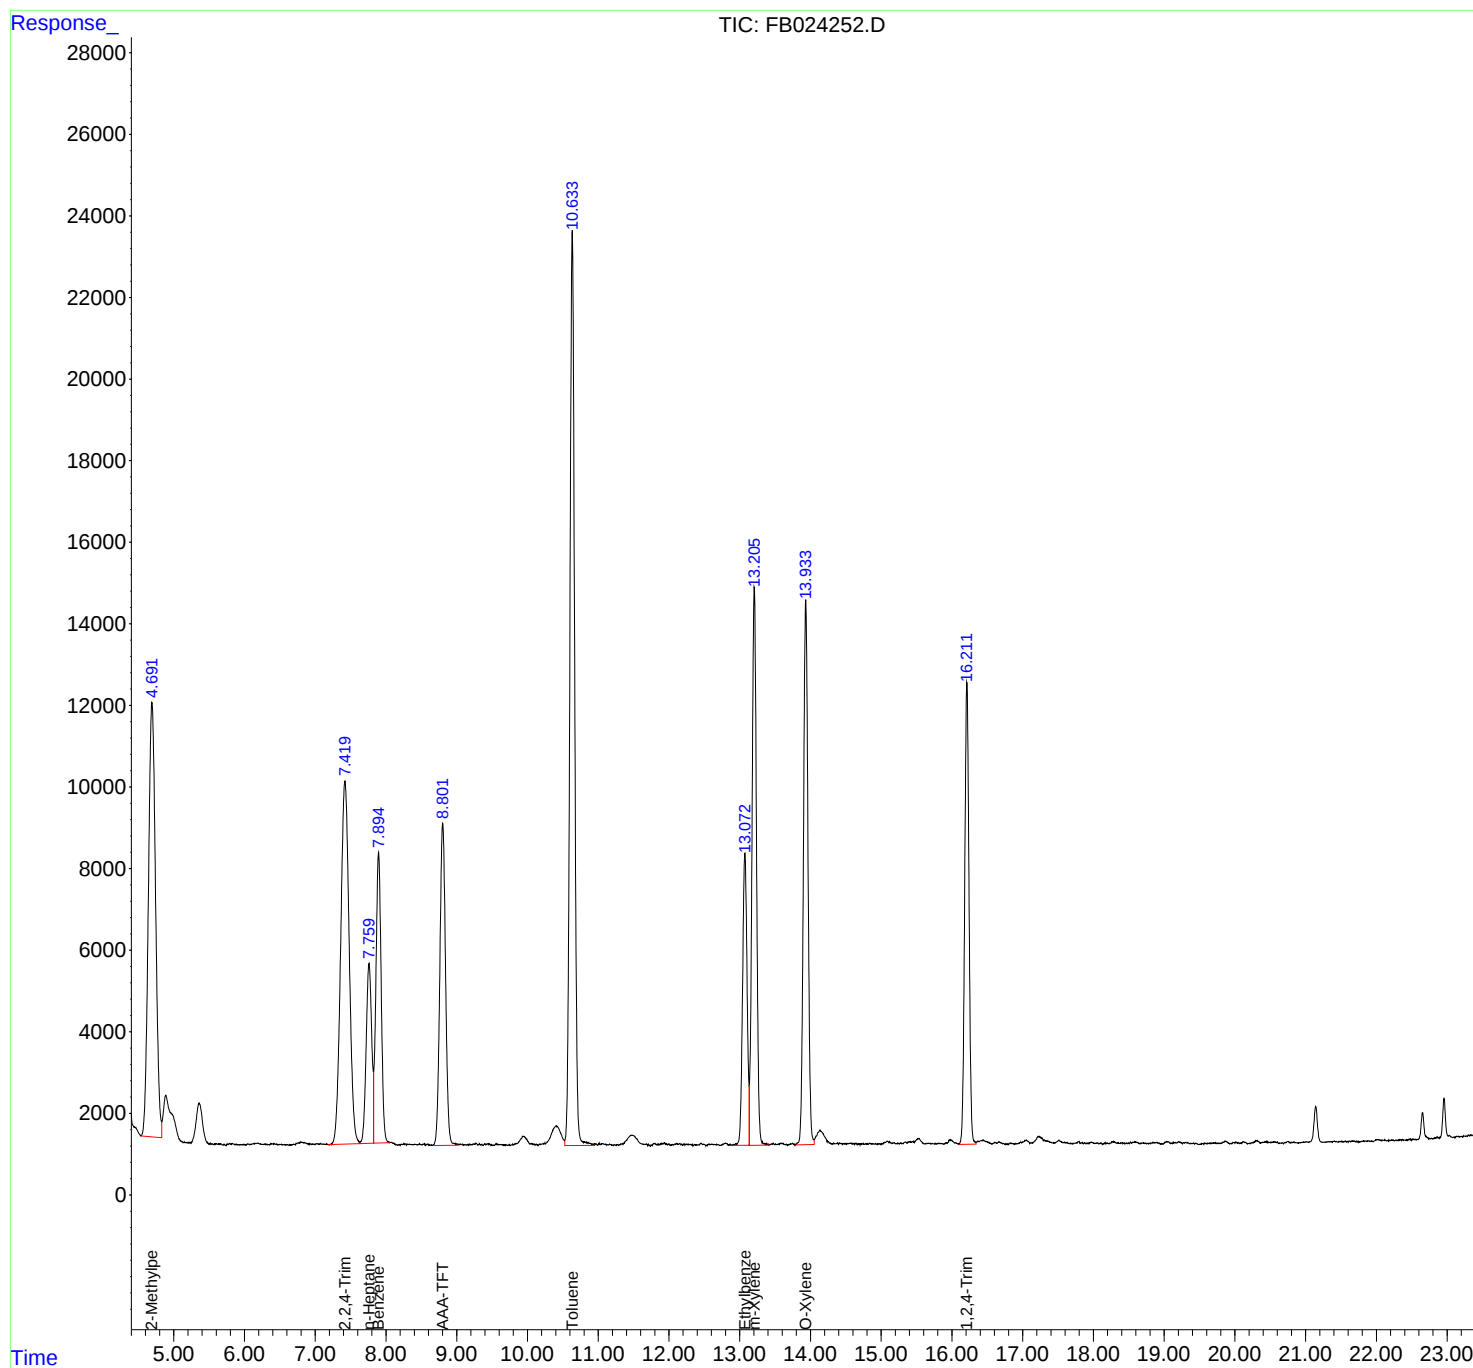

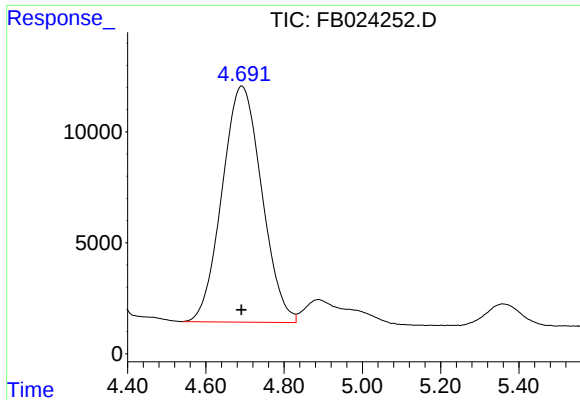


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.001 min
Response: 748760
Conc: 22.94 ng/ml

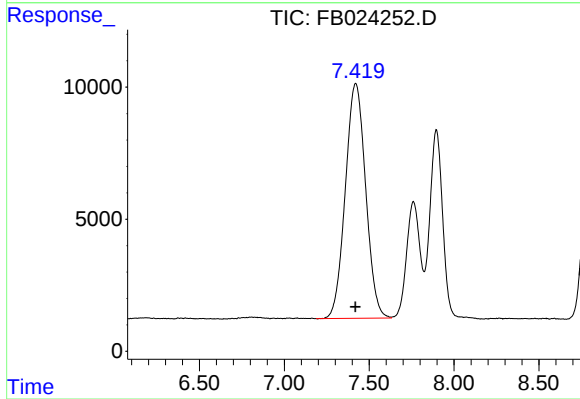


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 740796
Conc: 21.71 ng/ml

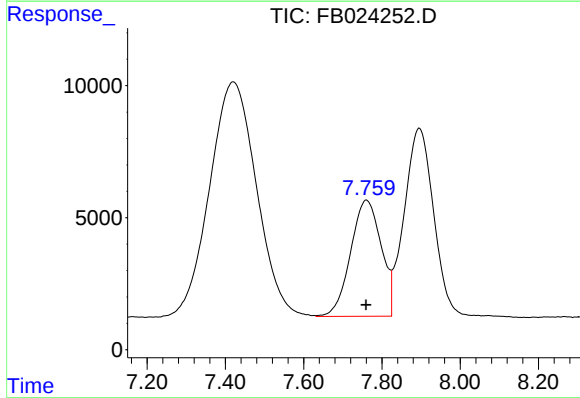


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.001 min
Response: 238919
Conc: 7.08 ng/ml

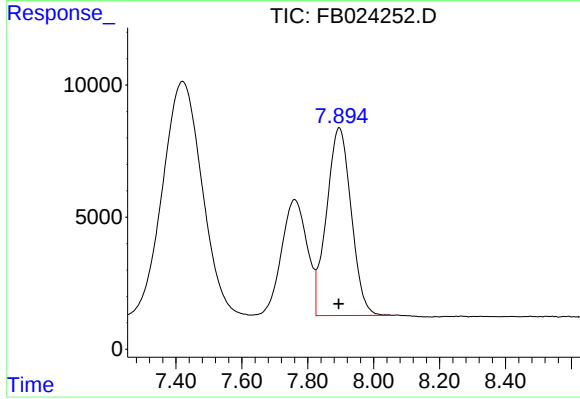


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.002 min
Response: 369780
Conc: 9.16 ng/ml

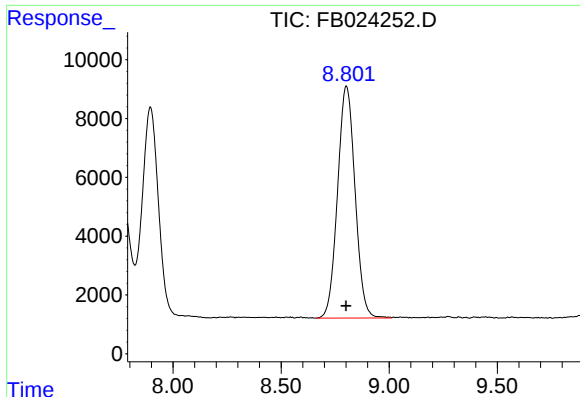


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.001 min
Response: 442684
Conc: 17.67 ng/ml

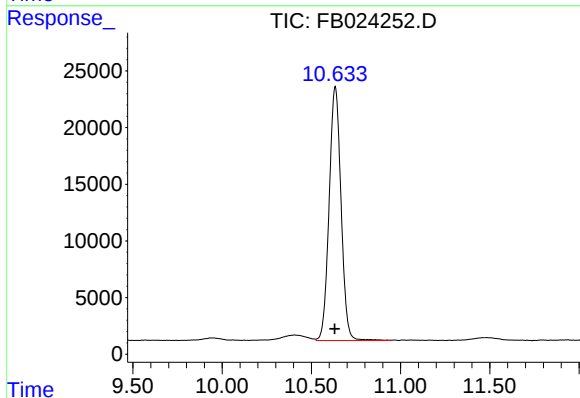


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.002 min
Response: 1038783
Conc: 26.42 ng/ml

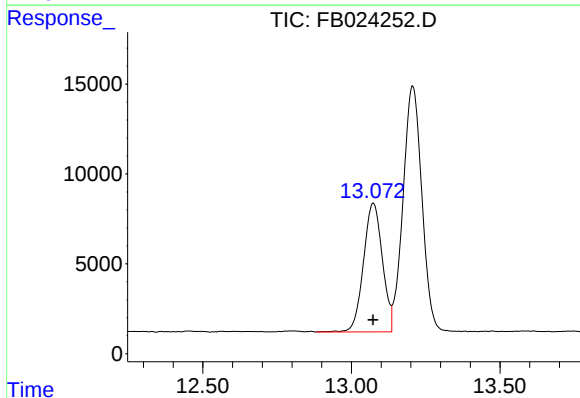


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.002 min
Response: 315607
Conc: 8.66 ng/ml

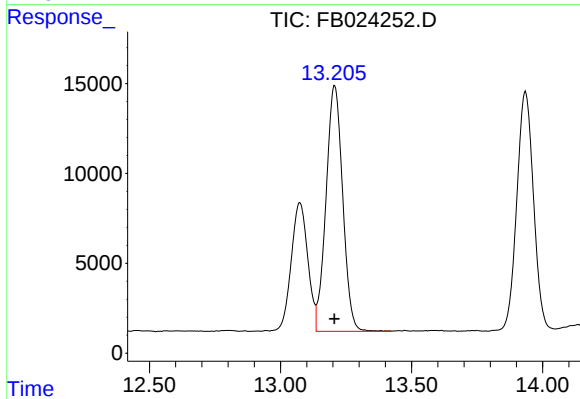

#8 m-Xylene

R.T.: 13.207 min
Delta R.T.: 0.001 min
Response: 604597
Conc: 17.27 ng/ml

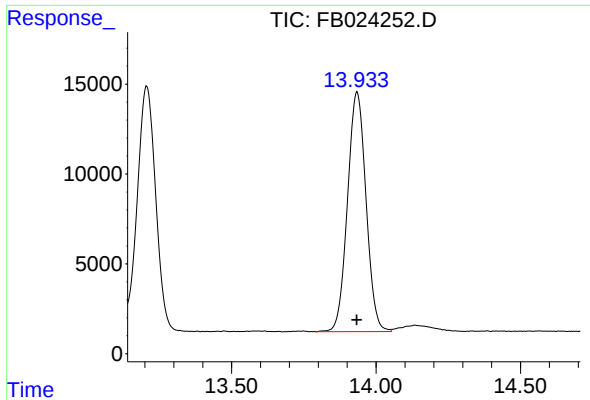


#9 O-Xylene

R.T.: 13.934 min

Delta R.T.: 0.000 min

Response: 592090

Conc: 17.37 ng/ml

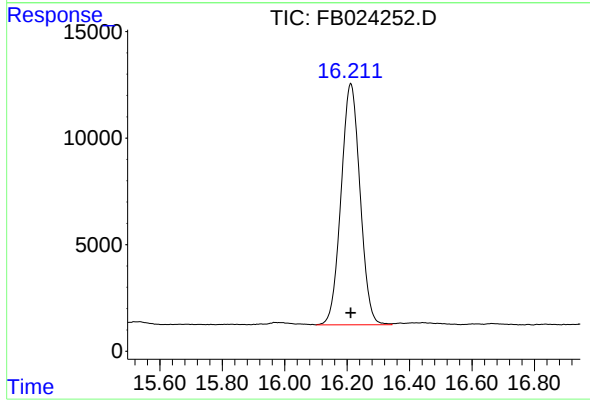

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min

Delta R.T.: 0.000 min

Response: 477285

Conc: 16.81 ng/ml