

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042423\
 Data File : FB029749.D
 Signal(s) : FID2B.CH
 Acq On : 25 Apr 2023 5:22
 Operator : YP/AJ
 Sample : 02470-16MS 50X
 Misc : 5.03G/5.00 ML MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 25 06:46:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
 Quant Title :
 QLast Update : Mon Apr 17 12:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	243323	18.259 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	308608	21.934 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	392206	25.533 ng/ml
3) t n-Heptane	7.743	117579	7.306 ng/ml
4) t Benzene	7.879	181416	9.136 ng/ml
6) t Toluene	10.612	519451	26.894 ng/ml
7) t Ethylbenzene	13.049	167529	9.256 ng/ml
8) t m-Xylene	13.182	322256	17.818 ng/ml
9) t O-Xylene	13.908	312556	17.824 ng/ml
10) t 1,2,4-Trimethylbenzene	16.184	288783	16.159 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042423\
Data File : FB029749.D
Signal(s) : FID2B.CH
Acq On : 25 Apr 2023 5:22
Operator : YP/AJ
Sample : 02470-16MS 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 25 06:46:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

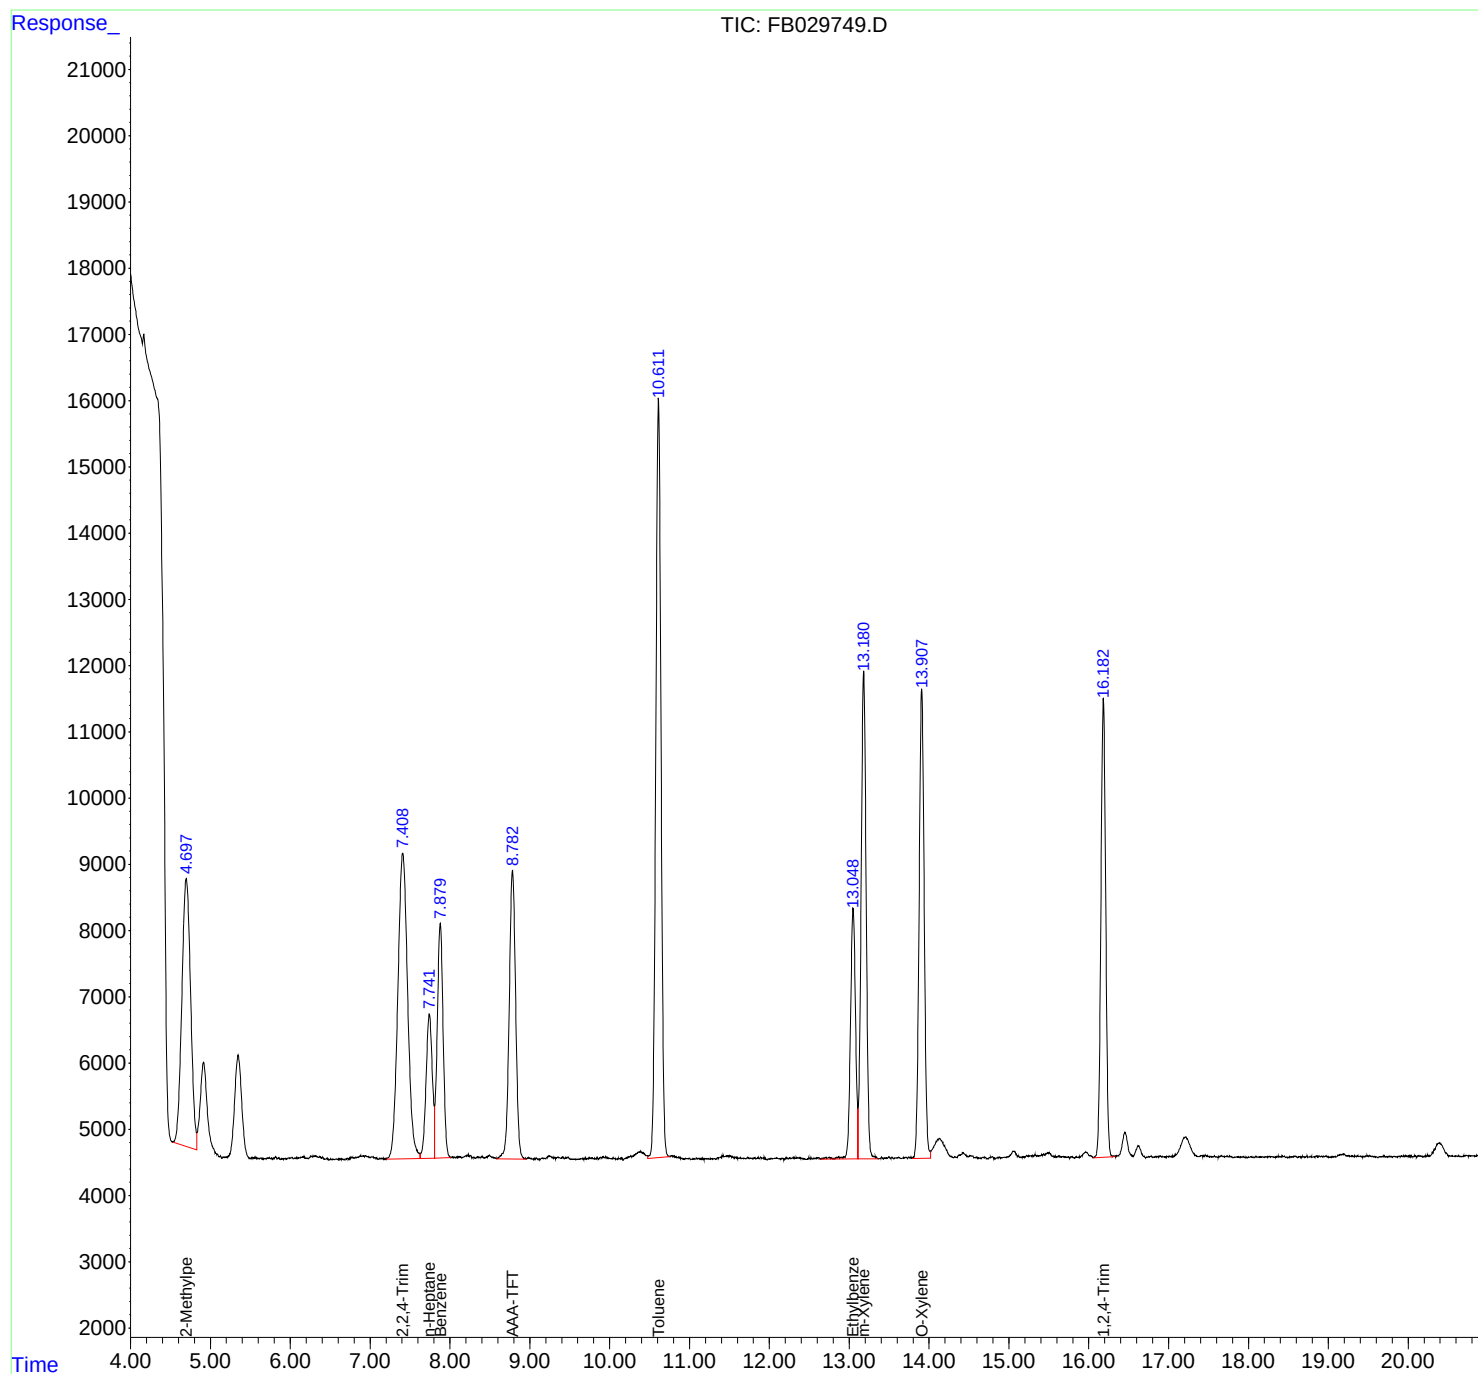


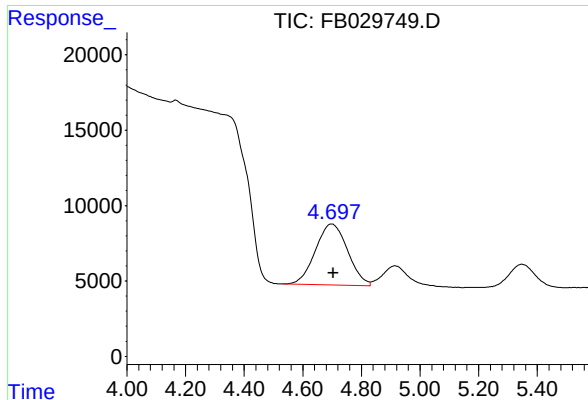

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.006 min
Response: 308608
Conc: 21.93 ng/ml

Instrument :
FID_B
ClientSampleId :

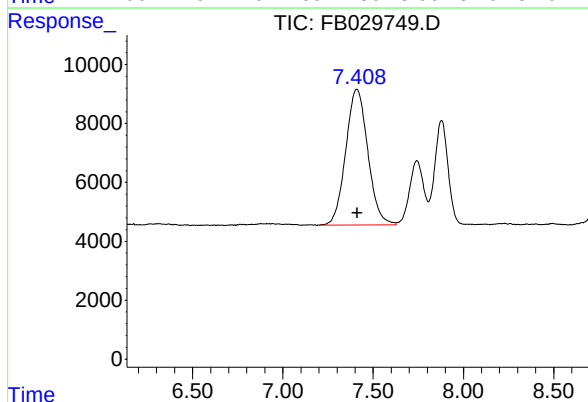


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.004 min
Response: 392206
Conc: 25.53 ng/ml

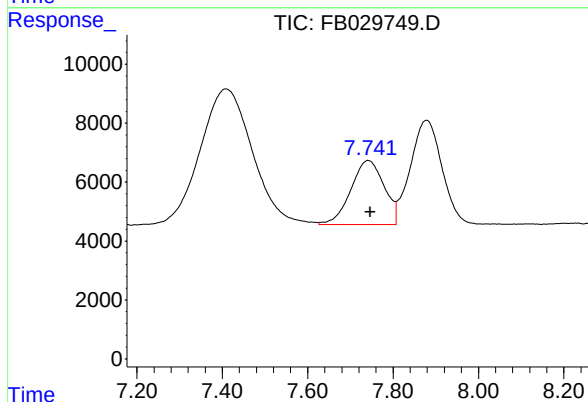


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.004 min
Response: 117579
Conc: 7.31 ng/ml

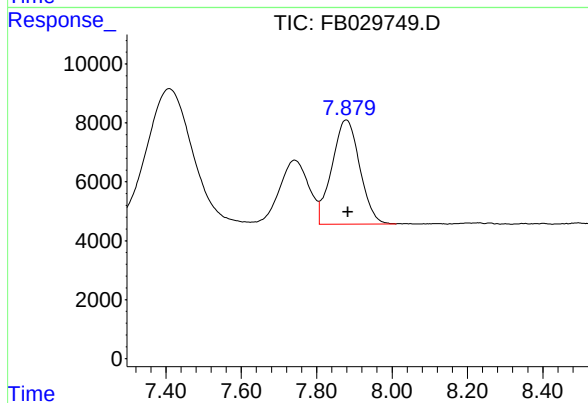

#4 Benzene

R.T.: 7.879 min
Delta R.T.: -0.004 min
Response: 181416
Conc: 9.14 ng/ml

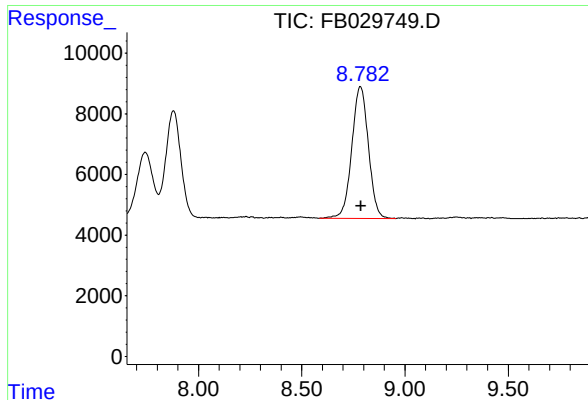


#5 AAA-TFT

R.T.: 8.784 min
Delta R.T.: -0.003 min
Response: 243323
Conc: 18.26 ng/ml

Instrument :


FID_B

ClientSampleId :

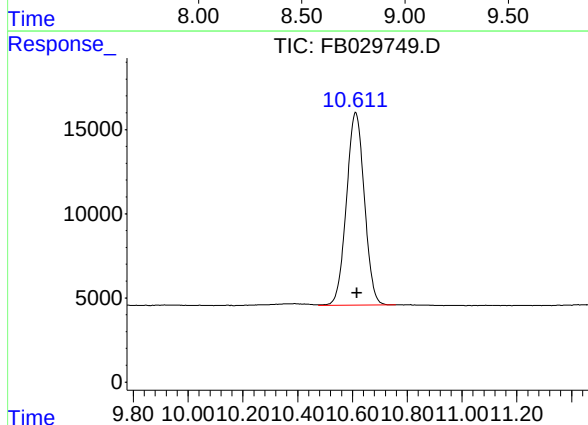


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.004 min
Response: 519451
Conc: 26.89 ng/ml

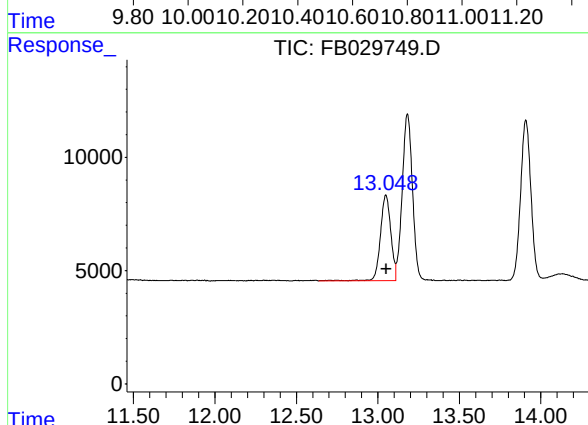


#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: -0.003 min
Response: 167529
Conc: 9.26 ng/ml

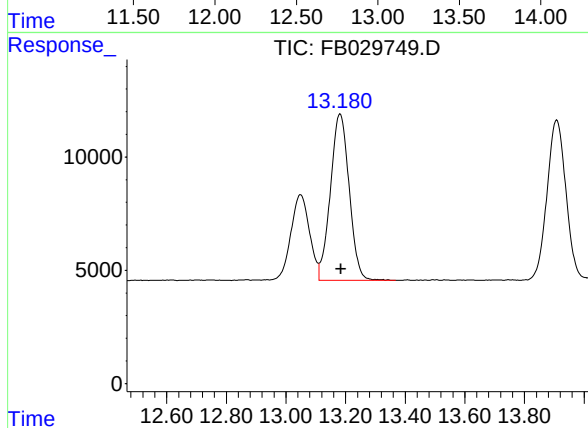

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: -0.003 min
Response: 322256
Conc: 17.82 ng/ml

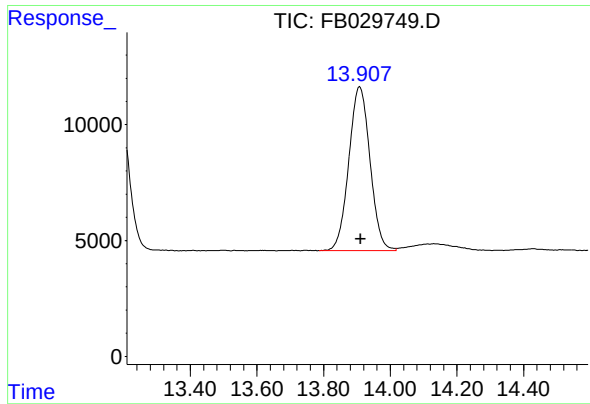

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: -0.003 min
Response: 312556
Conc: 17.82 ng/ml

Instrument :
FID_B
ClientSampleId :

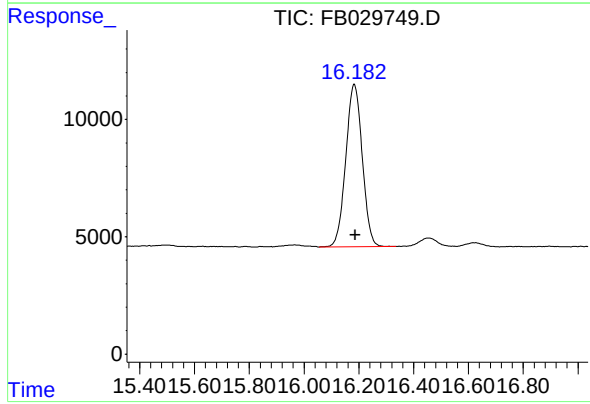

#10 1,2,4-Trimethylbenzene

R.T.: 16.184 min
Delta R.T.: -0.003 min
Response: 288783
Conc: 16.16 ng/ml