

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042423\
 Data File : FB029723.D
 Signal(s) : FID2B.CH
 Acq On : 24 Apr 2023 11:18
 Operator : YP/AJ
 Sample : BSF0424S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0424S1

Integration File: Calibration.e
 Quant Time: Apr 25 03:38:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
 Quant Title :
 QLast Update : Mon Apr 17 12:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	263528	19.775 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	370282	26.318 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	430282	28.012 ng/ml
3) t n-Heptane	7.745	137391	8.537 ng/ml
4) t Benzene	7.881	191036	9.621 ng/ml
6) t Toluene	10.613	561624	29.077 ng/ml
7) t Ethylbenzene	13.050	180823	9.991 ng/ml
8) t m-Xylene	13.182	355974	19.683 ng/ml
9) t O-Xylene	13.909	346574	19.764 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	349218	19.541 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042423\
Data File : FB029723.D
Signal(s) : FID2B.CH
Acq On : 24 Apr 2023 11:18
Operator : YP/AJ
Sample : BSF0424S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0424S1

Integration File: Calibration.e
Quant Time: Apr 25 03:38:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

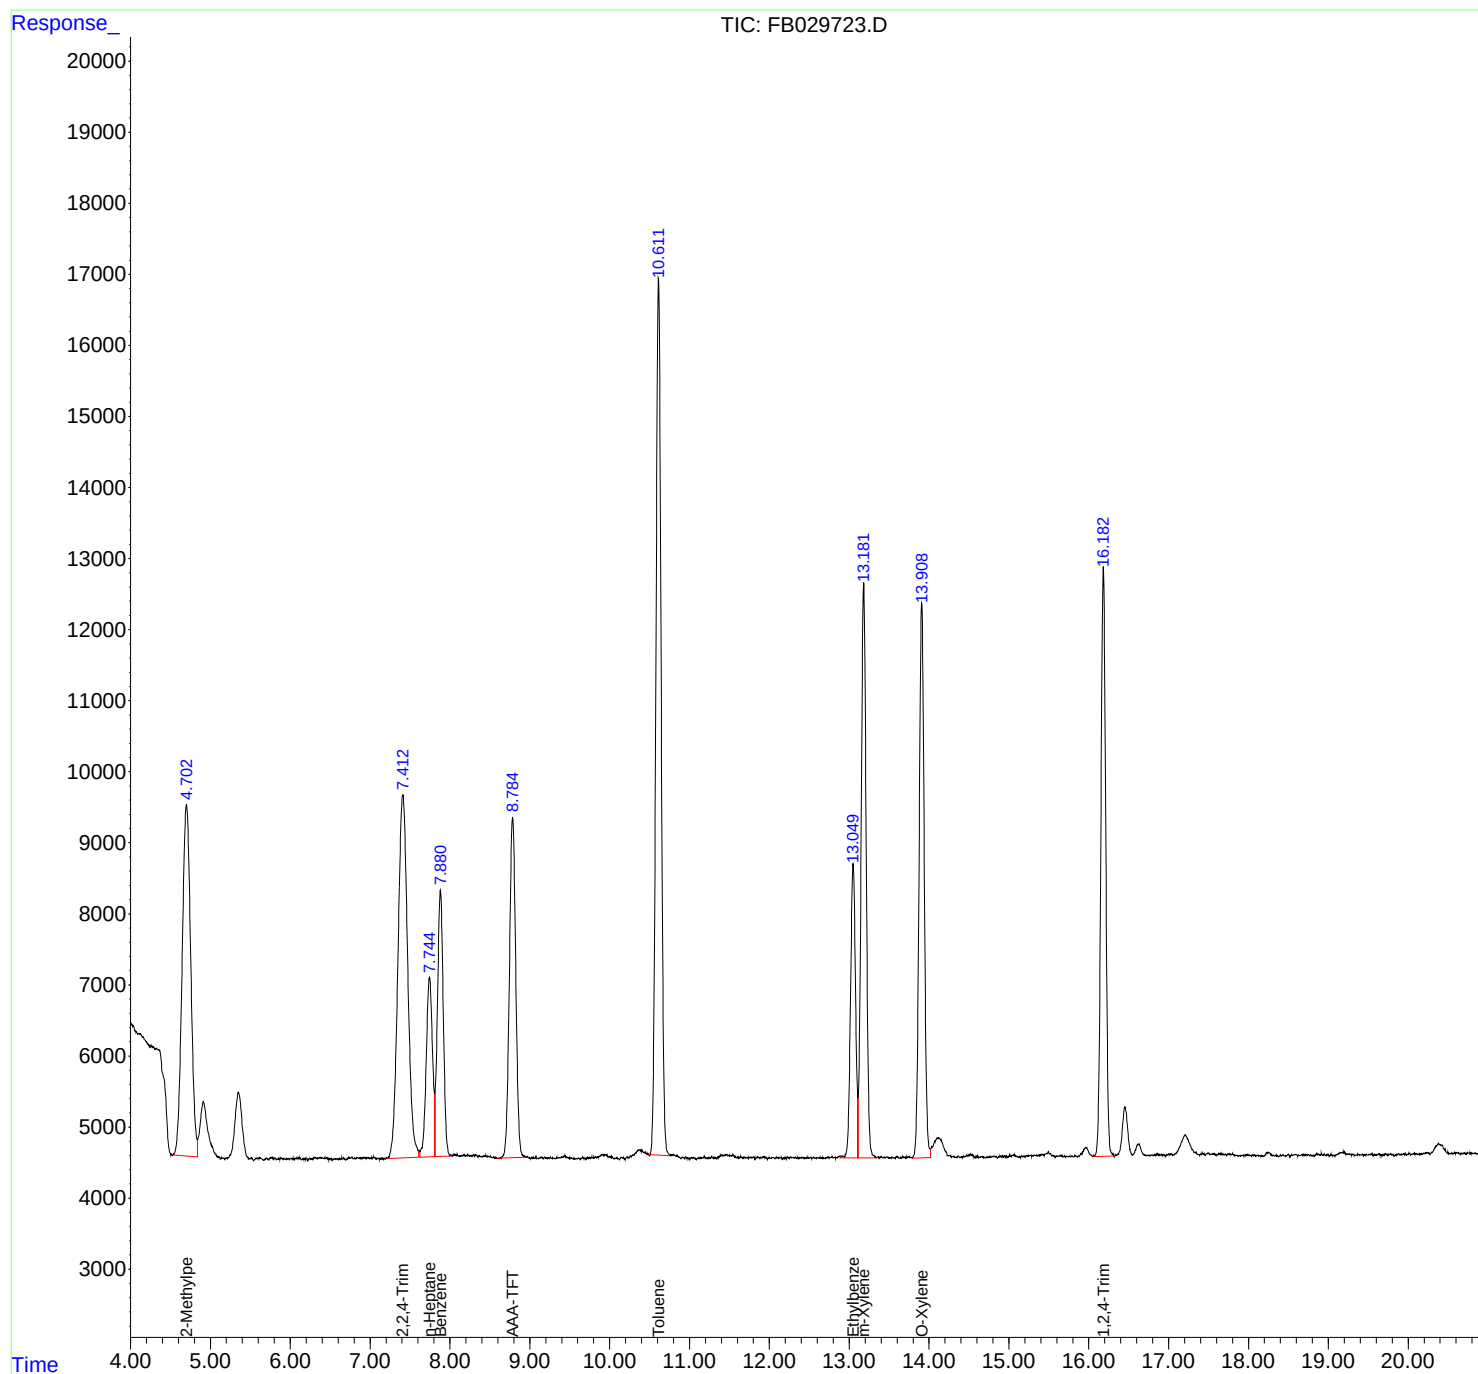


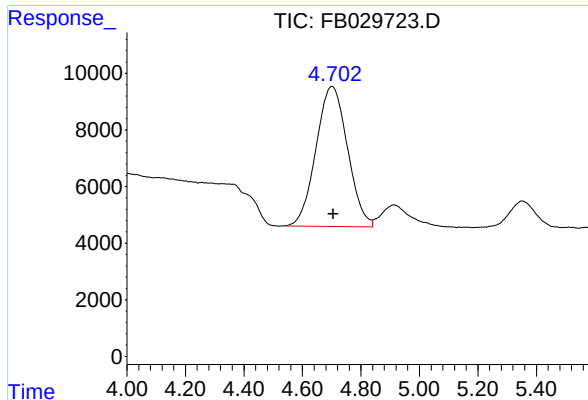

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.003 min
Response: 370282
Conc: 26.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0424S1

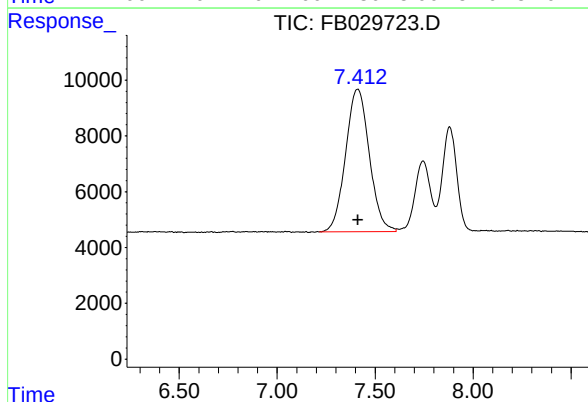


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: 0.000 min
Response: 430282
Conc: 28.01 ng/ml

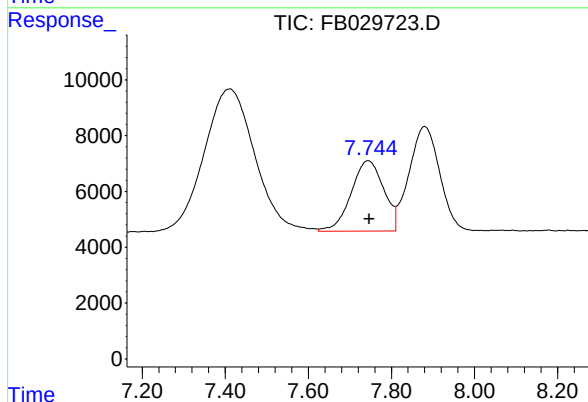


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.002 min
Response: 137391
Conc: 8.54 ng/ml

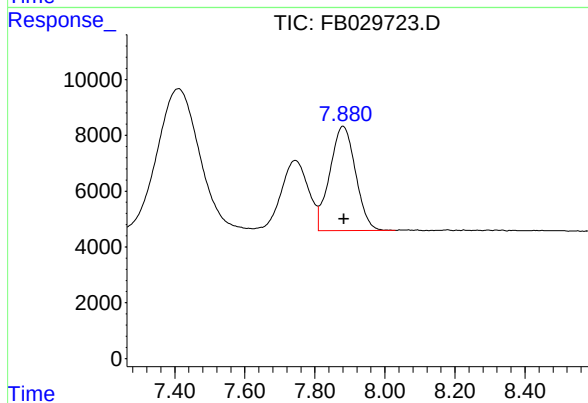

#4 Benzene


R.T.: 7.881 min
Delta R.T.: -0.002 min
Response: 191036
Conc: 9.62 ng/ml

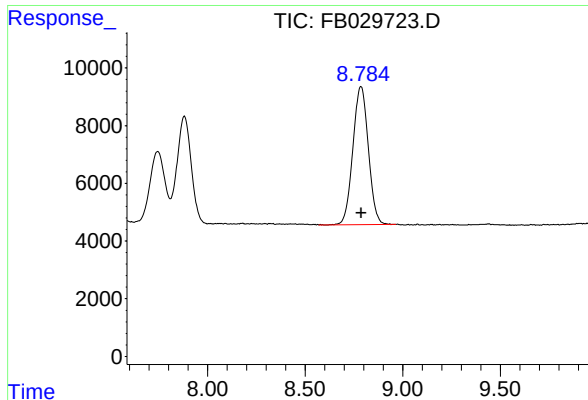

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.002 min
Response: 263528
Conc: 19.78 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0424S1

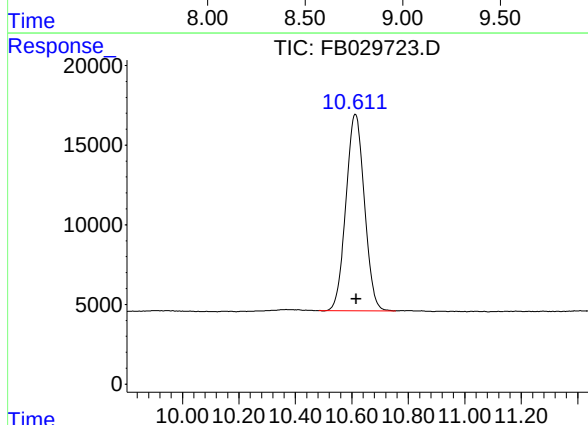


#6 Toluene

R.T.: 10.613 min
Delta R.T.: -0.003 min
Response: 561624
Conc: 29.08 ng/ml

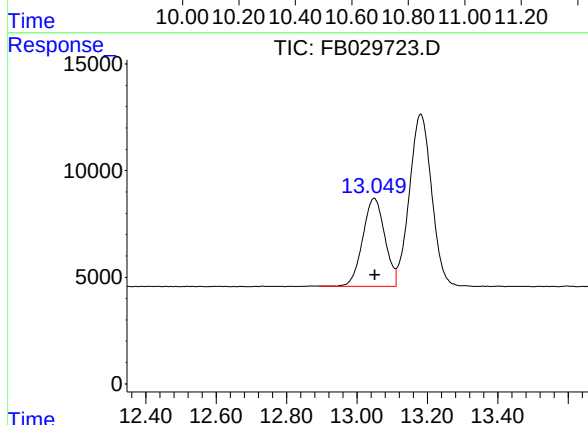


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: -0.002 min
Response: 180823
Conc: 9.99 ng/ml

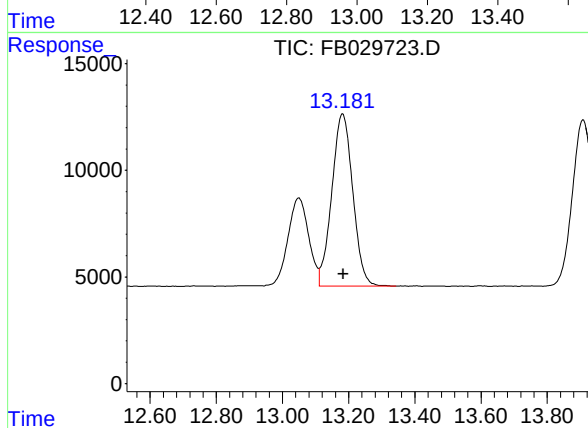

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: -0.003 min
Response: 355974
Conc: 19.68 ng/ml

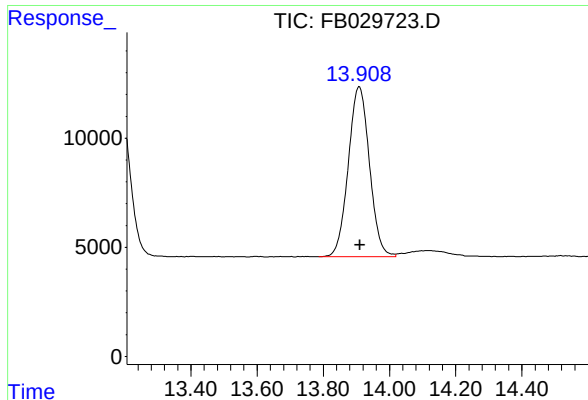

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: -0.003 min
Response: 346574
Conc: 19.76 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0424S1

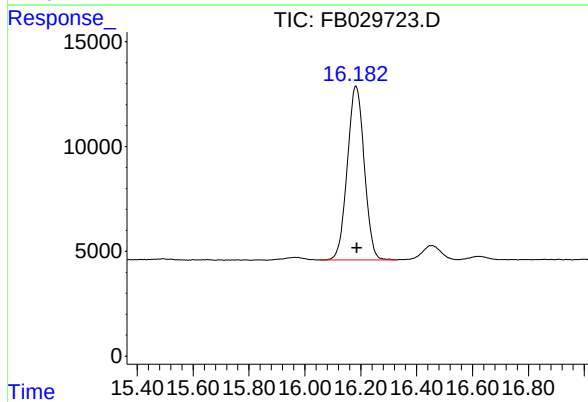

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.003 min
Response: 349218
Conc: 19.54 ng/ml