

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042423\
 Data File : FB029730.D
 Signal(s) : FID2B.CH
 Acq On : 24 Apr 2023 15:49
 Operator : YP/AJ
 Sample : BSF0424S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0424S2

Integration File: Calibration.e
 Quant Time: Apr 25 03:38:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
 Quant Title :
 QLast Update : Mon Apr 17 12:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.786	254840	19.123 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.700	364786	25.927 ng/ml
2) t	2,2,4-Trimethylpentane	7.410	421815	27.461 ng/ml
3) t	n-Heptane	7.745	132614	8.240 ng/ml
4) t	Benzene	7.880	192101	9.674 ng/ml
6) t	Toluene	10.614	577675	29.908 ng/ml
7) t	Ethylbenzene	13.050	185684	10.259 ng/ml
8) t	m-Xylene	13.183	365938	20.234 ng/ml
9) t	O-Xylene	13.910	353768	20.174 ng/ml
10) t	1,2,4-Trimethylbenzene	16.185	354334	19.827 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042423\
Data File : FB029730.D
Signal(s) : FID2B.CH
Acq On : 24 Apr 2023 15:49
Operator : YP/AJ
Sample : BSF0424S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0424S2

Integration File: Calibration.e
Quant Time: Apr 25 03:38:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

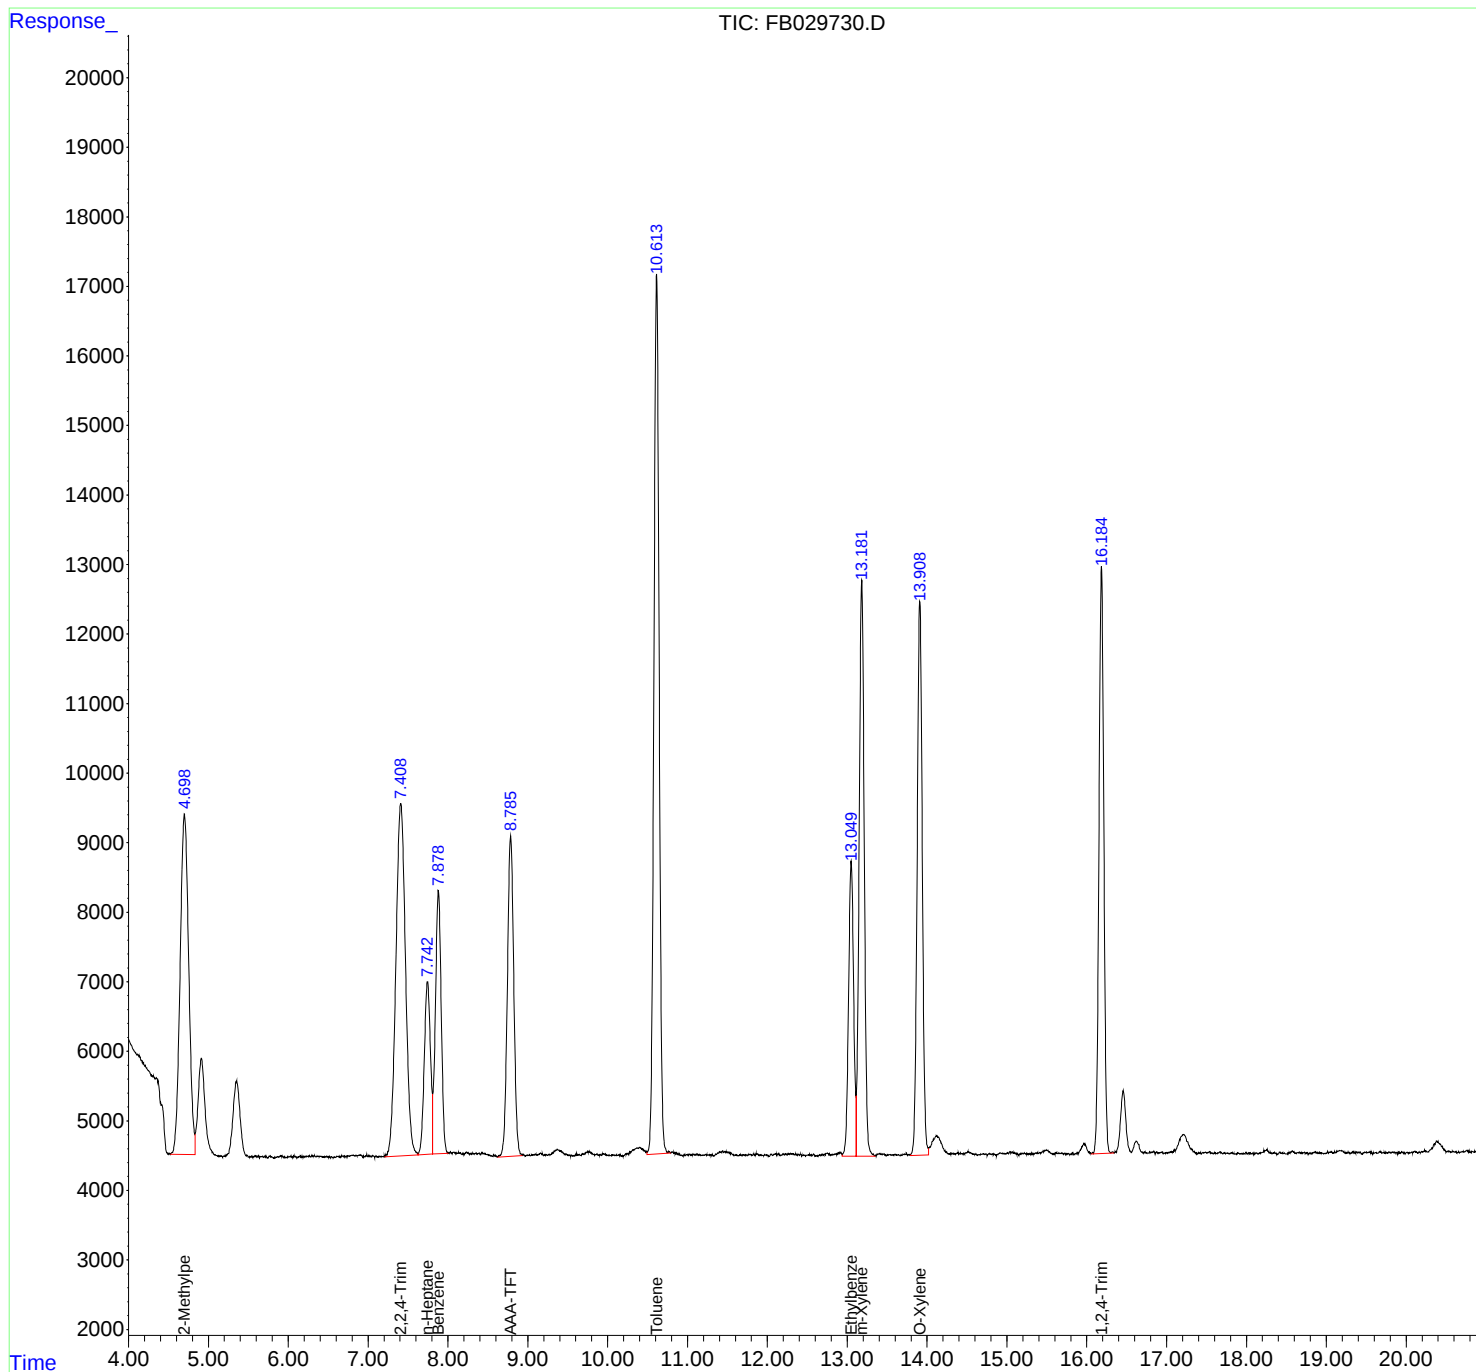


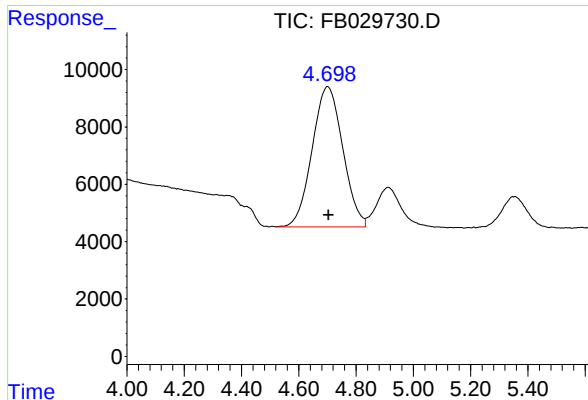

#1 2-Methylpentane


R.T.: 4.700 min
Delta R.T.: -0.005 min
Response: 364786
Conc: 25.93 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0424S2

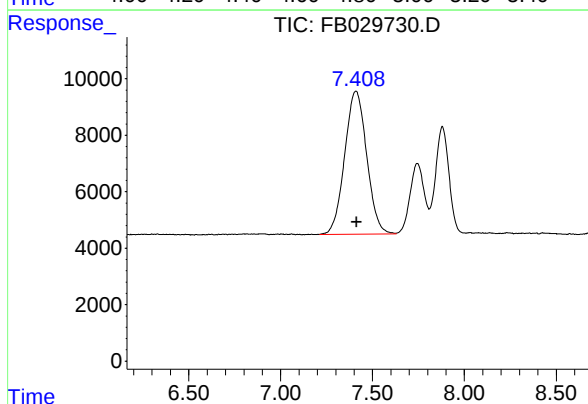


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.003 min
Response: 421815
Conc: 27.46 ng/ml

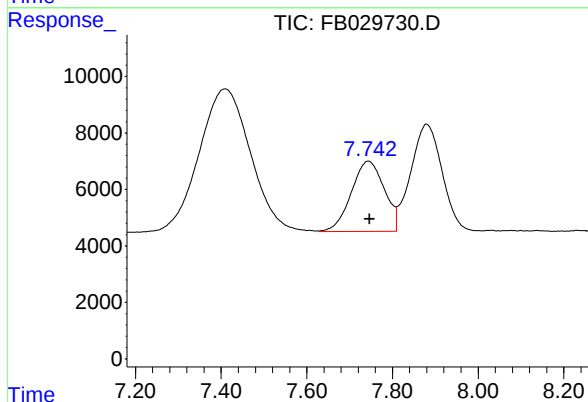


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.002 min
Response: 132614
Conc: 8.24 ng/ml

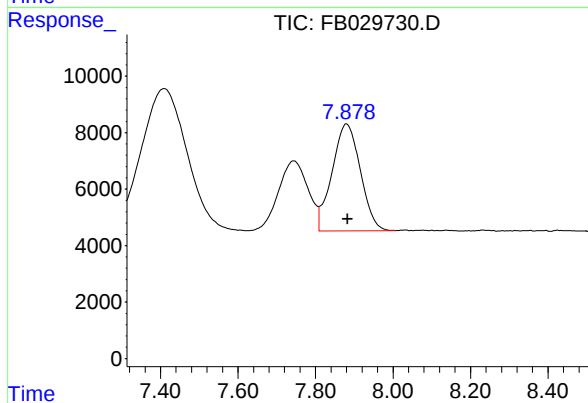

#4 Benzene


R.T.: 7.880 min
Delta R.T.: -0.003 min
Response: 192101
Conc: 9.67 ng/ml

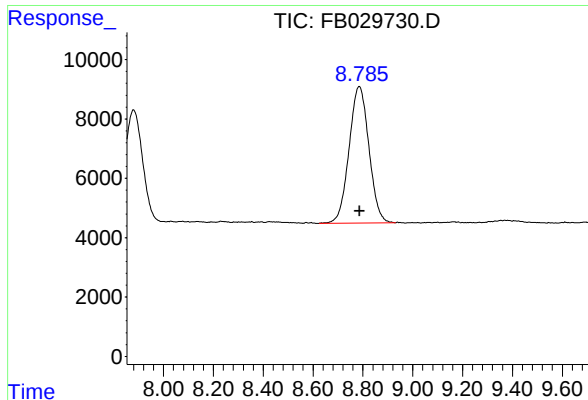

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.001 min
Response: 254840
Conc: 19.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0424S2

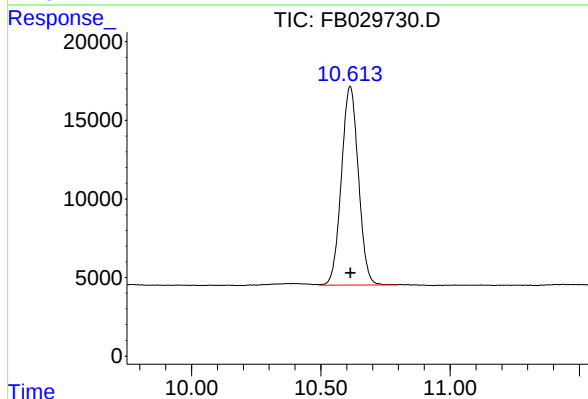


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.002 min
Response: 577675
Conc: 29.91 ng/ml

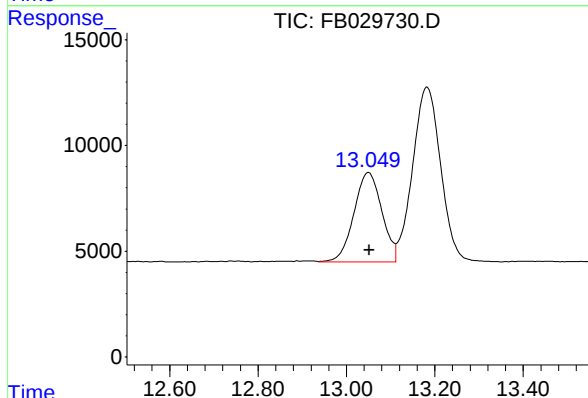


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: -0.002 min
Response: 185684
Conc: 10.26 ng/ml

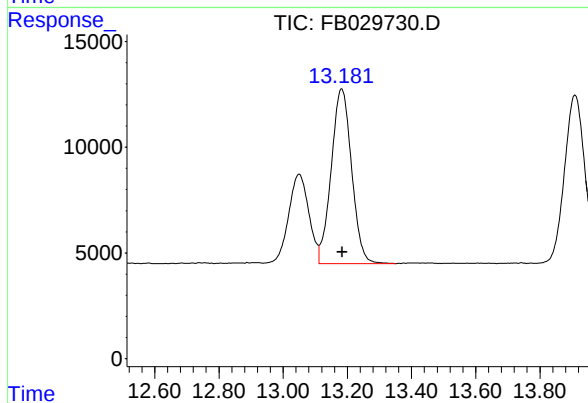

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: -0.002 min
Response: 365938
Conc: 20.23 ng/ml

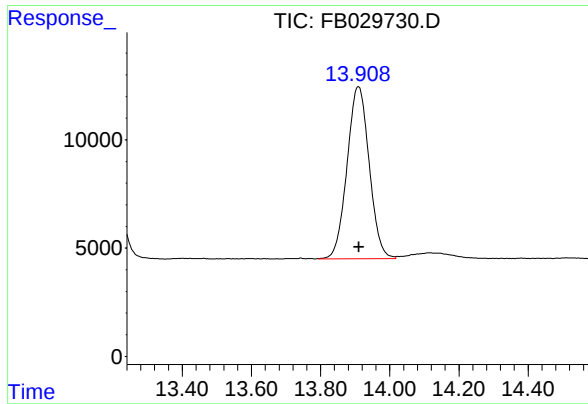

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.002 min
Response: 353768
Conc: 20.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0424S2

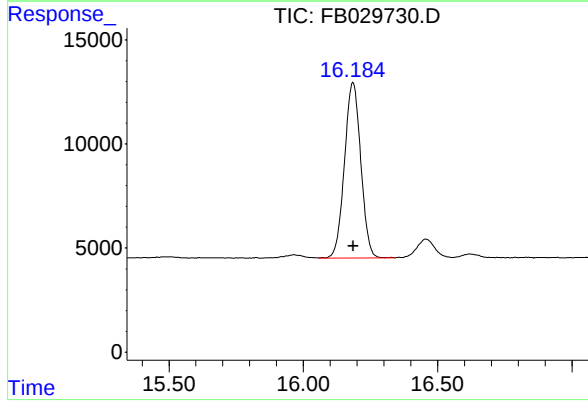

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: -0.002 min
Response: 354334
Conc: 19.83 ng/ml