

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042519\
 Data File : FB020846.D
 Signal(s) : FID2B.CH
 Acq On : 25 Apr 2019 10:25
 Operator : MJ/SJ
 Sample : BSF0425S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 26 00:32:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	383000	20.765 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.866	1071642	30.441 ng/ml
2) t 2,2,4-Trimethylpentane	7.619	999270	33.517 ng/ml
3) t n-Heptane	7.951	396267	10.094 ng/ml
4) t Benzene	8.088	420945	10.248 ng/ml
6) t Toluene	10.838	928057	30.714 ng/ml
7) t Ethylbenzene	13.288	272151	10.638 ng/ml
8) t m-Xylene	13.421	553969	20.960 ng/ml
9) t O-Xylene	14.152	562179	20.766 ng/ml
10) t 1,2,4-Trimethylbenzene	16.437	544840	20.853 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042519\
Data File : FB020846.D
Signal(s) : FID2B.CH
Acq On : 25 Apr 2019 10:25
Operator : MJ/SJ
Sample : BSF0425S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 26 00:32:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

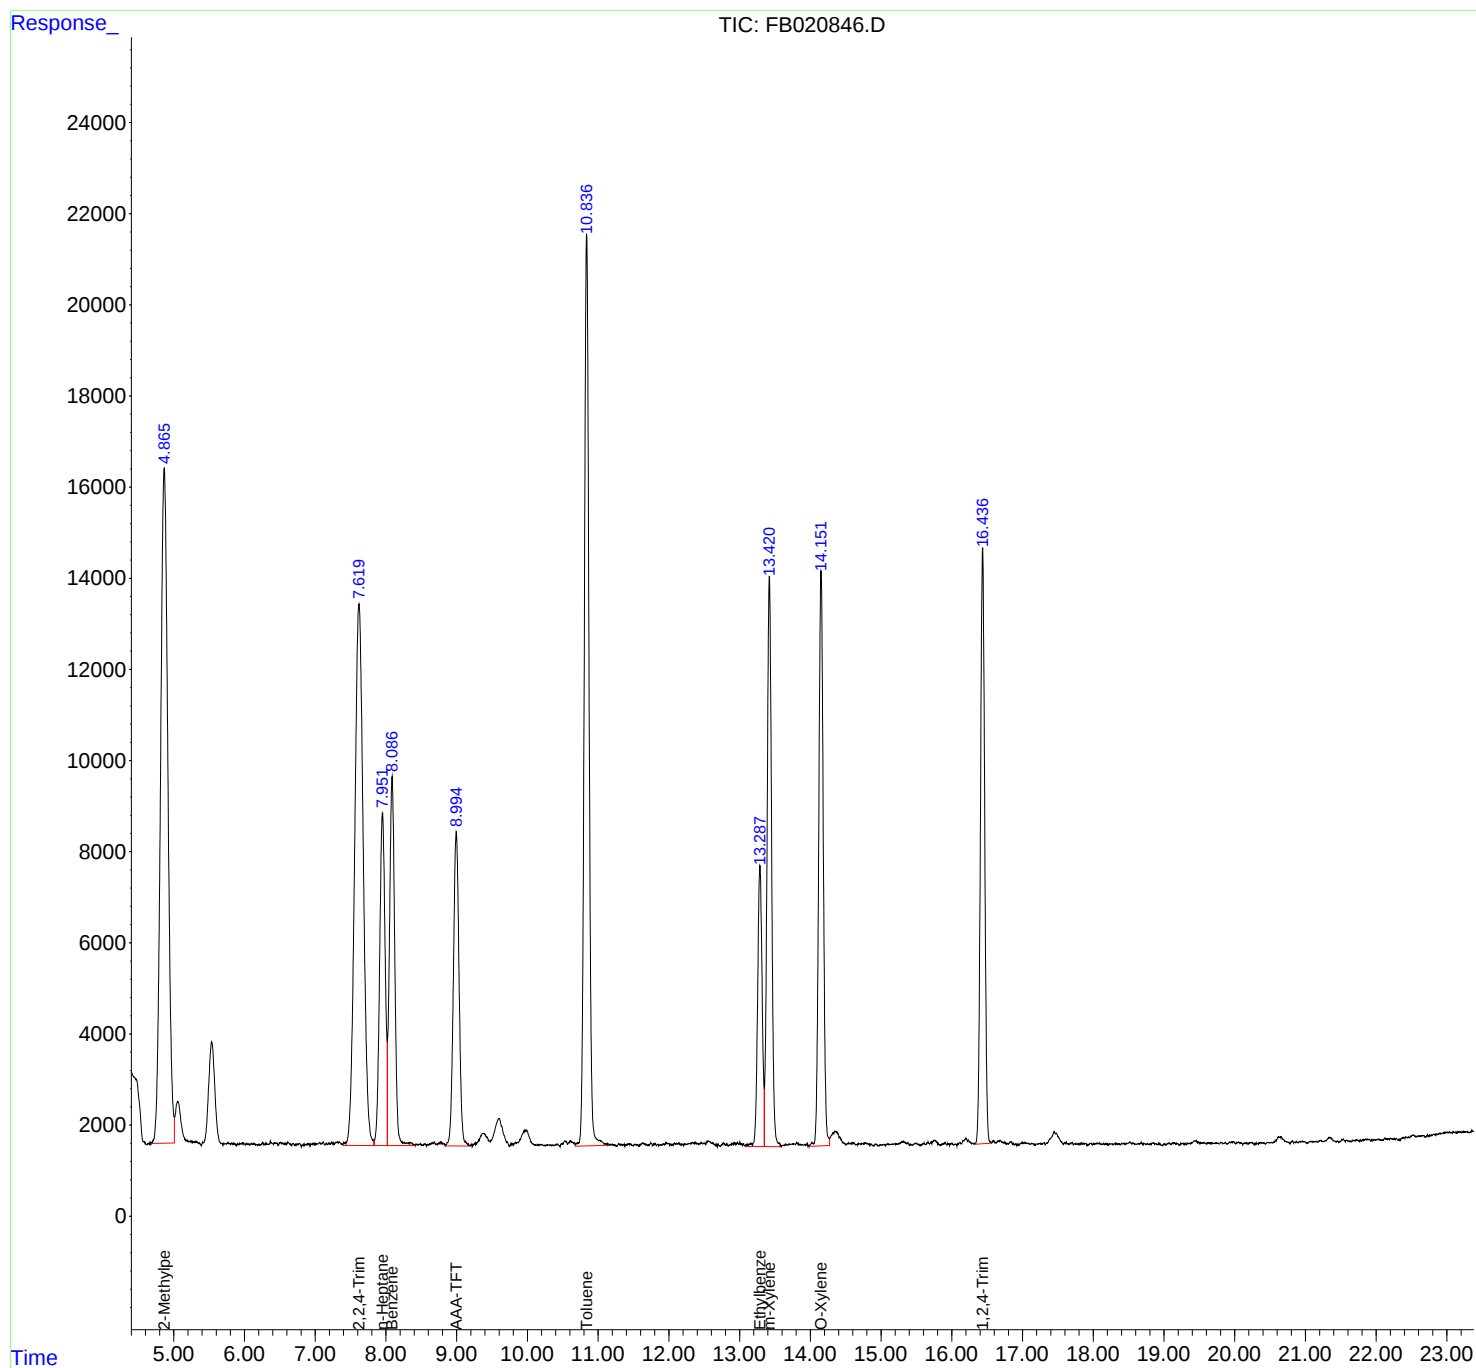

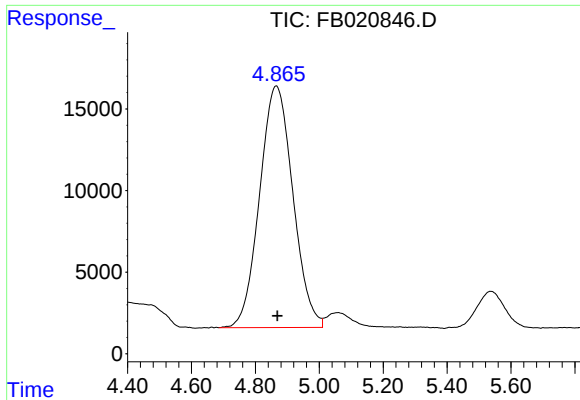


#1 2-Methylpentane

R.T.: 4.866 min
Delta R.T.: -0.003 min
Response: 1071642
Conc: 30.44 ng/ml

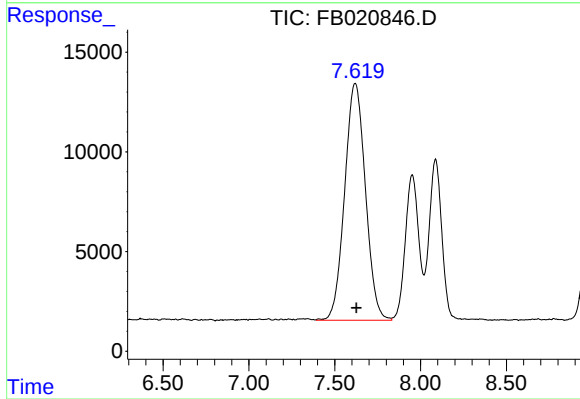


#2 2,2,4-Trimethylpentane

R.T.: 7.619 min
Delta R.T.: -0.007 min
Response: 999270
Conc: 33.52 ng/ml

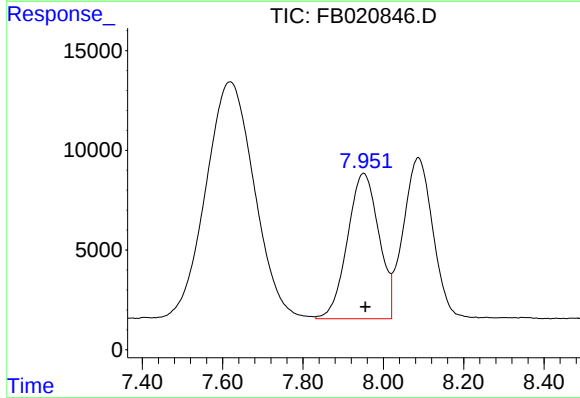


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.004 min
Response: 396267
Conc: 10.09 ng/ml

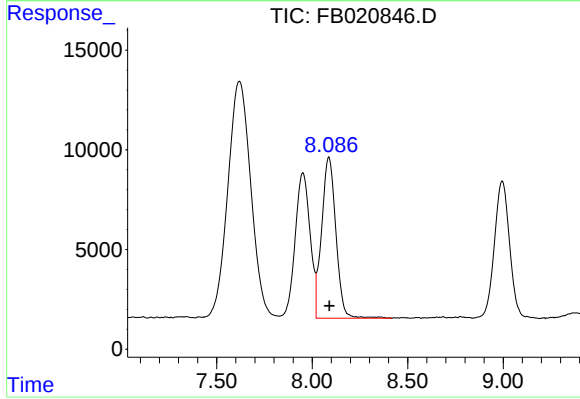


#4 Benzene

R.T.: 8.088 min
Delta R.T.: -0.003 min
Response: 420945
Conc: 10.25 ng/ml

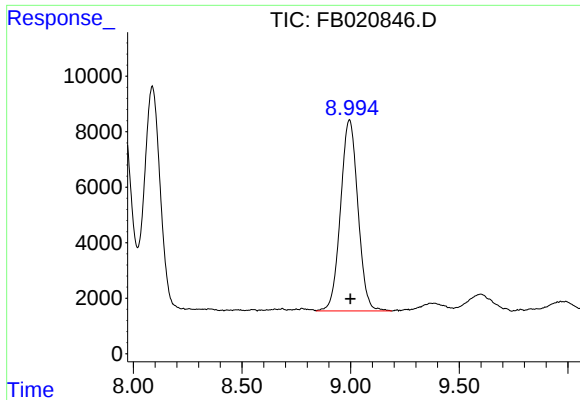


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: -0.004 min
Response: 383000
Conc: 20.77 ng/ml

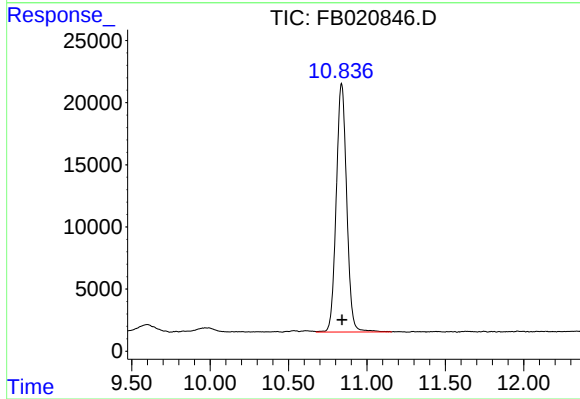


#6 Toluene

R.T.: 10.838 min
Delta R.T.: -0.004 min
Response: 928057
Conc: 30.71 ng/ml

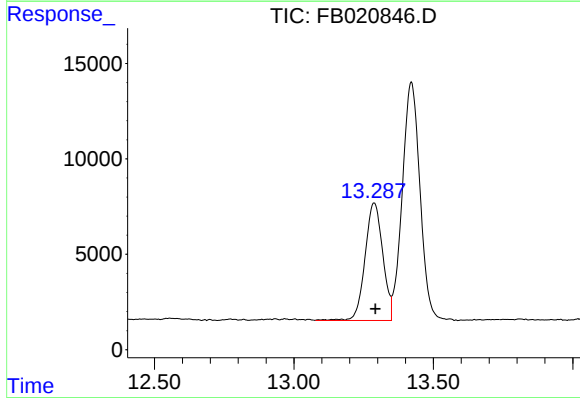


#7 Ethylbenzene

R.T.: 13.288 min
Delta R.T.: -0.004 min
Response: 272151
Conc: 10.64 ng/ml

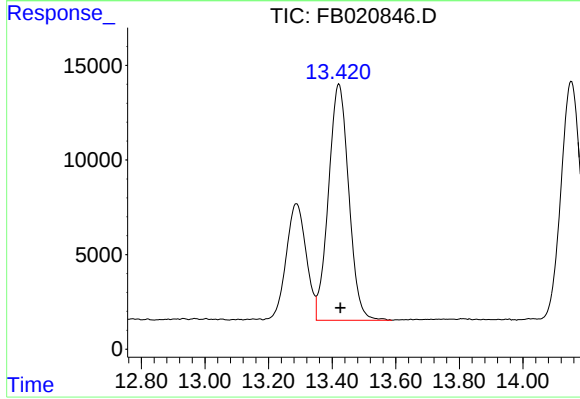

#8 m-Xylene

R.T.: 13.421 min
Delta R.T.: -0.004 min
Response: 553969
Conc: 20.96 ng/ml

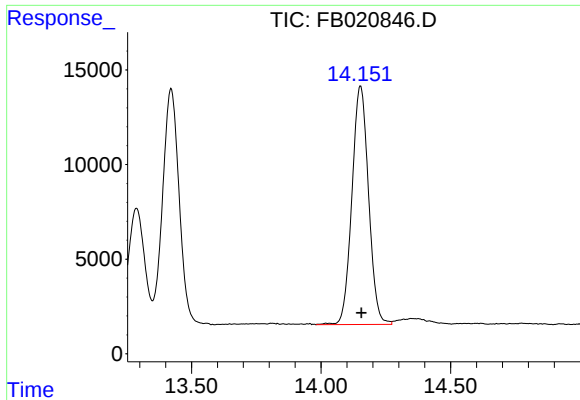


#9 O-Xylene

R.T.: 14.152 min

Delta R.T.: -0.004 min

Response: 562179

Conc: 20.77 ng/ml

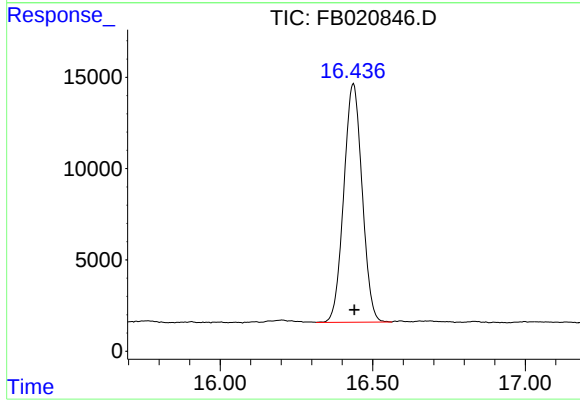

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min

Delta R.T.: -0.004 min

Response: 544840

Conc: 20.85 ng/ml