

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042519\
 Data File : FB020851.D
 Signal(s) : FID2B.CH
 Acq On : 25 Apr 2019 12:55
 Operator : MJ/SJ
 Sample : K2203-19MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 26 00:33:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	381811	20.701 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.865	912292	25.915 ng/ml
2) t 2,2,4-Trimethylpentane	7.620	757660	25.413 ng/ml
3) t n-Heptane	7.952	301814	7.688 ng/ml
4) t Benzene	8.088	398990	9.714 ng/ml
6) t Toluene	10.839	869498	28.776 ng/ml
7) t Ethylbenzene	13.290	239753	9.372 ng/ml
8) t m-Xylene	13.422	496261	18.777 ng/ml
9) t O-Xylene	14.153	509728	18.829 ng/ml
10) t 1,2,4-Trimethylbenzene	16.438	475408	18.196 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042519\
Data File : FB020851.D
Signal(s) : FID2B.CH
Acq On : 25 Apr 2019 12:55
Operator : MJ/SJ
Sample : K2203-19MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 26 00:33:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

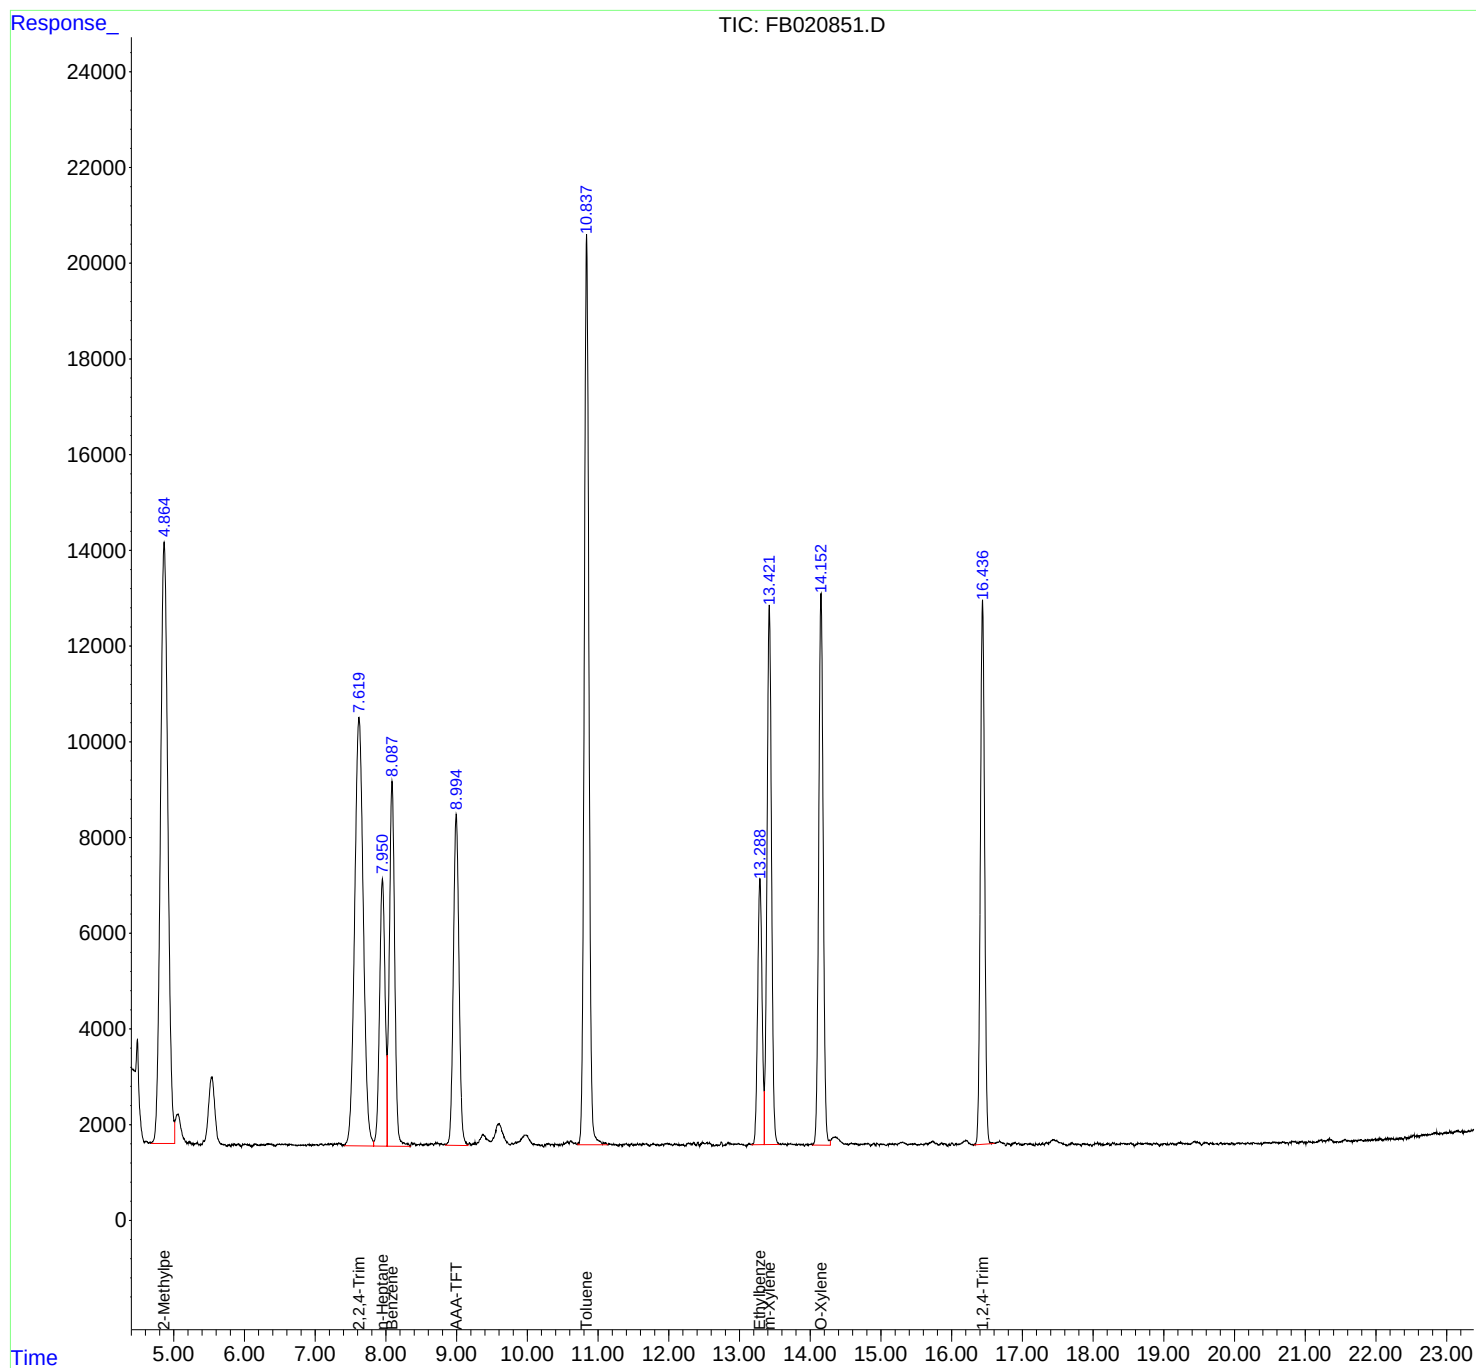

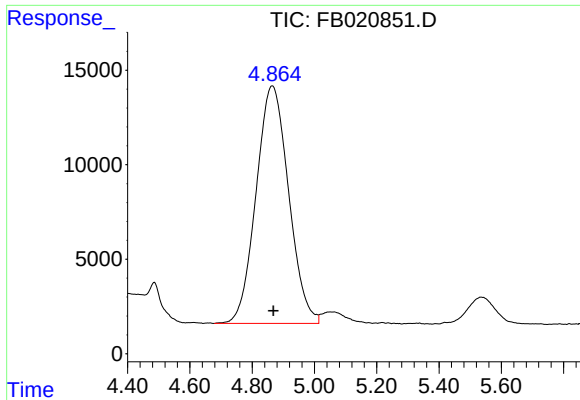


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: -0.004 min
Response: 912292
Conc: 25.91 ng/ml

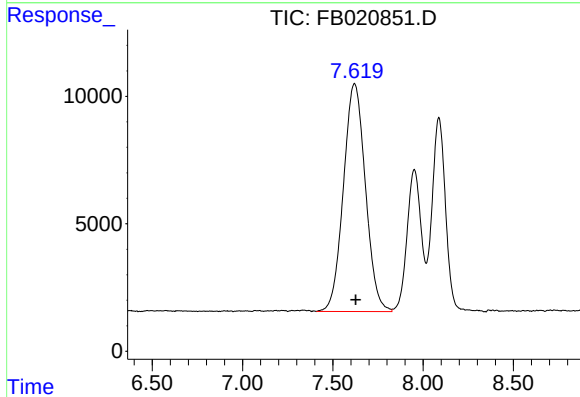


#2 2,2,4-Trimethylpentane

R.T.: 7.620 min
Delta R.T.: -0.006 min
Response: 757660
Conc: 25.41 ng/ml

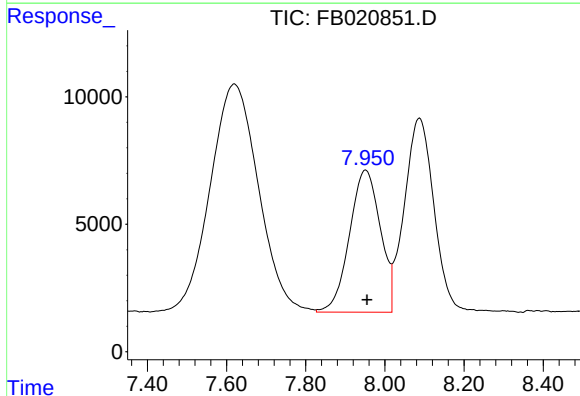


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: -0.004 min
Response: 301814
Conc: 7.69 ng/ml

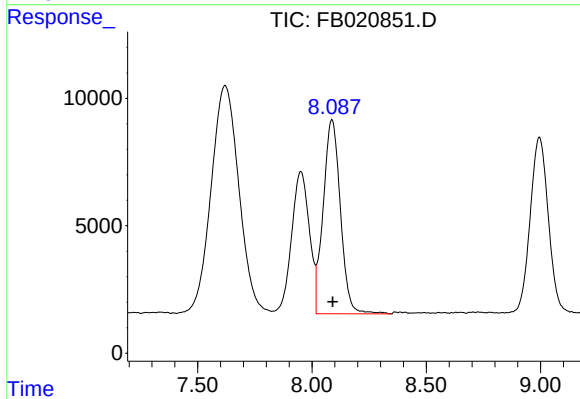


#4 Benzene

R.T.: 8.088 min
Delta R.T.: -0.004 min
Response: 398990
Conc: 9.71 ng/ml

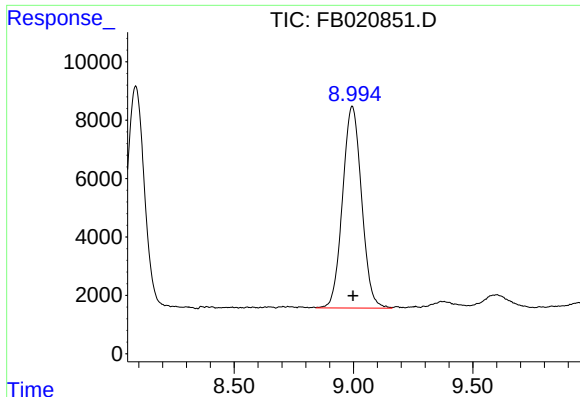


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: -0.004 min
Response: 381811
Conc: 20.70 ng/ml

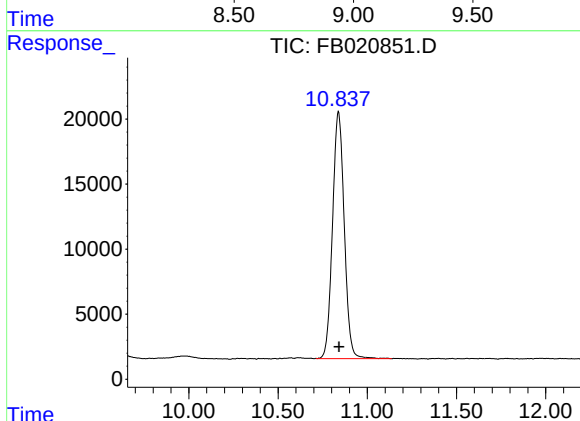


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.004 min
Response: 869498
Conc: 28.78 ng/ml

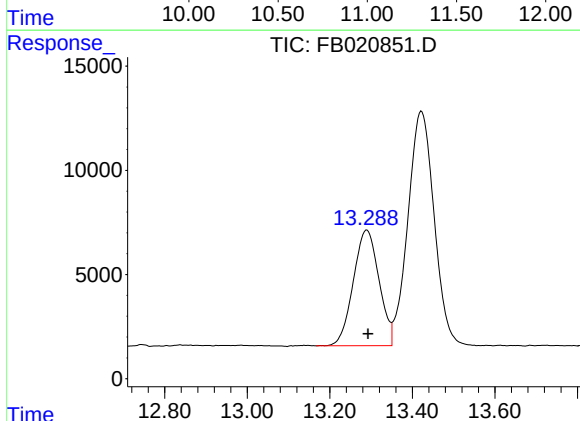


#7 Ethylbenzene

R.T.: 13.290 min
Delta R.T.: -0.003 min
Response: 239753
Conc: 9.37 ng/ml

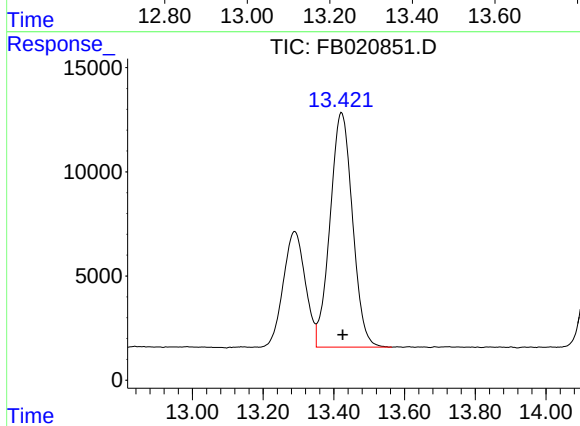


#8 m-Xylene

R.T.: 13.422 min
Delta R.T.: -0.003 min
Response: 496261
Conc: 18.78 ng/ml

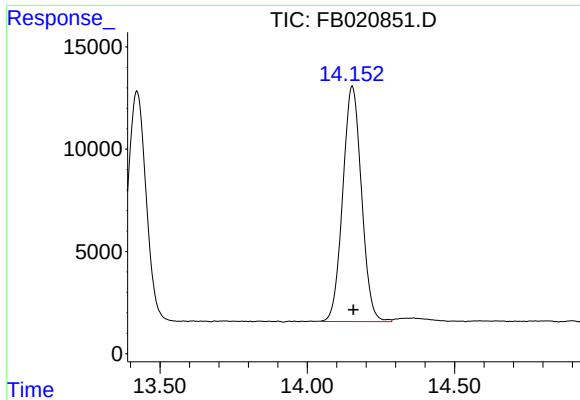

#9 O-Xylene

R.T.: 14.153 min
Delta R.T.: -0.003 min
Response: 509728
Conc: 18.83 ng/ml

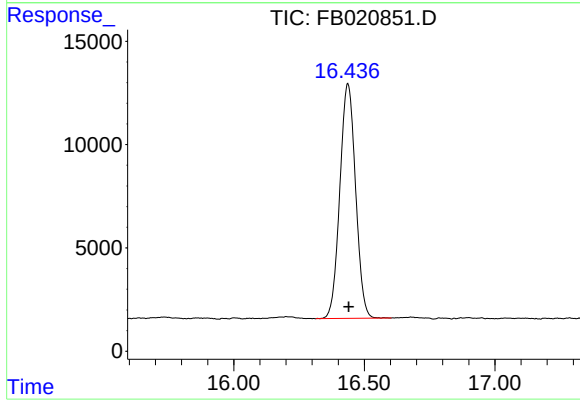

#10 1,2,4-Trimethylbenzene

R.T.: 16.438 min
Delta R.T.: -0.003 min
Response: 475408
Conc: 18.20 ng/ml