

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042519\
 Data File : FB020852.D
 Signal(s) : FID2B.CH
 Acq On : 25 Apr 2019 13:25
 Operator : MJ/SJ
 Sample : K2203-19MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 26 00:33:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.995	378960	20.546 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.864	901686	25.613 ng/ml
2) t	2,2,4-Trimethylpentane	7.619	742446	24.903 ng/ml
3) t	n-Heptane	7.951	289239	7.368 ng/ml
4) t	Benzene	8.087	390089	9.497 ng/ml
6) t	Toluene	10.838	846391	28.011 ng/ml
7) t	Ethylbenzene	13.289	240133	9.387 ng/ml
8) t	m-Xylene	13.422	491310	18.590 ng/ml
9) t	O-Xylene	14.153	502111	18.547 ng/ml
10) t	1,2,4-Trimethylbenzene	16.437	474662	18.167 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042519\
Data File : FB020852.D
Signal(s) : FID2B.CH
Acq On : 25 Apr 2019 13:25
Operator : MJ/SJ
Sample : K2203-19MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 26 00:33:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

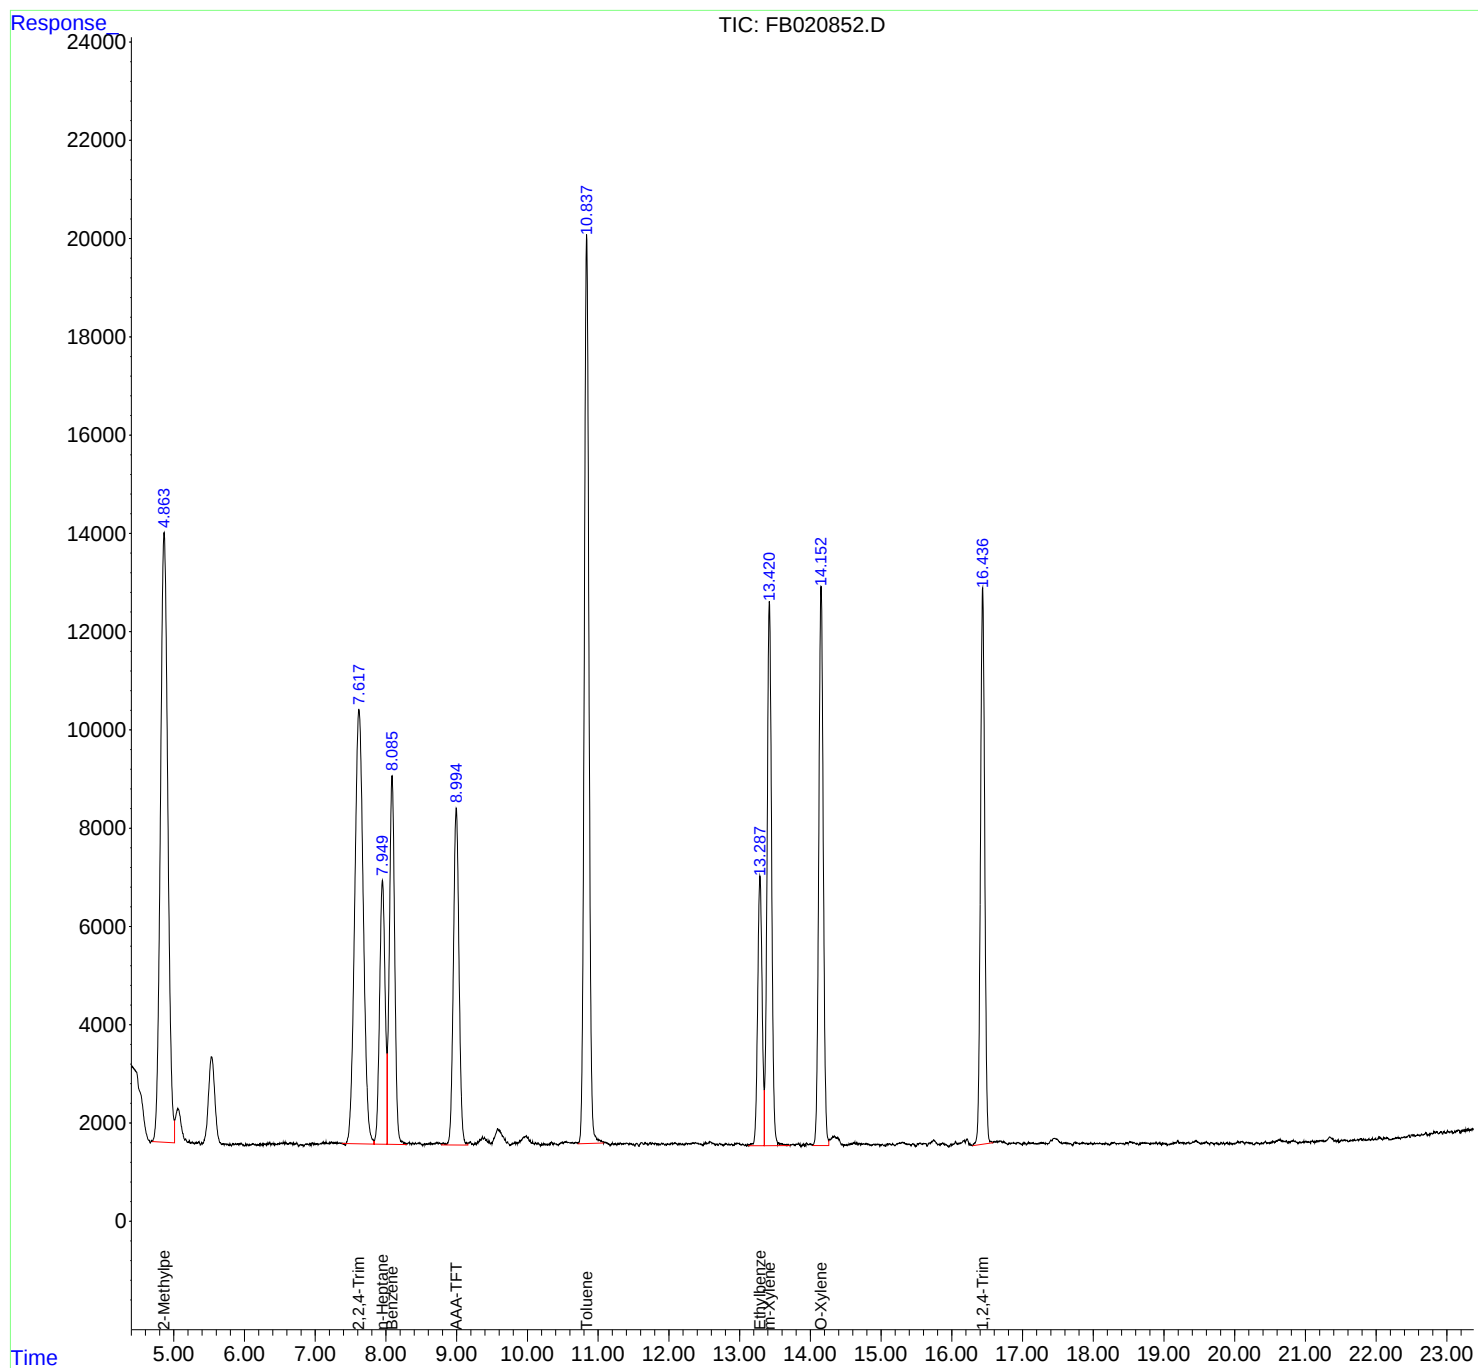

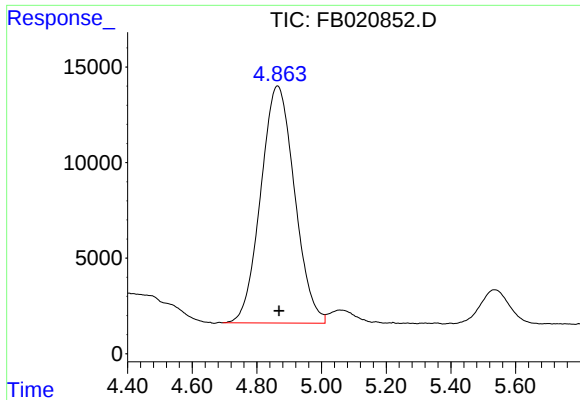


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: -0.005 min
Response: 901686
Conc: 25.61 ng/ml

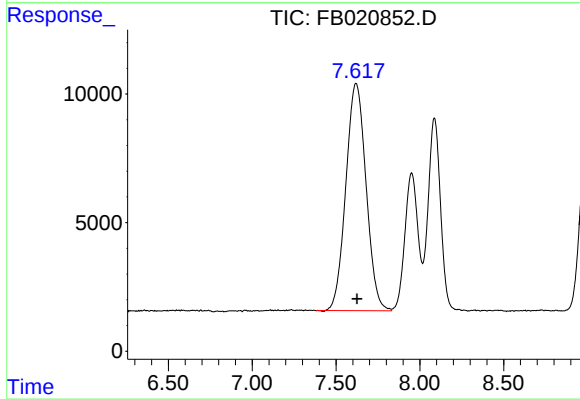


#2 2,2,4-Trimethylpentane

R.T.: 7.619 min
Delta R.T.: -0.007 min
Response: 742446
Conc: 24.90 ng/ml

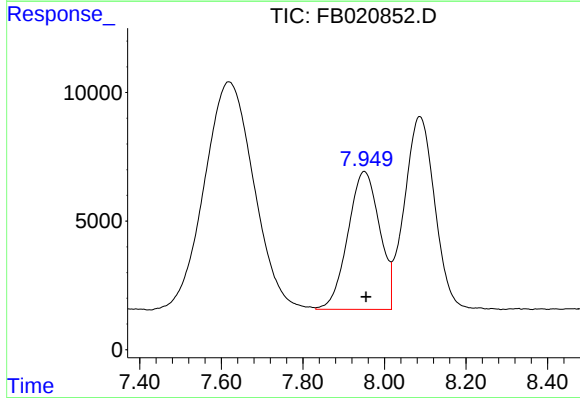


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.004 min
Response: 289239
Conc: 7.37 ng/ml

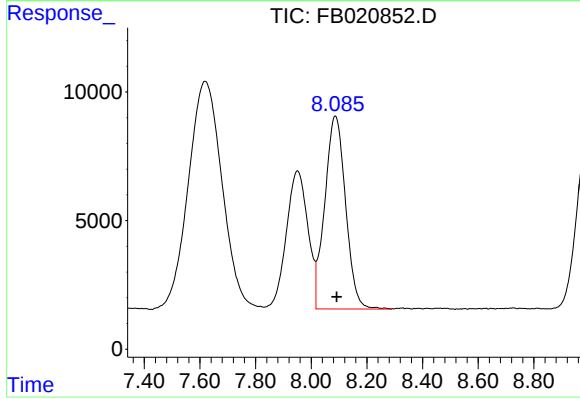


#4 Benzene

R.T.: 8.087 min
Delta R.T.: -0.004 min
Response: 390089
Conc: 9.50 ng/ml

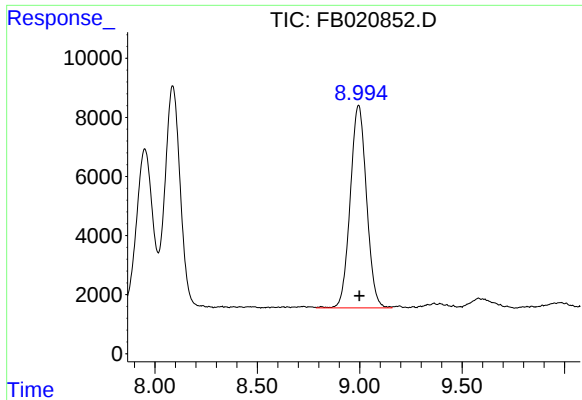


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: -0.004 min
Response: 378960
Conc: 20.55 ng/ml

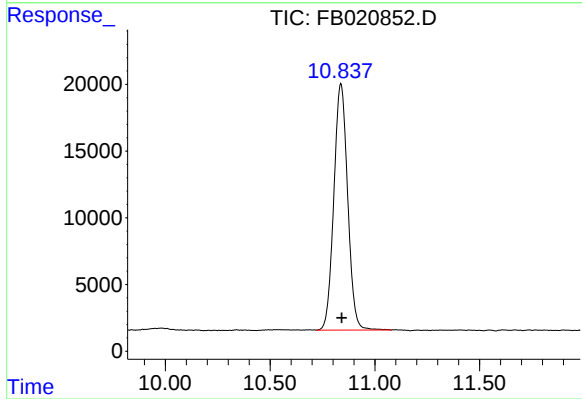


#6 Toluene

R.T.: 10.838 min
Delta R.T.: -0.004 min
Response: 846391
Conc: 28.01 ng/ml

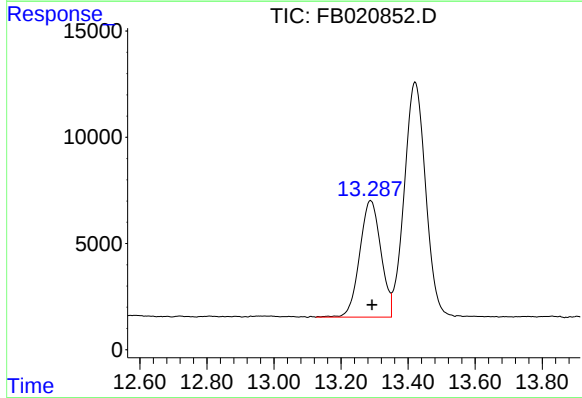


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.004 min
Response: 240133
Conc: 9.39 ng/ml

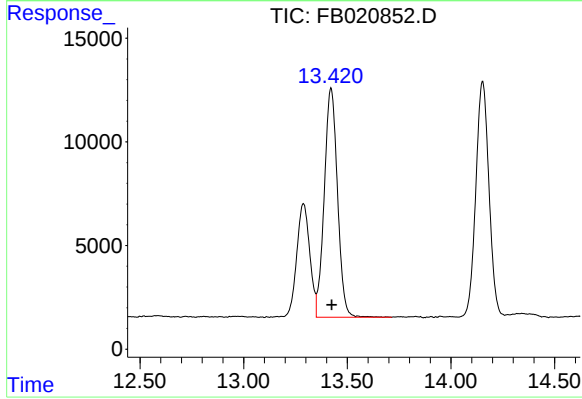


#8 m-Xylene

R.T.: 13.422 min
Delta R.T.: -0.004 min
Response: 491310
Conc: 18.59 ng/ml

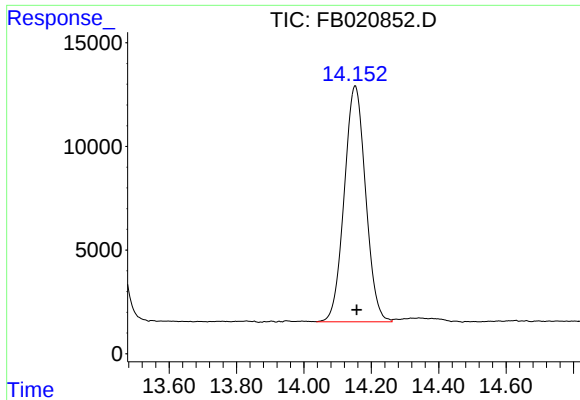

#9 O-Xylene

R.T.: 14.153 min
Delta R.T.: -0.004 min
Response: 502111
Conc: 18.55 ng/ml

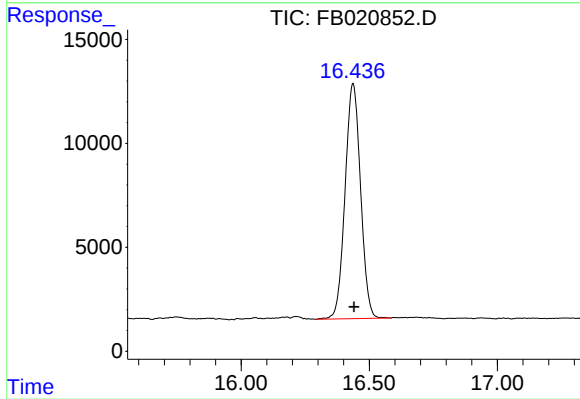

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min
Delta R.T.: -0.003 min
Response: 474662
Conc: 18.17 ng/ml