

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042524\
 Data File : FB030701.D
 Signal(s) : FID2B.CH
 Acq On : 25 Apr 2024 11:56
 Operator : YP/AJ
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 26 06:42:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
 Quant Title :
 QLast Update : Wed Apr 10 11:39:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	432842	30.287 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.435	68650	4.085 ng/ml
3) t n-Heptane	7.762	78449	4.300 ng/ml
4) t Benzene	7.889	78944	3.704 ng/ml
6) t Toluene	10.619	388794	18.835 ng/ml
7) t Ethylbenzene	13.055	95956	5.002 ng/ml
8) t m-Xylene	13.186	413293	21.648 ng/ml
9) t O-Xylene	13.917	200817	10.758 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	402582	21.684 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042524\
Data File : FB030701.D
Signal(s) : FID2B.CH
Acq On : 25 Apr 2024 11:56
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 26 06:42:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
Quant Title :
QLast Update : Wed Apr 10 11:39:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

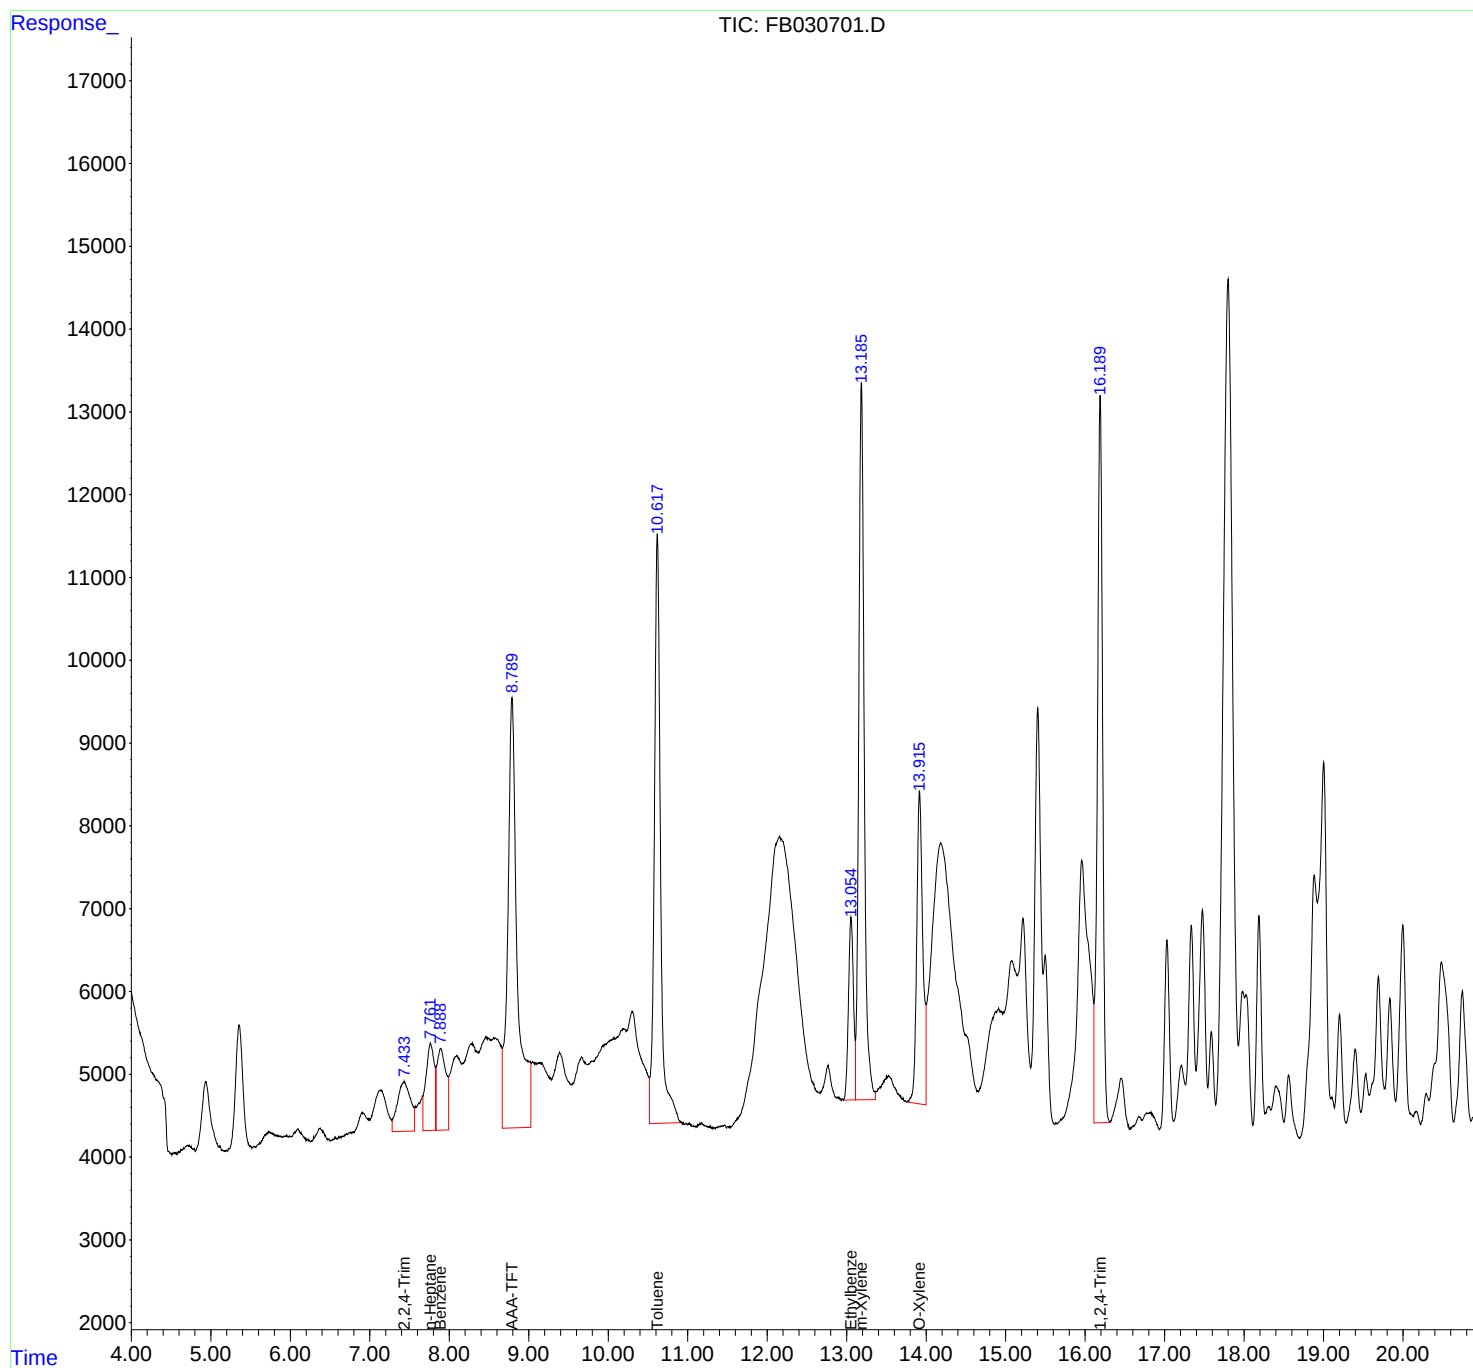


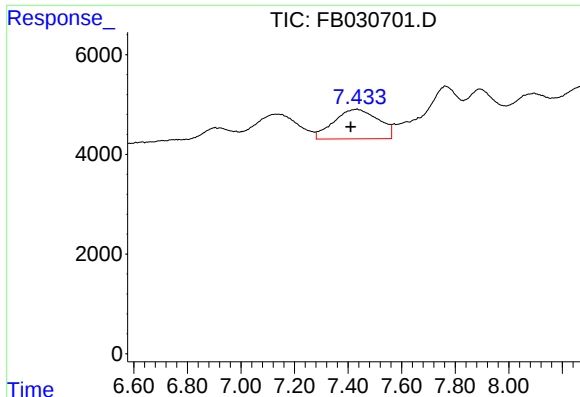

#2 2,2,4-Trimethylpentane


R.T.: 7.435 min
Delta R.T.: 0.024 min
Response: 68650
Conc: 4.09 ng/ml

Instrument :
FID_B
ClientSampleId :

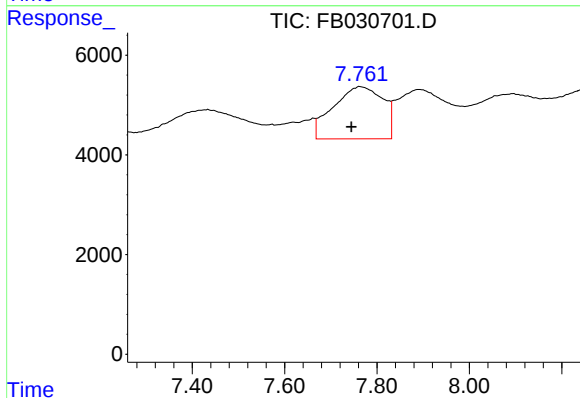


#3 n-Heptane

R.T.: 7.762 min
Delta R.T.: 0.018 min
Response: 78449
Conc: 4.30 ng/ml

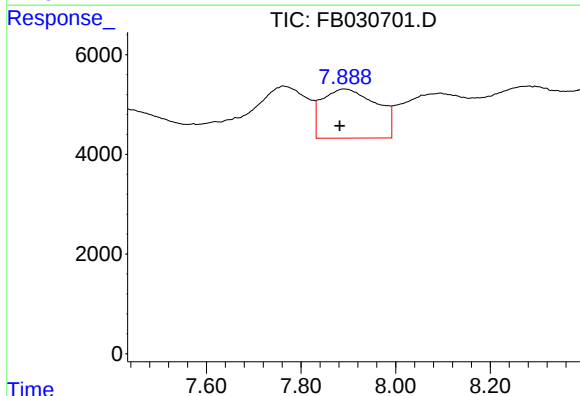


#4 Benzene

R.T.: 7.889 min
Delta R.T.: 0.008 min
Response: 78944
Conc: 3.70 ng/ml

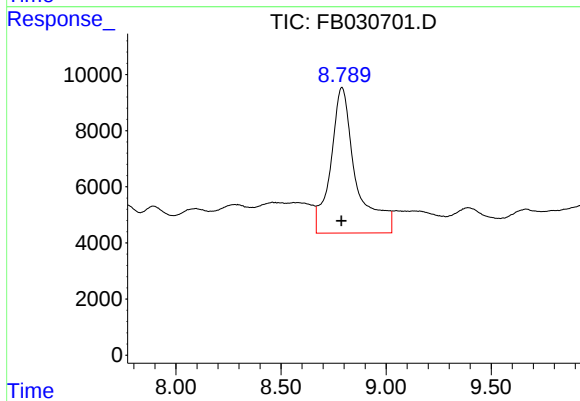

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.004 min
Response: 432842
Conc: 30.29 ng/ml

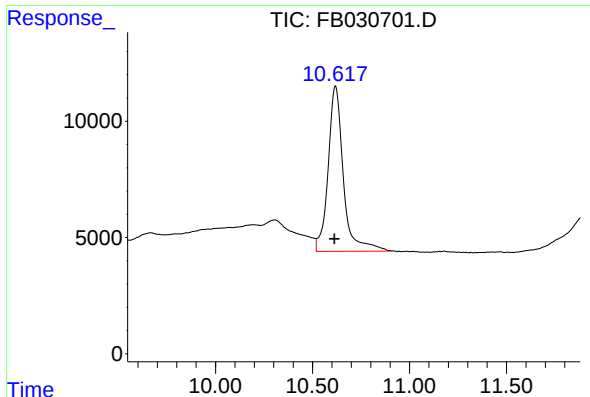

#6 Toluene


R.T.: 10.619 min
Delta R.T.: 0.005 min
Response: 388794
Conc: 18.83 ng/ml

Instrument :
FID_B
ClientSampleId :

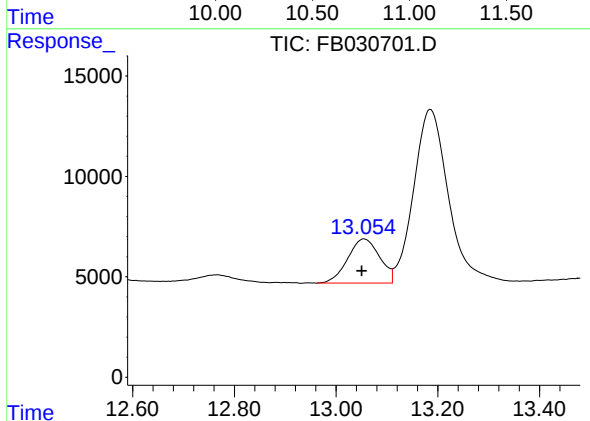


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.005 min
Response: 95956
Conc: 5.00 ng/ml

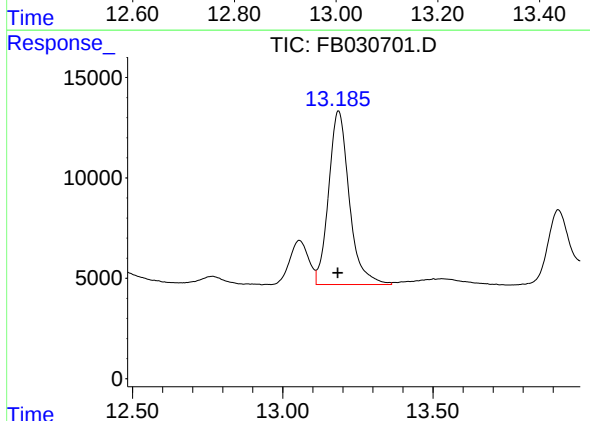


#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: 0.003 min
Response: 413293
Conc: 21.65 ng/ml

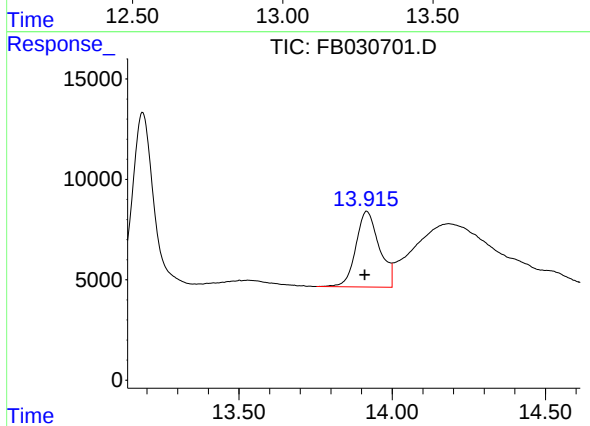

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.007 min
Response: 200817
Conc: 10.76 ng/ml

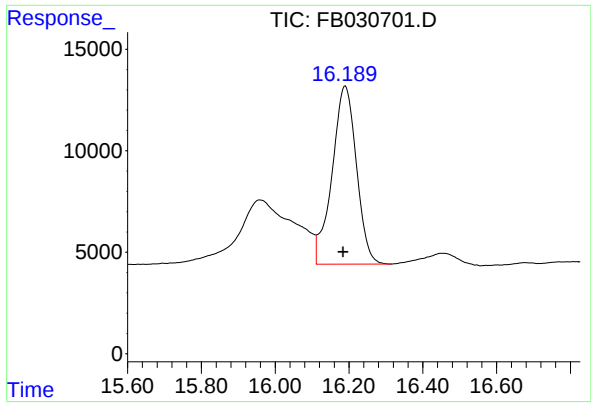

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.006 min
Response: 402582
Conc: 21.68 ng/ml

Instrument :

FID_B

ClientSampleId :