

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042525\
 Data File : FB031645.D
 Signal(s) : FID2B.CH
 Acq On : 25 Apr 2025 9:42
 Operator : YP/AJ
 Sample : VBF0425S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 VBF0425S1

Integration File: Calibration.e
 Quant Time: Apr 26 01:28:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
 Quant Title :
 QLast Update : Wed Apr 23 13:48:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	435450	18.988 ng/ml
Target Compounds			
6) t Toluene	10.627	11165	0.280 ng/ml
7) t Ethylbenzene	13.055	4601	0.129 ng/ml
8) t m-Xylene	13.187	11056	0.283 ng/ml
9) t O-Xylene	13.912	14039	0.381 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	20516	0.761 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042525\
Data File : FB031645.D
Signal(s) : FID2B.CH
Acq On : 25 Apr 2025 9:42
Operator : YP/AJ
Sample : VBF0425S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0425S1

Integration File: Calibration.e
Quant Time: Apr 26 01:28:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

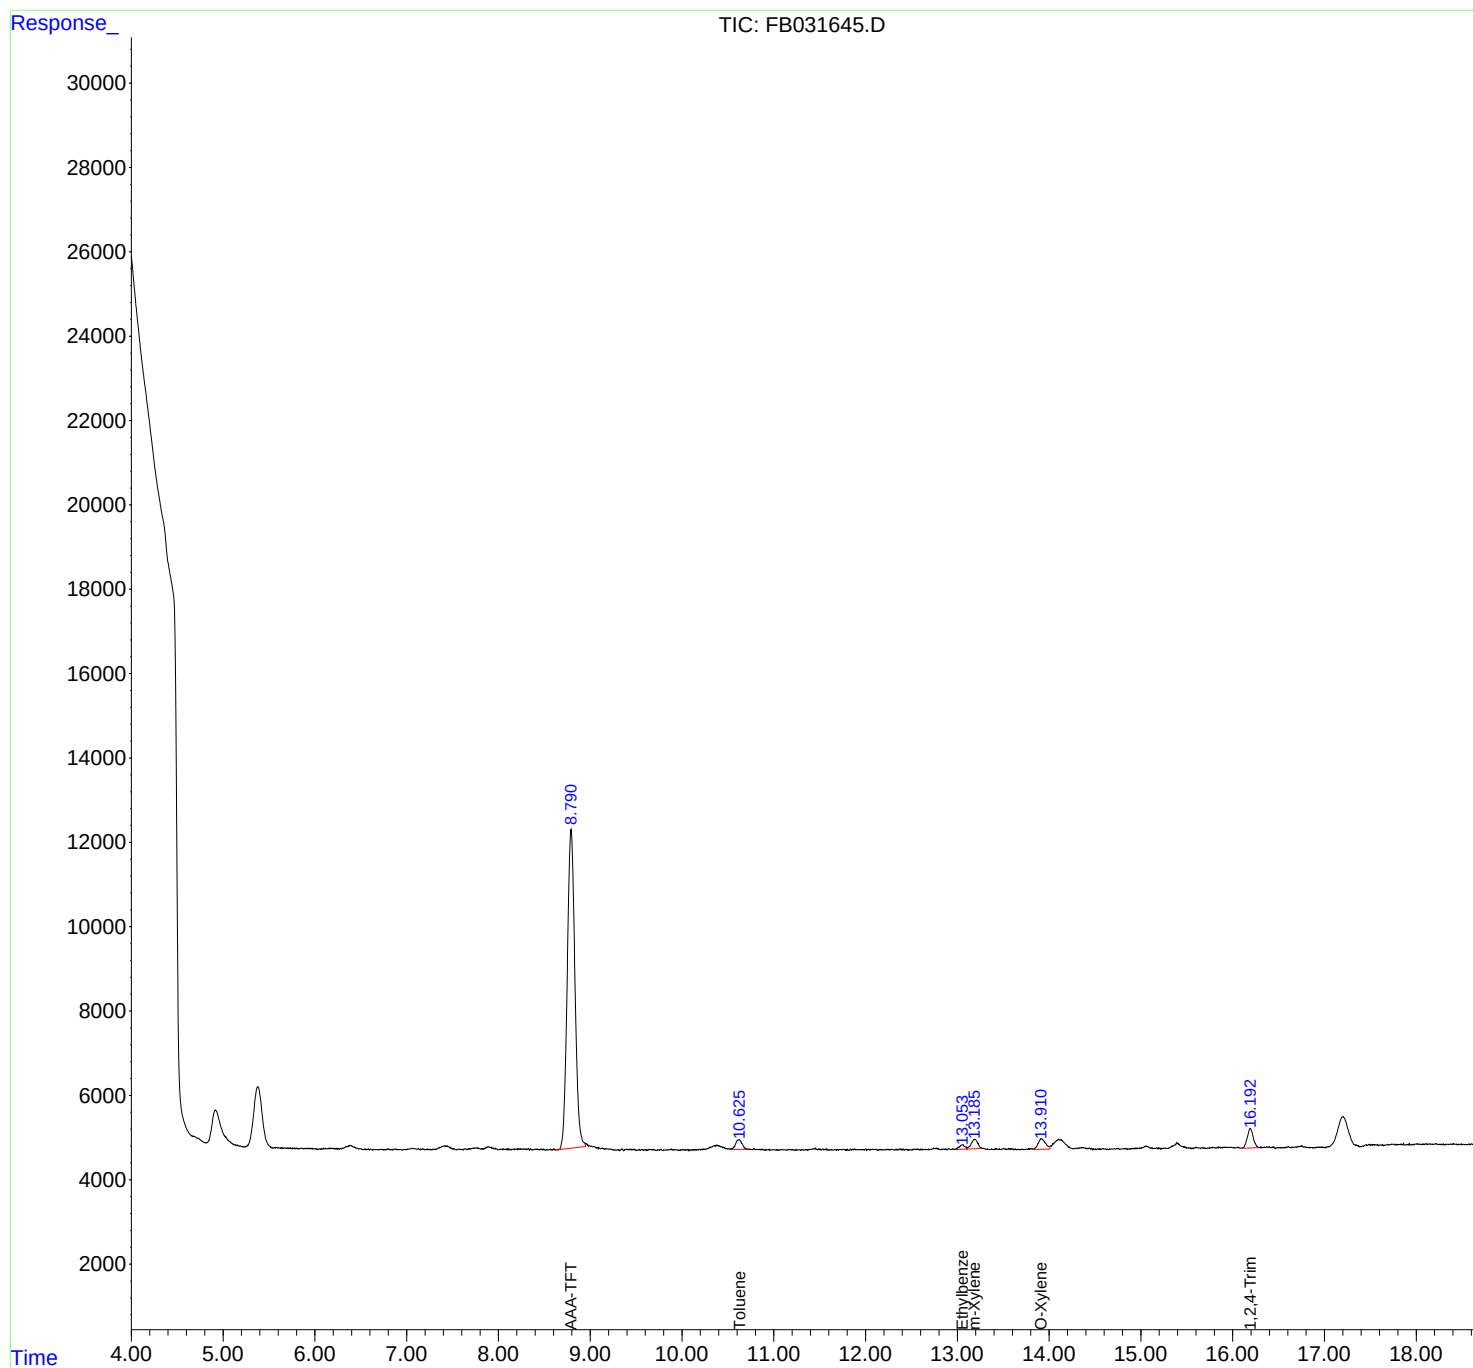


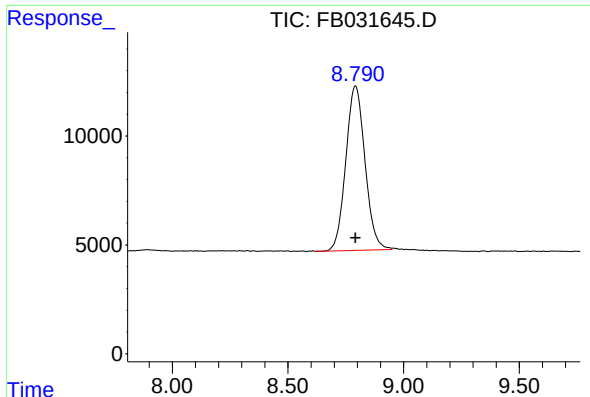

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 435450
Conc: 18.99 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0425S1

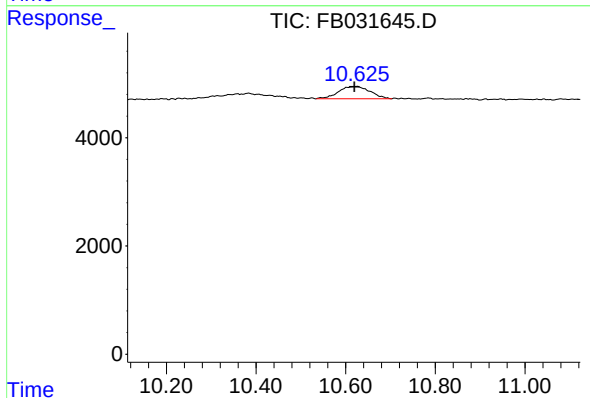


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.007 min
Response: 11165
Conc: 0.28 ng/ml

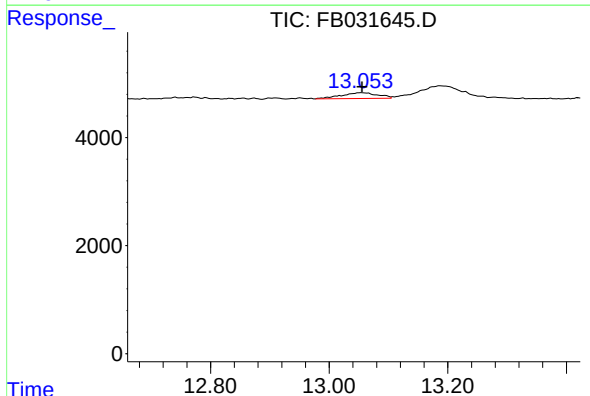


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 4601
Conc: 0.13 ng/ml

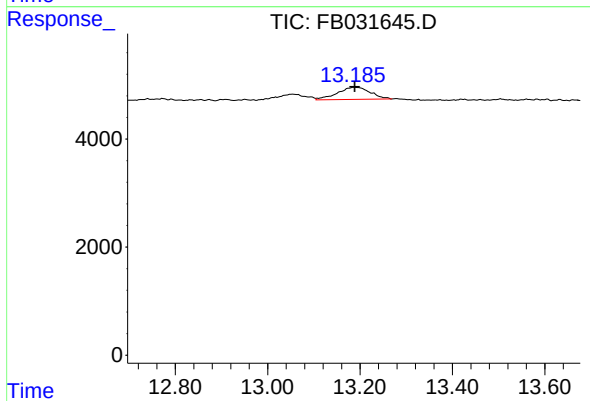

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.002 min
Response: 11056
Conc: 0.28 ng/ml

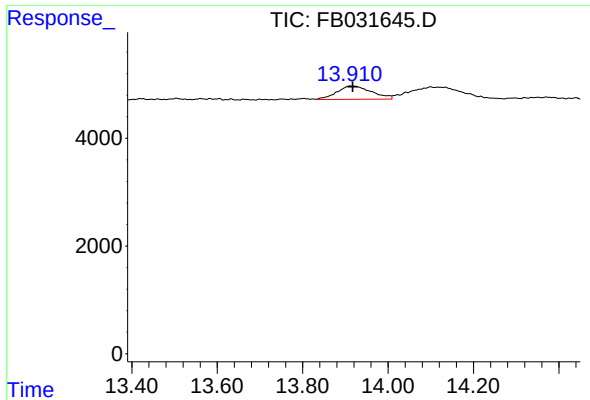

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.005 min
Response: 14039
Conc: 0.38 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0425S1

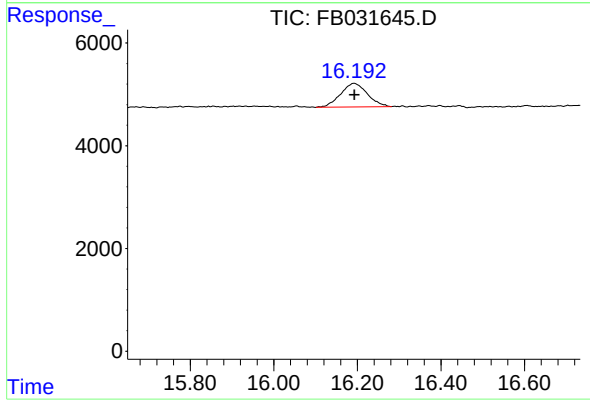

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 20516
Conc: 0.76 ng/ml