

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042525\
 Data File : FB031647.D
 Signal(s) : FID2B.CH
 Acq On : 25 Apr 2025 10:37
 Operator : YP/AJ
 Sample : BSF0425S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0425S1

Integration File: Calibration.e
 Quant Time: Apr 26 01:28:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
 Quant Title :
 QLast Update : Wed Apr 23 13:48:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	554206	24.166 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.724	692440	31.161 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	1130107	33.084 ng/ml
3) t n-Heptane	7.755	322015	10.469 ng/ml
4) t Benzene	7.895	445046	10.883 ng/ml
6) t Toluene	10.621	1323232	33.212 ng/ml
7) t Ethylbenzene	13.056	396945	11.108 ng/ml
8) t m-Xylene	13.190	869991	22.266 ng/ml
9) t O-Xylene	13.918	817973	22.201 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	605970	22.465 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042525\
Data File : FB031647.D
Signal(s) : FID2B.CH
Acq On : 25 Apr 2025 10:37
Operator : YP/AJ
Sample : BSF0425S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0425S1

Integration File: Calibration.e
Quant Time: Apr 26 01:28:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

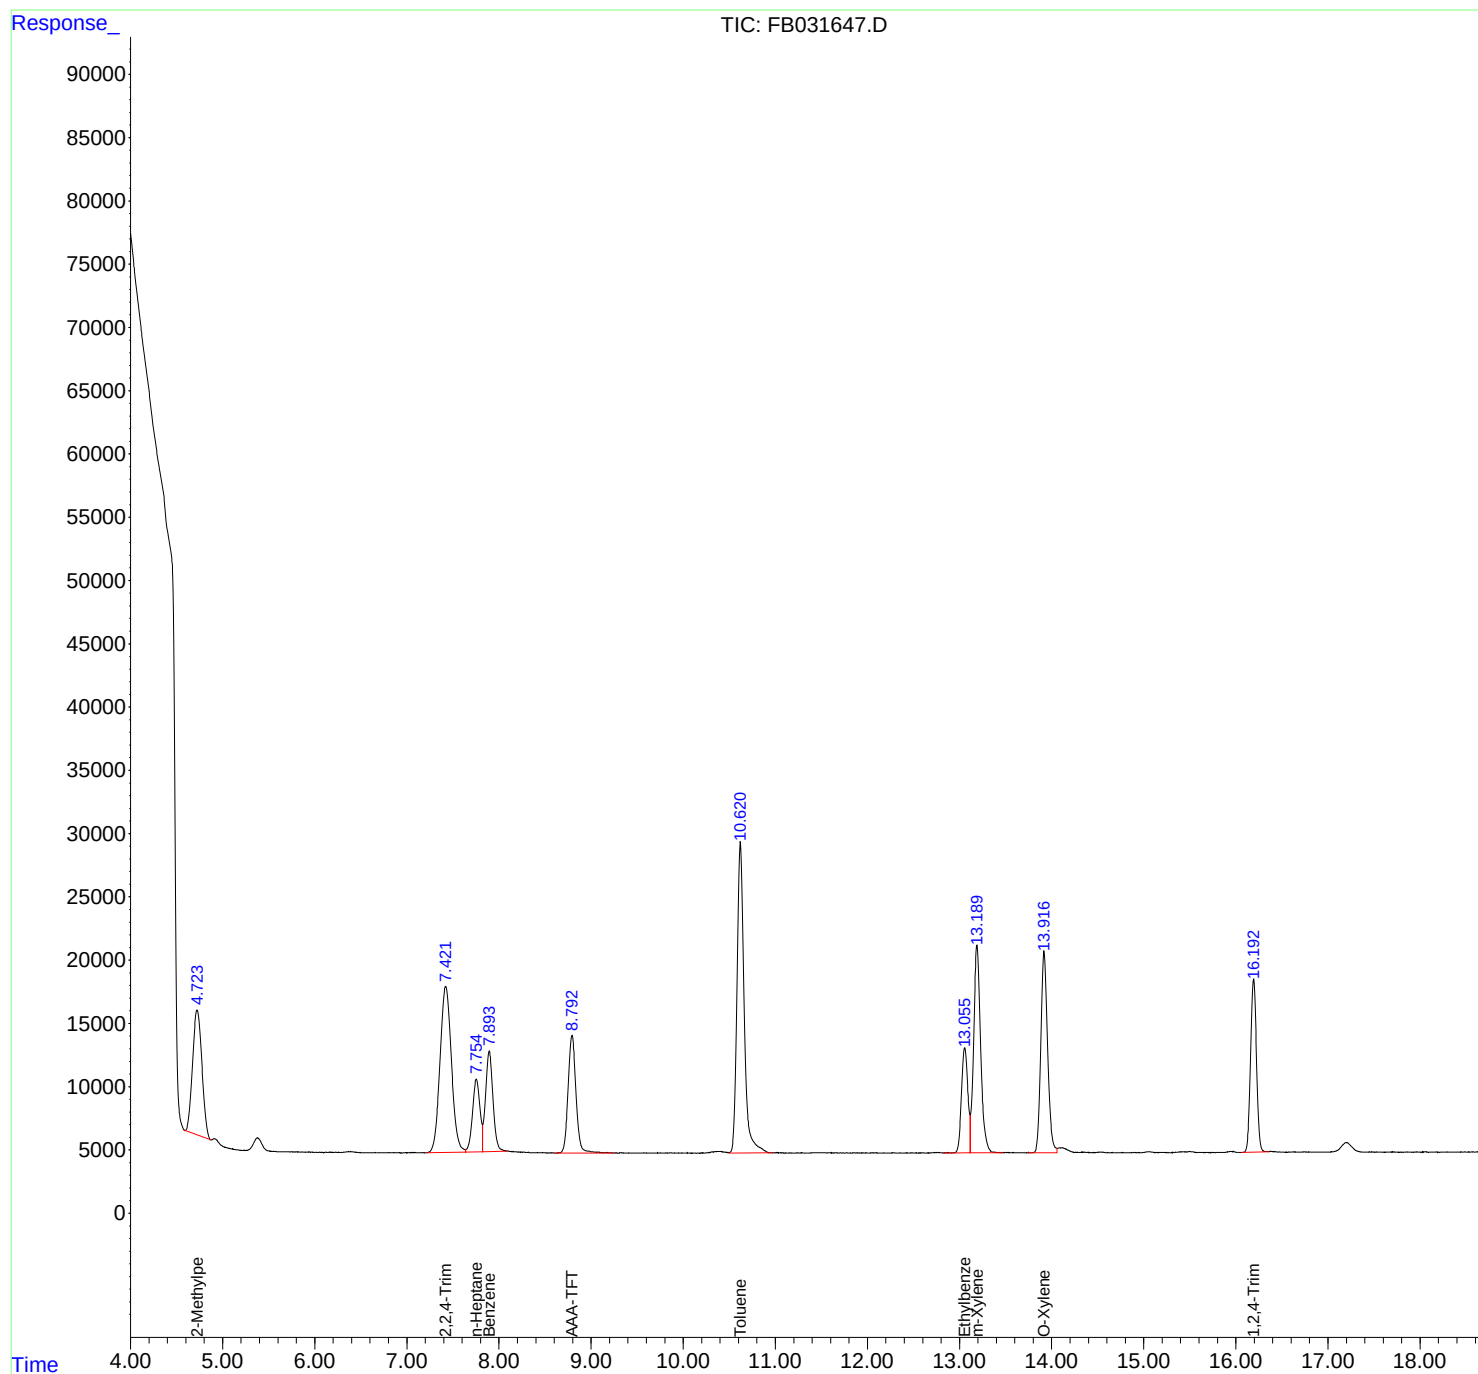


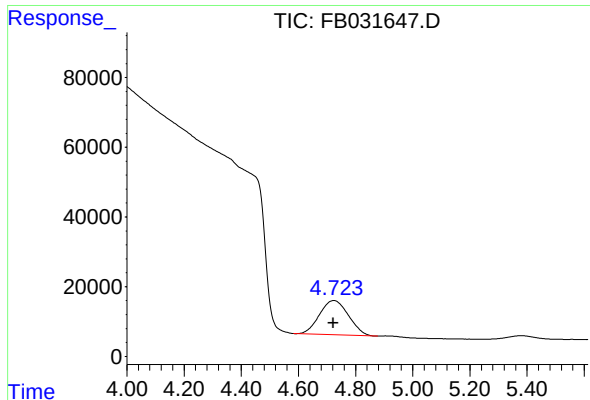

#1 2-Methylpentane


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 692440
Conc: 31.16 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0425S1

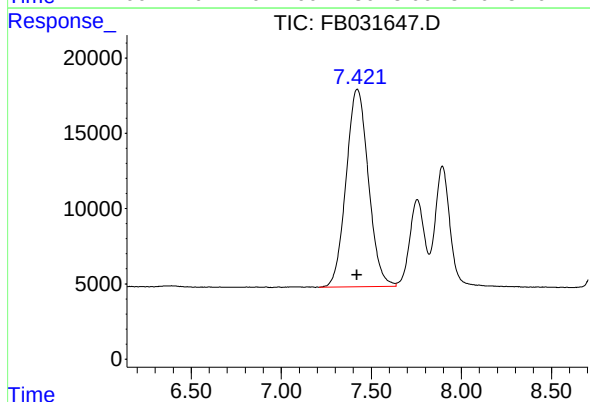


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.002 min
Response: 1130107
Conc: 33.08 ng/ml

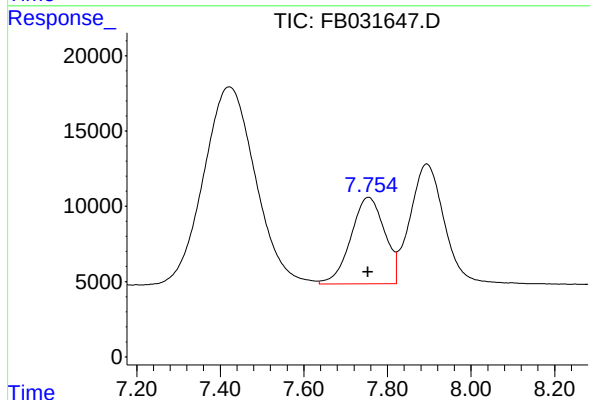


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.002 min
Response: 322015
Conc: 10.47 ng/ml

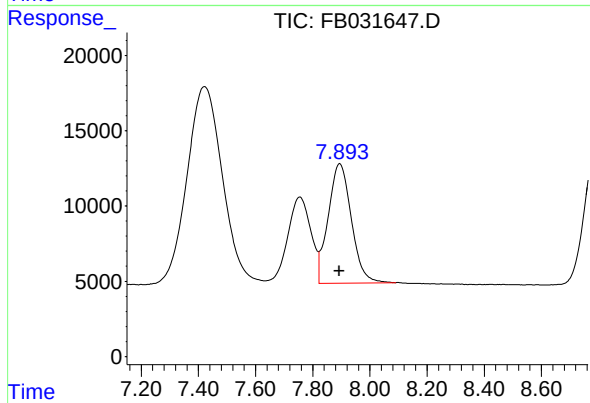

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.001 min
Response: 445046
Conc: 10.88 ng/ml

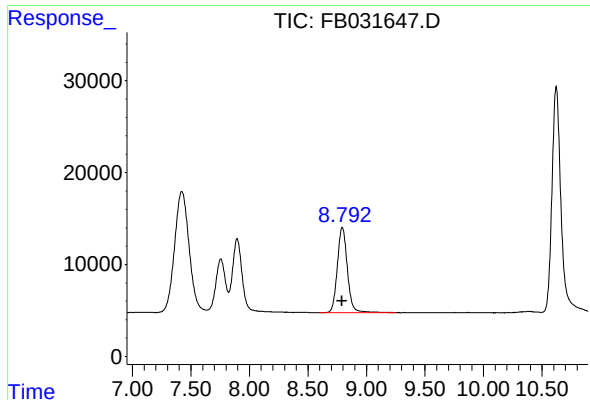

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.001 min
Response: 554206
Conc: 24.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0425S1

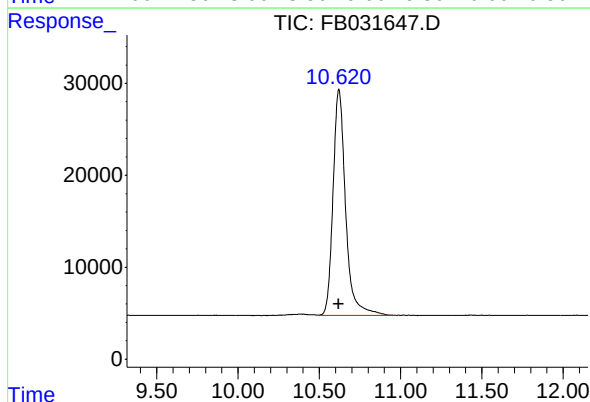


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.001 min
Response: 1323232
Conc: 33.21 ng/ml

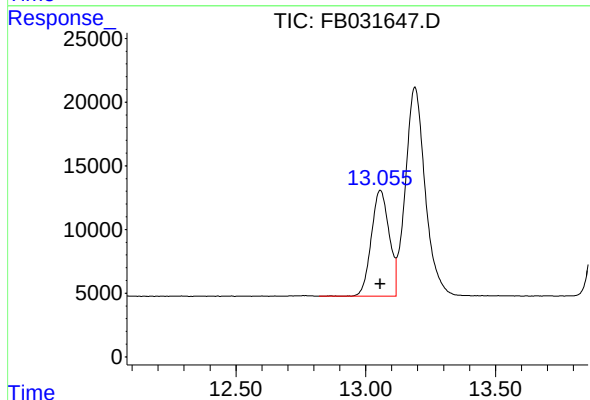


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 396945
Conc: 11.11 ng/ml

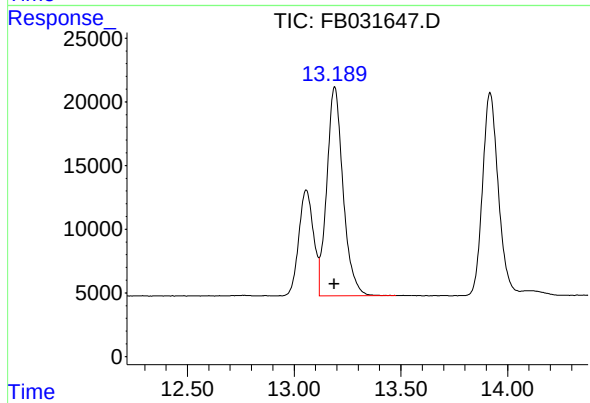

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 869991
Conc: 22.27 ng/ml

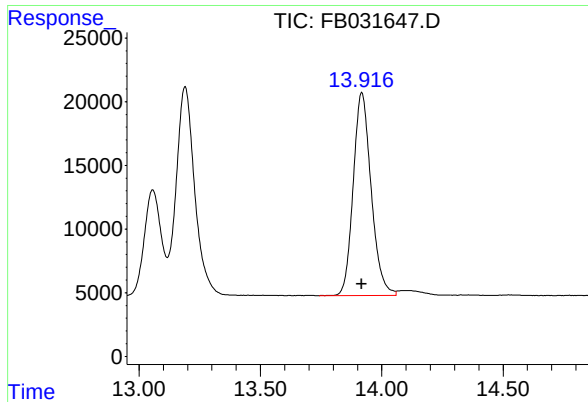

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 817973
Conc: 22.20 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0425S1

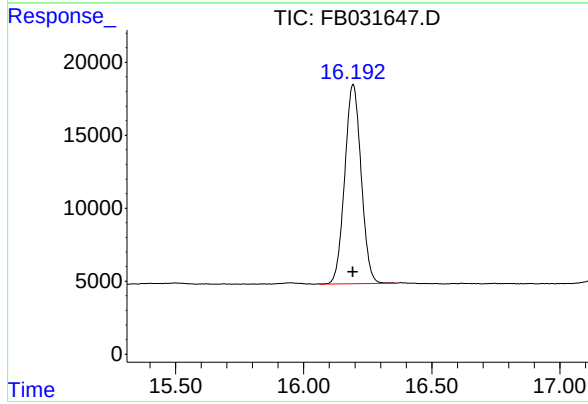

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 605970
Conc: 22.46 ng/ml