

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042525\
 Data File : FB031651.D
 Signal(s) : FID2B.CH
 Acq On : 25 Apr 2025 12:43
 Operator : YP/AJ
 Sample : BSF0425S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0425S2

Integration File: Calibration.e
 Quant Time: Apr 26 01:29:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
 Quant Title :
 QLast Update : Wed Apr 23 13:48:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	488811	21.315 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.724	682445	30.711 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	1076405	31.512 ng/ml
3) t n-Heptane	7.756	323454	10.516 ng/ml
4) t Benzene	7.895	434140	10.617 ng/ml
6) t Toluene	10.622	1261093	31.653 ng/ml
7) t Ethylbenzene	13.057	377988	10.578 ng/ml
8) t m-Xylene	13.191	827634	21.182 ng/ml
9) t O-Xylene	13.918	780090	21.173 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	572559	21.226 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042525\
Data File : FB031651.D
Signal(s) : FID2B.CH
Acq On : 25 Apr 2025 12:43
Operator : YP/AJ
Sample : BSF0425S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0425S2

Integration File: Calibration.e
Quant Time: Apr 26 01:29:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

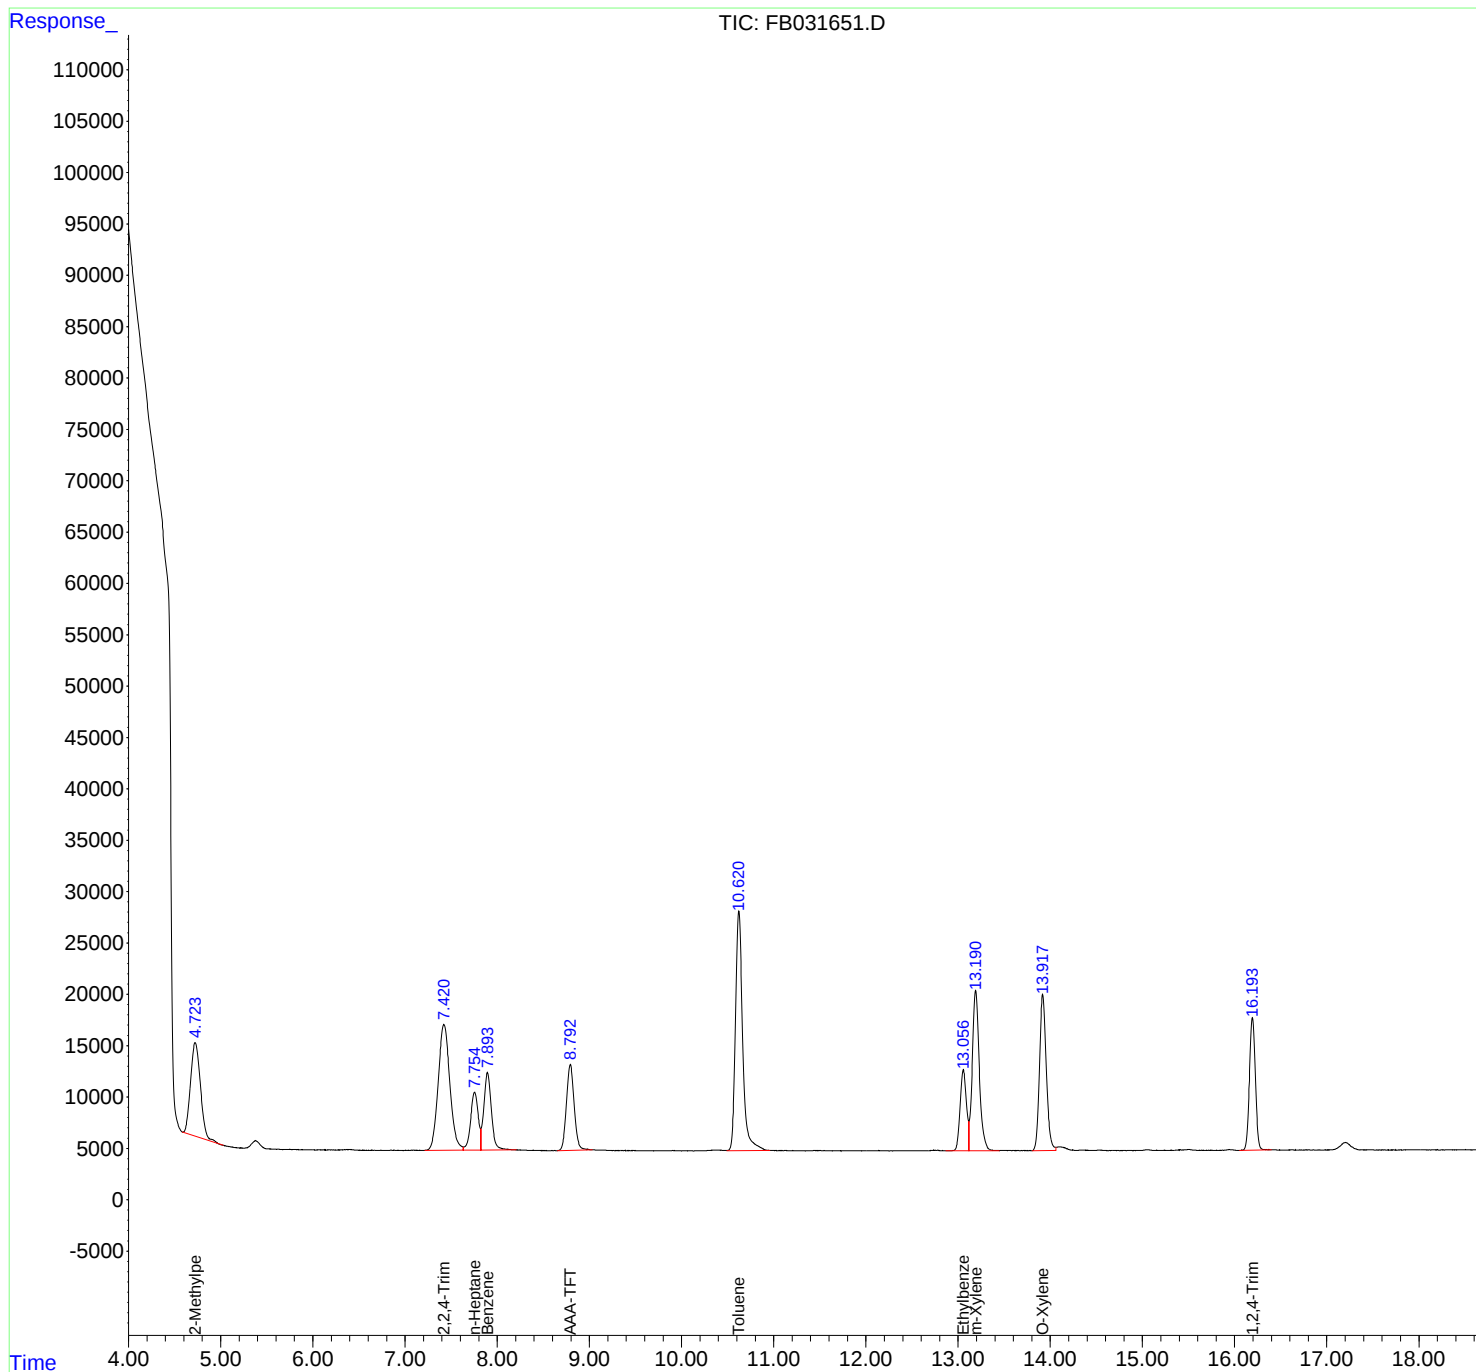


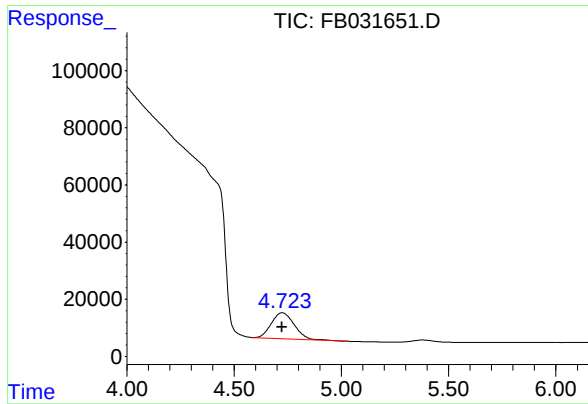

#1 2-Methylpentane


R.T.: 4.724 min
Delta R.T.: 0.001 min
Response: 682445
Conc: 30.71 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0425S2

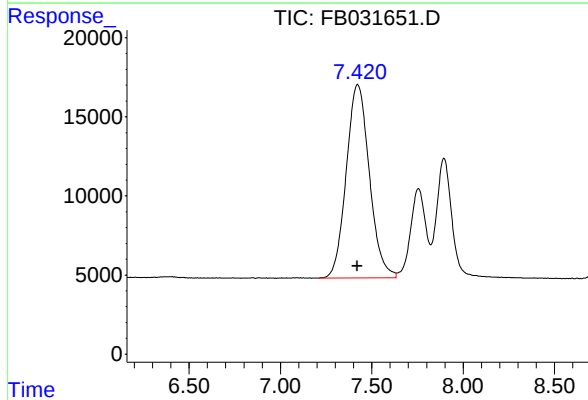


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.001 min
Response: 1076405
Conc: 31.51 ng/ml

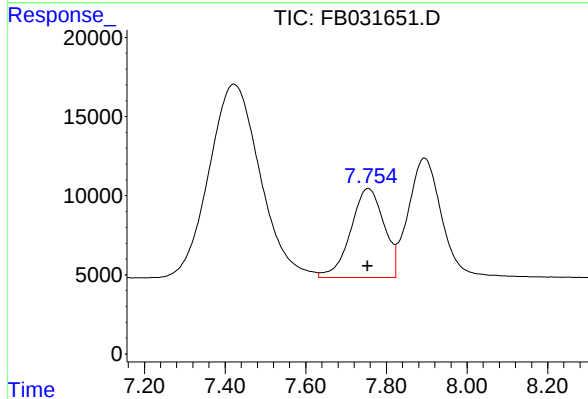


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.002 min
Response: 323454
Conc: 10.52 ng/ml

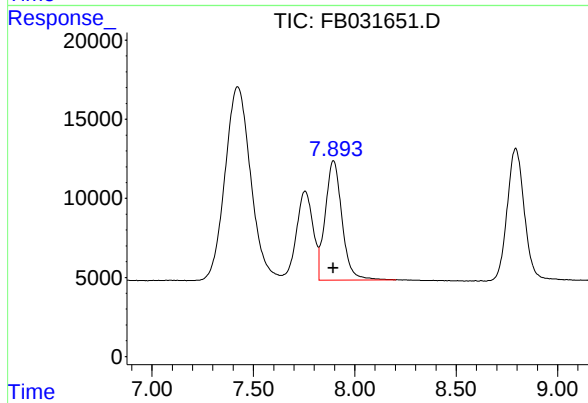

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.002 min
Response: 434140
Conc: 10.62 ng/ml

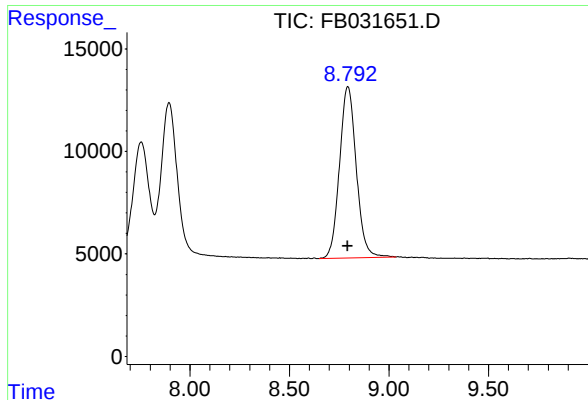

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 488811
Conc: 21.31 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0425S2

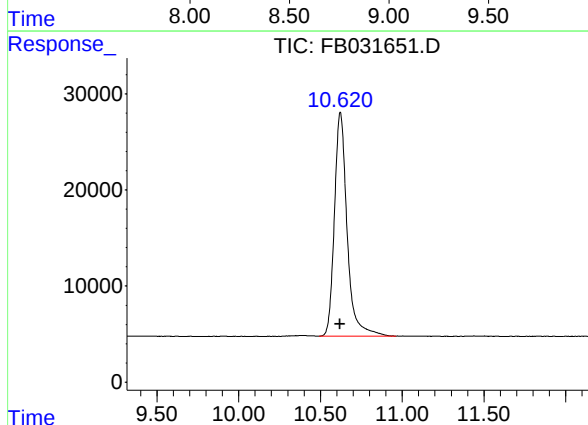


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 1261093
Conc: 31.65 ng/ml

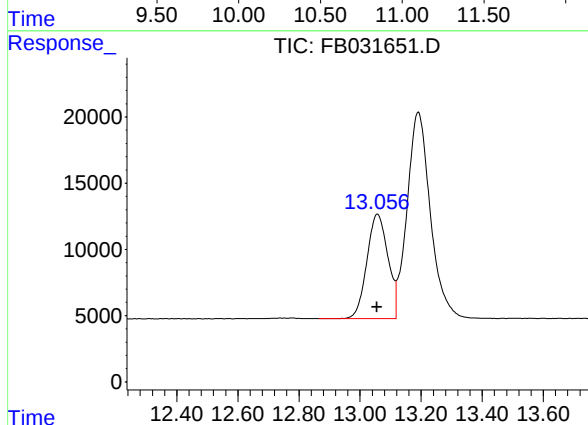


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.001 min
Response: 377988
Conc: 10.58 ng/ml

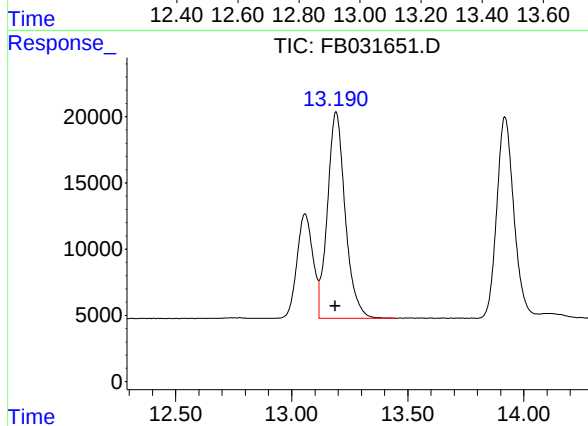

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 827634
Conc: 21.18 ng/ml

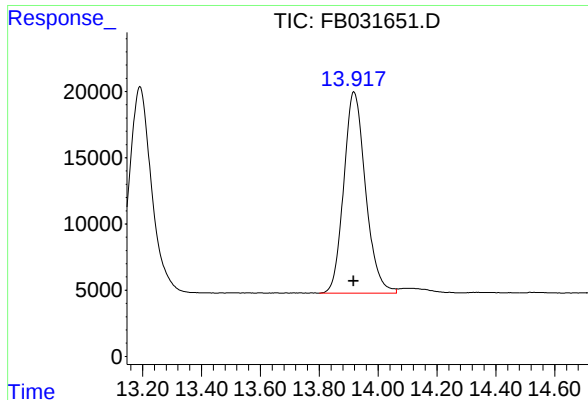

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.001 min
Response: 780090
Conc: 21.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0425S2

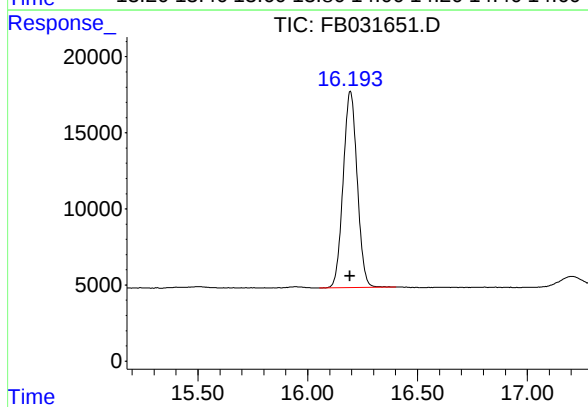

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 572559
Conc: 21.23 ng/ml