

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042619\
 Data File : FB020856.D
 Signal(s) : FID2B.CH
 Acq On : 26 Apr 2019 10:11
 Operator : MJ/SJ
 Sample : BSF0426S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 26 23:46:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.998	411535	22.312 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.866	1041641	29.589 ng/ml
2) t 2,2,4-Trimethylpentane	7.622	961273	32.243 ng/ml
3) t n-Heptane	7.954	389410	9.920 ng/ml
4) t Benzene	8.090	414401	10.089 ng/ml
6) t Toluene	10.841	929560	30.764 ng/ml
7) t Ethylbenzene	13.292	266179	10.405 ng/ml
8) t m-Xylene	13.425	556239	21.046 ng/ml
9) t O-Xylene	14.155	566115	20.911 ng/ml
10) t 1,2,4-Trimethylbenzene	16.440	555040	21.244 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042619\
Data File : FB020856.D
Signal(s) : FID2B.CH
Acq On : 26 Apr 2019 10:11
Operator : MJ/SJ
Sample : BSF0426S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 26 23:46:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

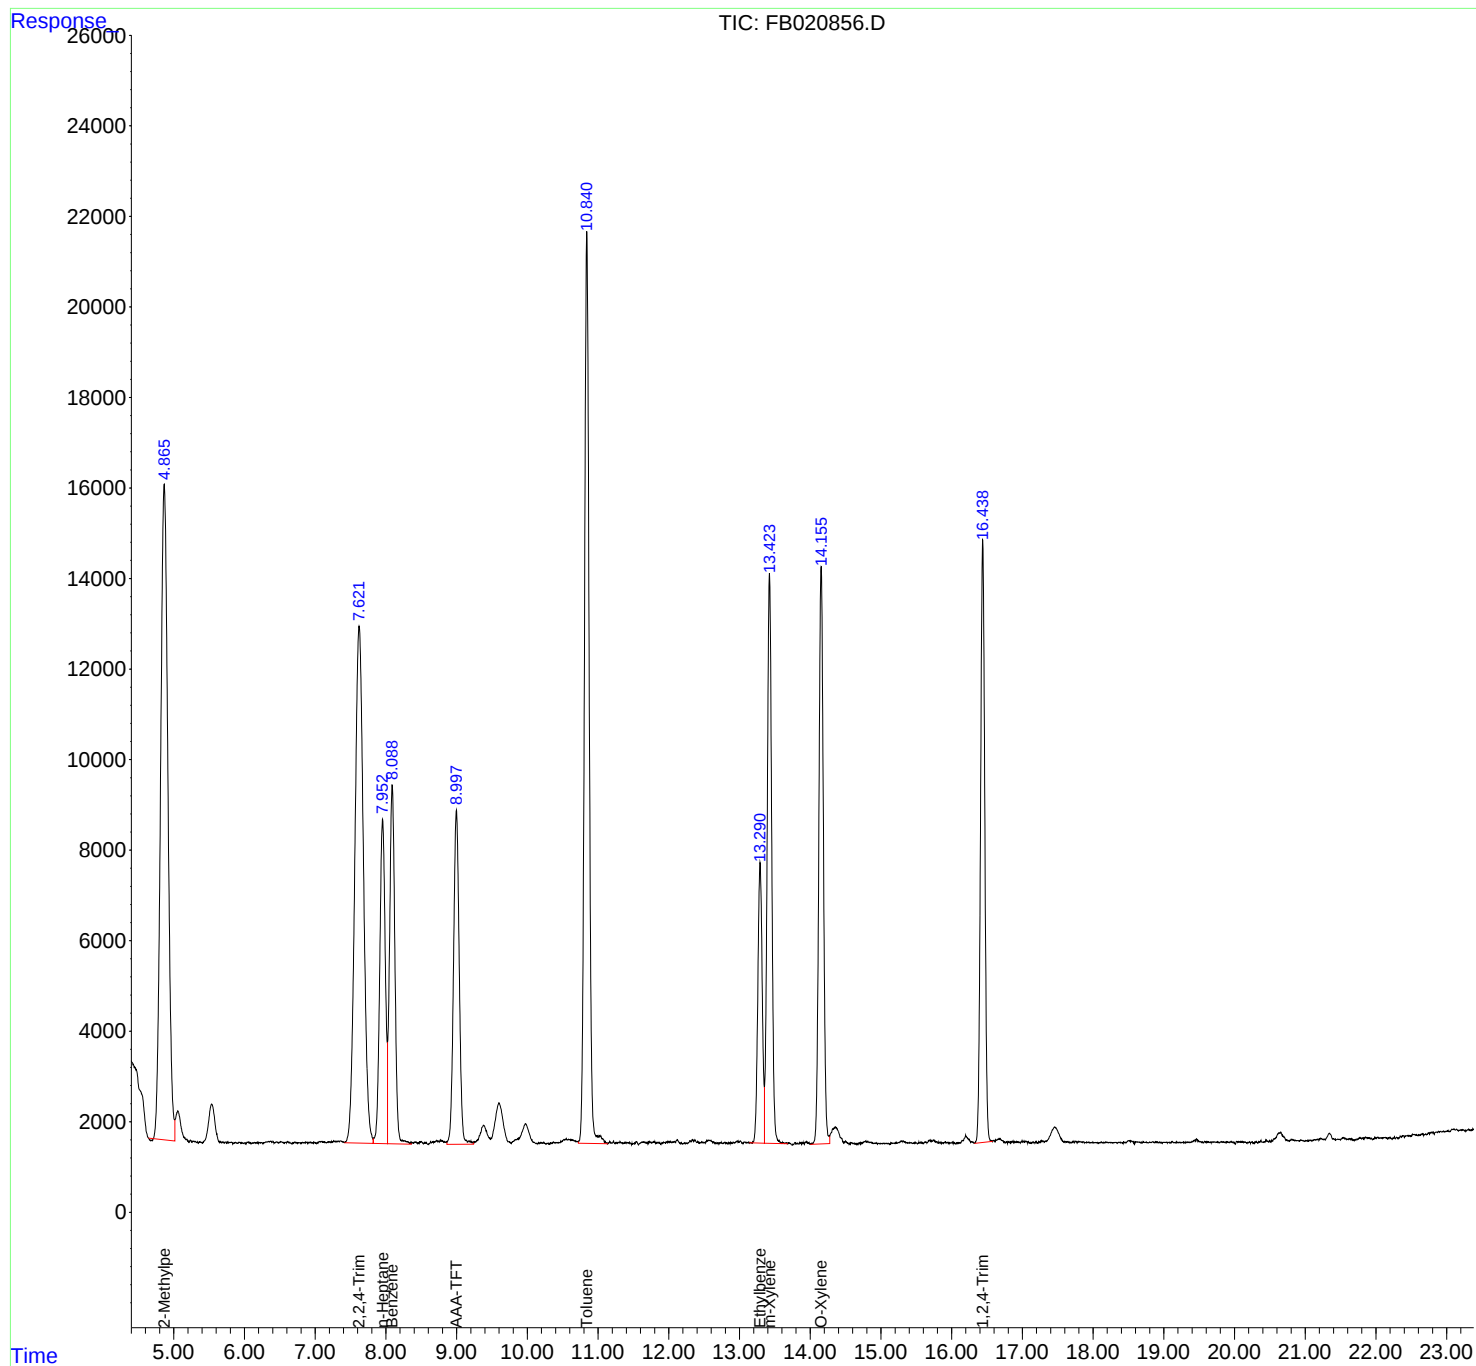

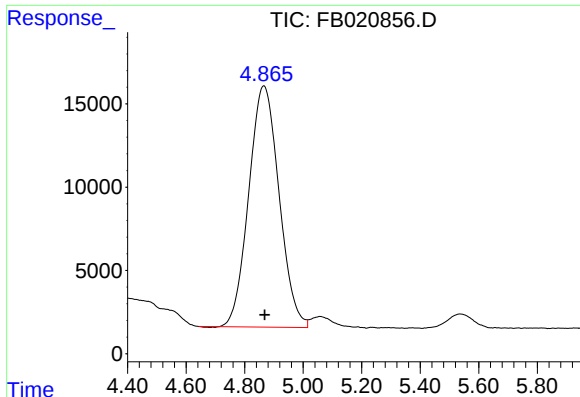


#1 2-Methylpentane

R.T.: 4.866 min
Delta R.T.: -0.003 min
Response: 1041641
Conc: 29.59 ng/ml

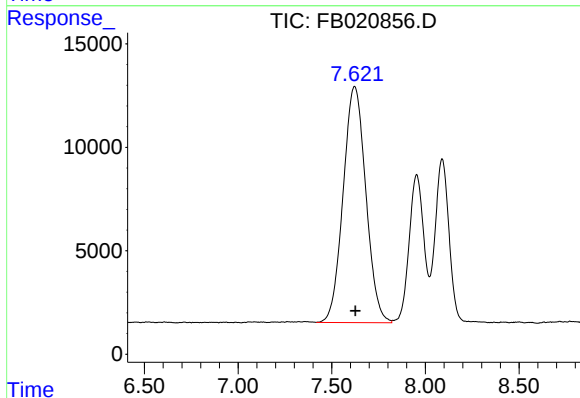


#2 2,2,4-Trimethylpentane

R.T.: 7.622 min
Delta R.T.: -0.004 min
Response: 961273
Conc: 32.24 ng/ml

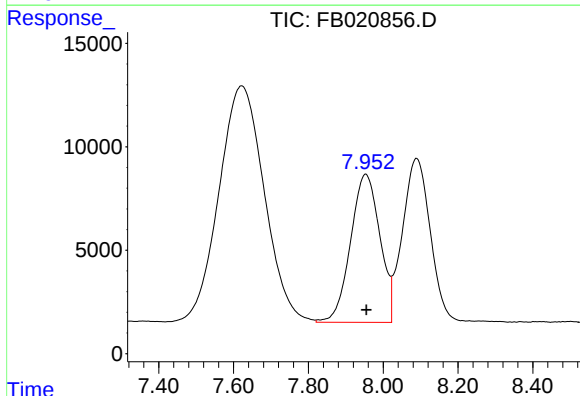


#3 n-Heptane

R.T.: 7.954 min
Delta R.T.: -0.001 min
Response: 389410
Conc: 9.92 ng/ml

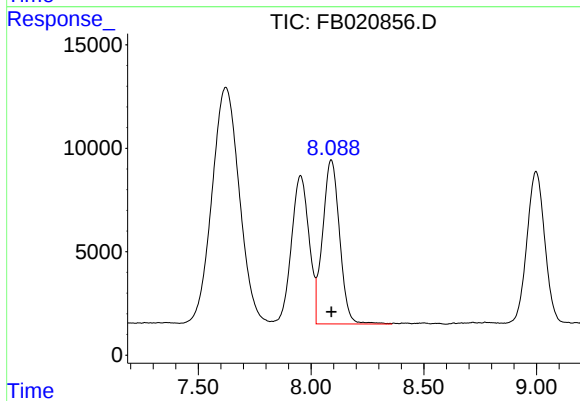


#4 Benzene

R.T.: 8.090 min
Delta R.T.: -0.001 min
Response: 414401
Conc: 10.09 ng/ml

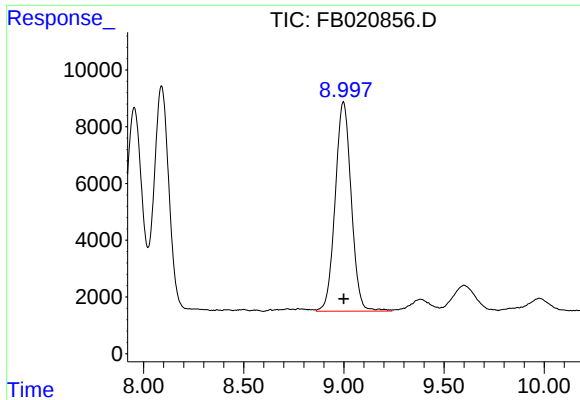


#5 AAA-TFT

R.T.: 8.998 min
 Delta R.T.: 0.000 min
 Response: 411535
 Conc: 22.31 ng/ml

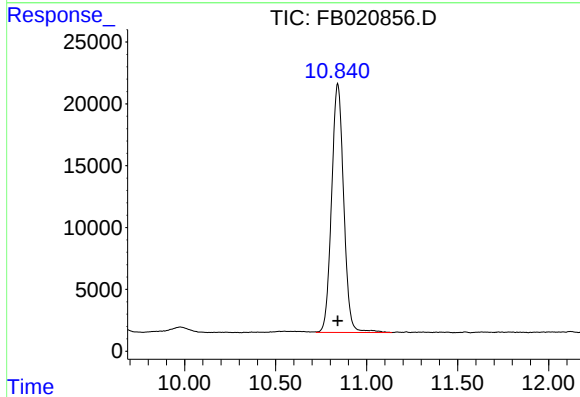


#6 Toluene

R.T.: 10.841 min
 Delta R.T.: 0.000 min
 Response: 929560
 Conc: 30.76 ng/ml

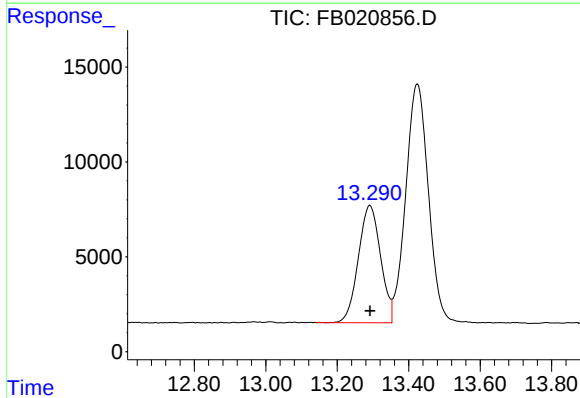


#7 Ethylbenzene

R.T.: 13.292 min
 Delta R.T.: 0.000 min
 Response: 266179
 Conc: 10.40 ng/ml

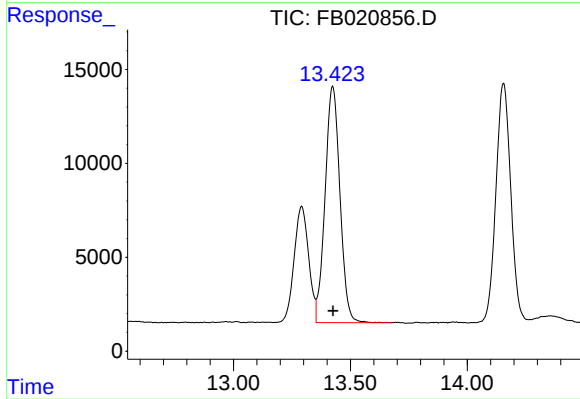

#8 m-Xylene

R.T.: 13.425 min
 Delta R.T.: 0.000 min
 Response: 556239
 Conc: 21.05 ng/ml

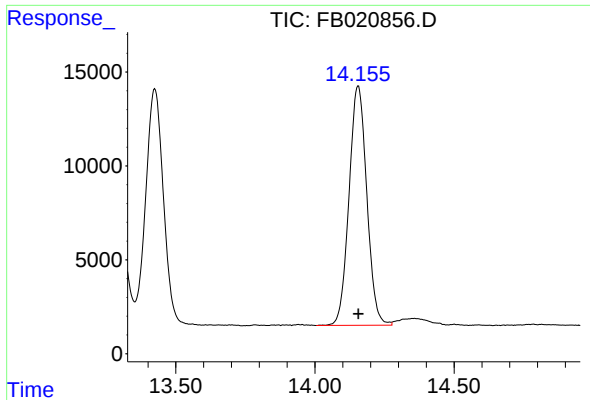


#9 O-Xylene

R.T.: 14.155 min

Delta R.T.: -0.001 min

Response: 566115

Conc: 20.91 ng/ml

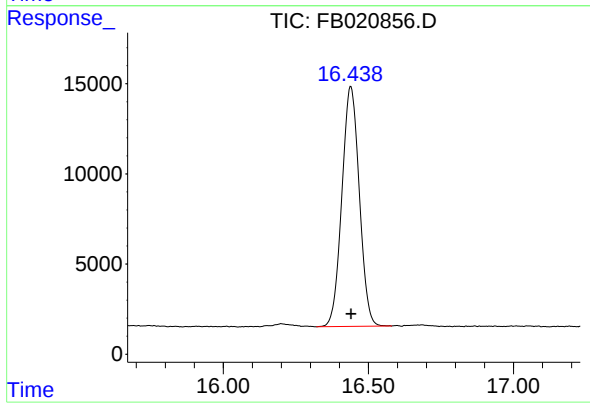

#10 1,2,4-Trimethylbenzene

R.T.: 16.440 min

Delta R.T.: 0.000 min

Response: 555040

Conc: 21.24 ng/ml