

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042624\
 Data File : FB030711.D
 Signal(s) : FID2B.CH
 Acq On : 26 Apr 2024 10:44
 Operator : YP/AJ
 Sample : BSF0426S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 27 02:58:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
 Quant Title :
 QLast Update : Wed Apr 10 11:39:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.785	245425	17.173 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	444782	27.163 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	473957	28.203 ng/ml
3) t n-Heptane	7.743	163873	8.983 ng/ml
4) t Benzene	7.880	205992	9.665 ng/ml
6) t Toluene	10.612	607530	29.431 ng/ml
7) t Ethylbenzene	13.048	187300	9.764 ng/ml
8) t m-Xylene	13.181	375965	19.693 ng/ml
9) t O-Xylene	13.908	358932	19.229 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	343553	18.505 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042624\
Data File : FB030711.D
Signal(s) : FID2B.CH
Acq On : 26 Apr 2024 10:44
Operator : YP/AJ
Sample : BSF0426S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 27 02:58:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
Quant Title :
QLast Update : Wed Apr 10 11:39:18 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

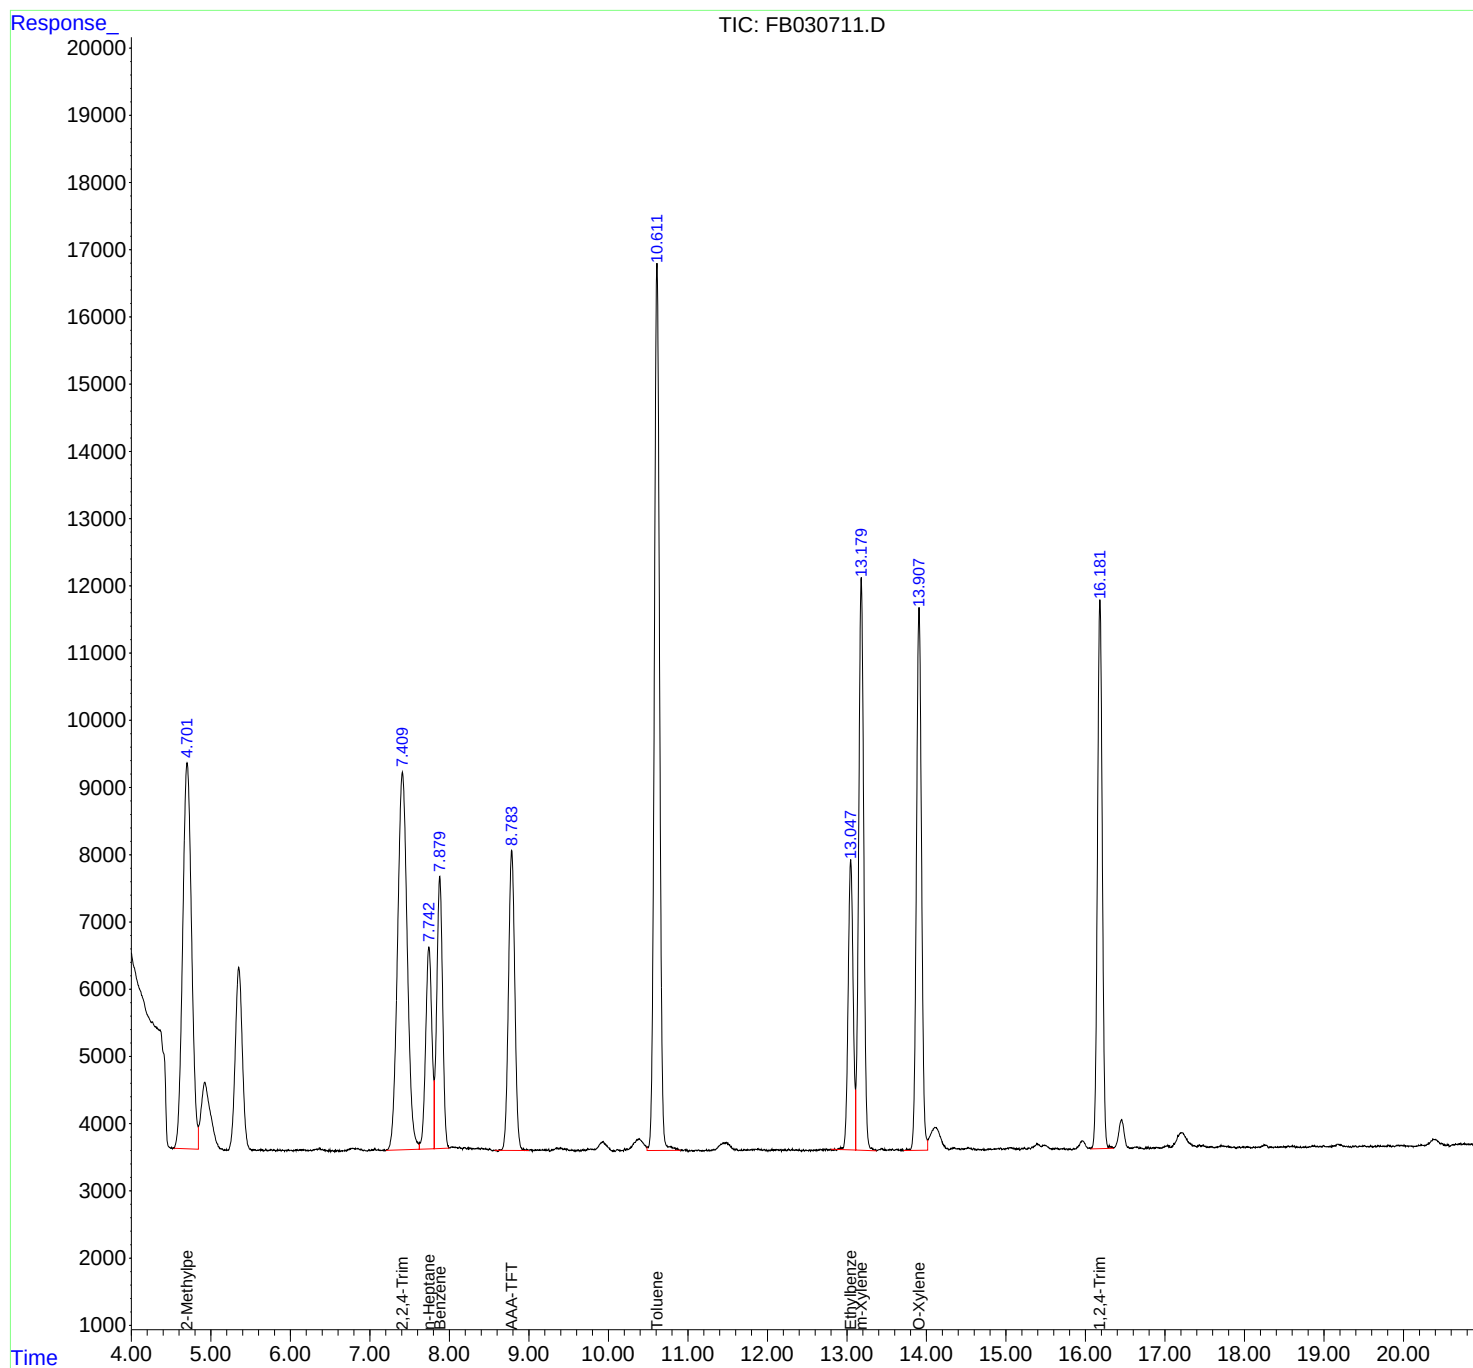

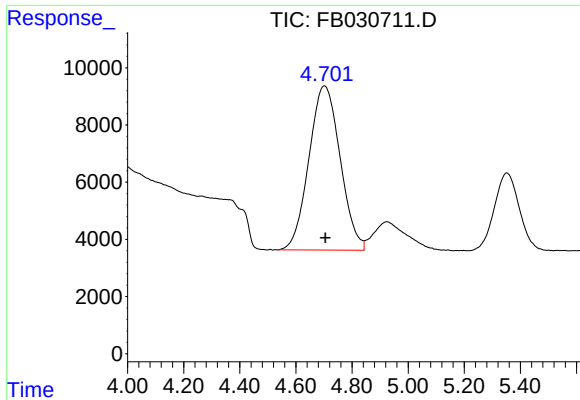


#1 2-Methylpentane

R.T.: 4.702 min
Delta R.T.: -0.003 min
Response: 444782
Conc: 27.16 ng/ml

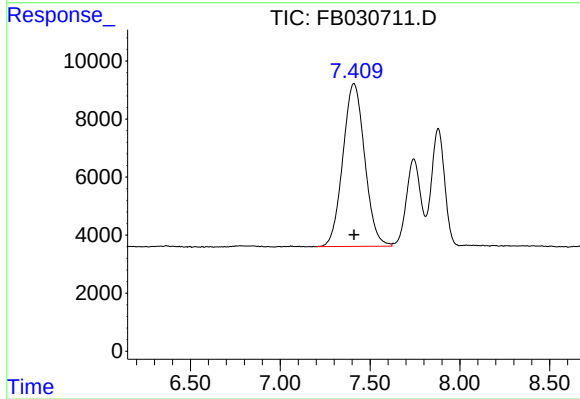


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: 0.000 min
Response: 473957
Conc: 28.20 ng/ml

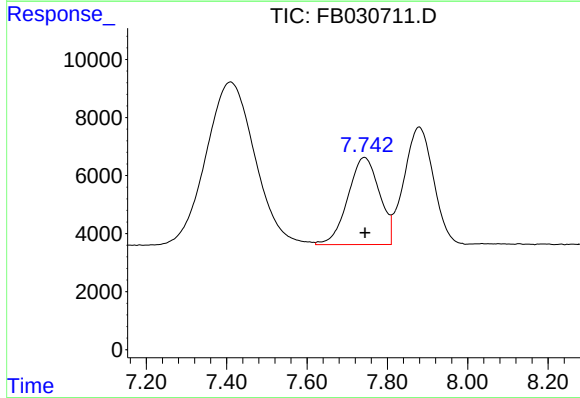


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.001 min
Response: 163873
Conc: 8.98 ng/ml

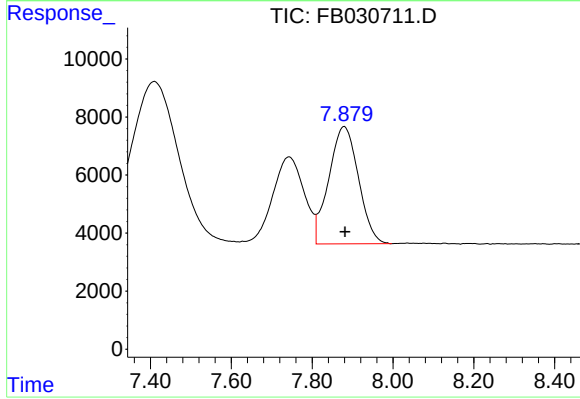


#4 Benzene

R.T.: 7.880 min
Delta R.T.: -0.002 min
Response: 205992
Conc: 9.67 ng/ml

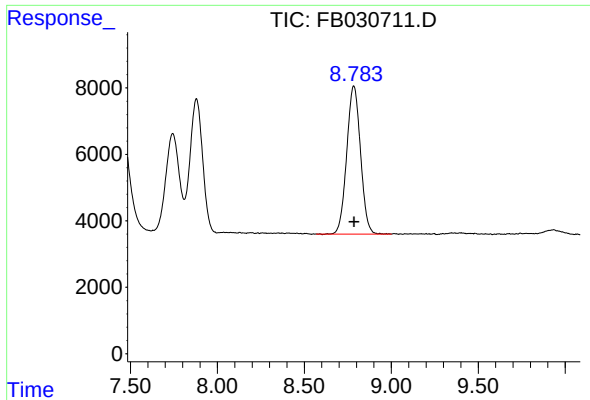


#5 AAA-TFT

R.T.: 8.785 min
Delta R.T.: -0.002 min
Response: 245425
Conc: 17.17 ng/ml

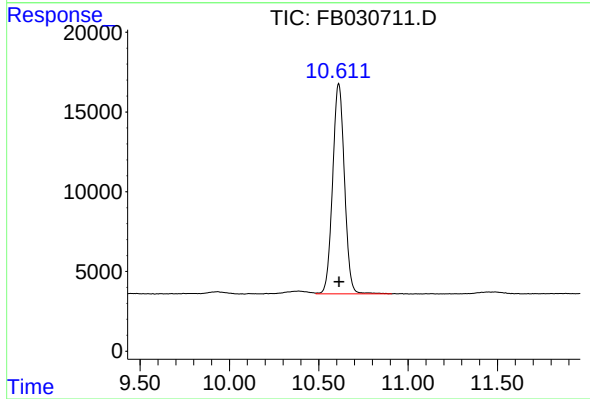


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.002 min
Response: 607530
Conc: 29.43 ng/ml

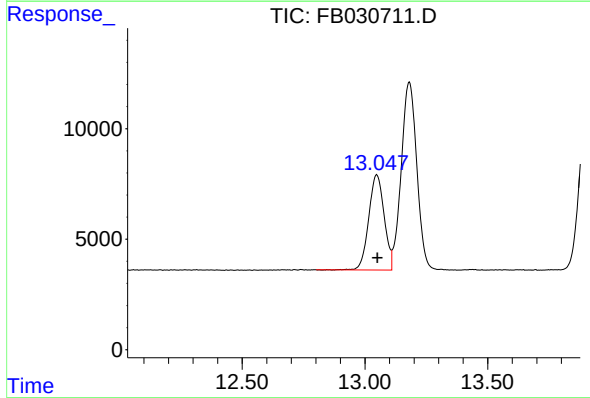


#7 Ethylbenzene

R.T.: 13.048 min
Delta R.T.: -0.002 min
Response: 187300
Conc: 9.76 ng/ml

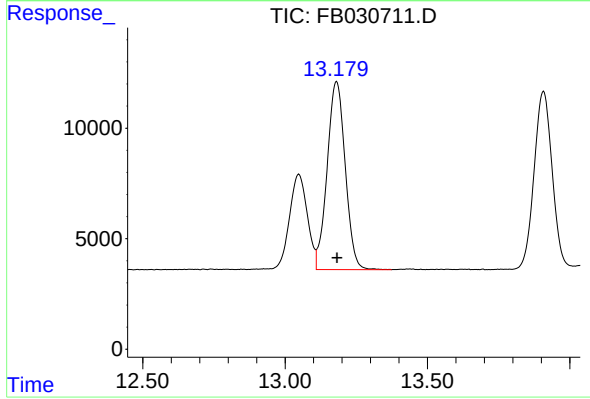


#8 m-Xylene

R.T.: 13.181 min
Delta R.T.: -0.002 min
Response: 375965
Conc: 19.69 ng/ml

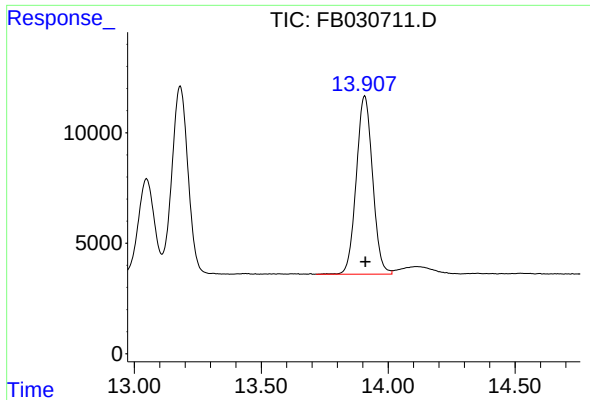

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: -0.002 min
Response: 358932
Conc: 19.23 ng/ml

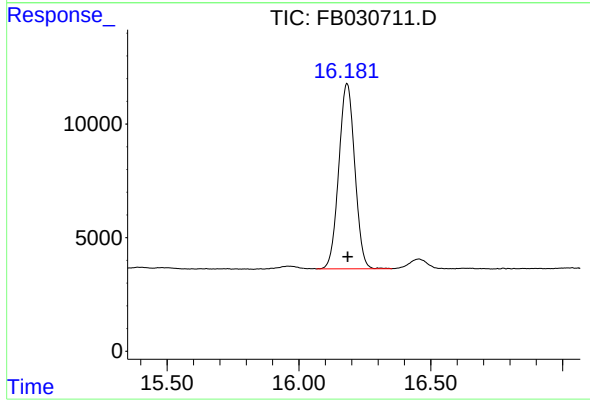

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.002 min
Response: 343553
Conc: 18.50 ng/ml