

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042721\
 Data File : FB025654.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2021 12:33
 Operator : DD/AJ
 Sample : M2176-04MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 28 03:34:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.232	393919	20.031 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.183	646614	26.728 ng/ml
2) t 2,2,4-Trimethylpentane	7.886	560434	30.134 ng/ml
3) t n-Heptane	8.205	251101	8.570 ng/ml
4) t Benzene	8.358	374773	9.700 ng/ml
6) t Toluene	11.054	1072162	29.705 ng/ml
7) t Ethylbenzene	13.464	347926	10.148 ng/ml
8) t m-Xylene	13.594	688093	20.243 ng/ml
9) t O-Xylene	14.318	652677	20.034 ng/ml
10) t 1,2,4-Trimethylbenzene	16.572	522541	19.878 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042721\
Data File : FB025654.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2021 12:33
Operator : DD/AJ
Sample : M2176-04MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 28 03:34:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

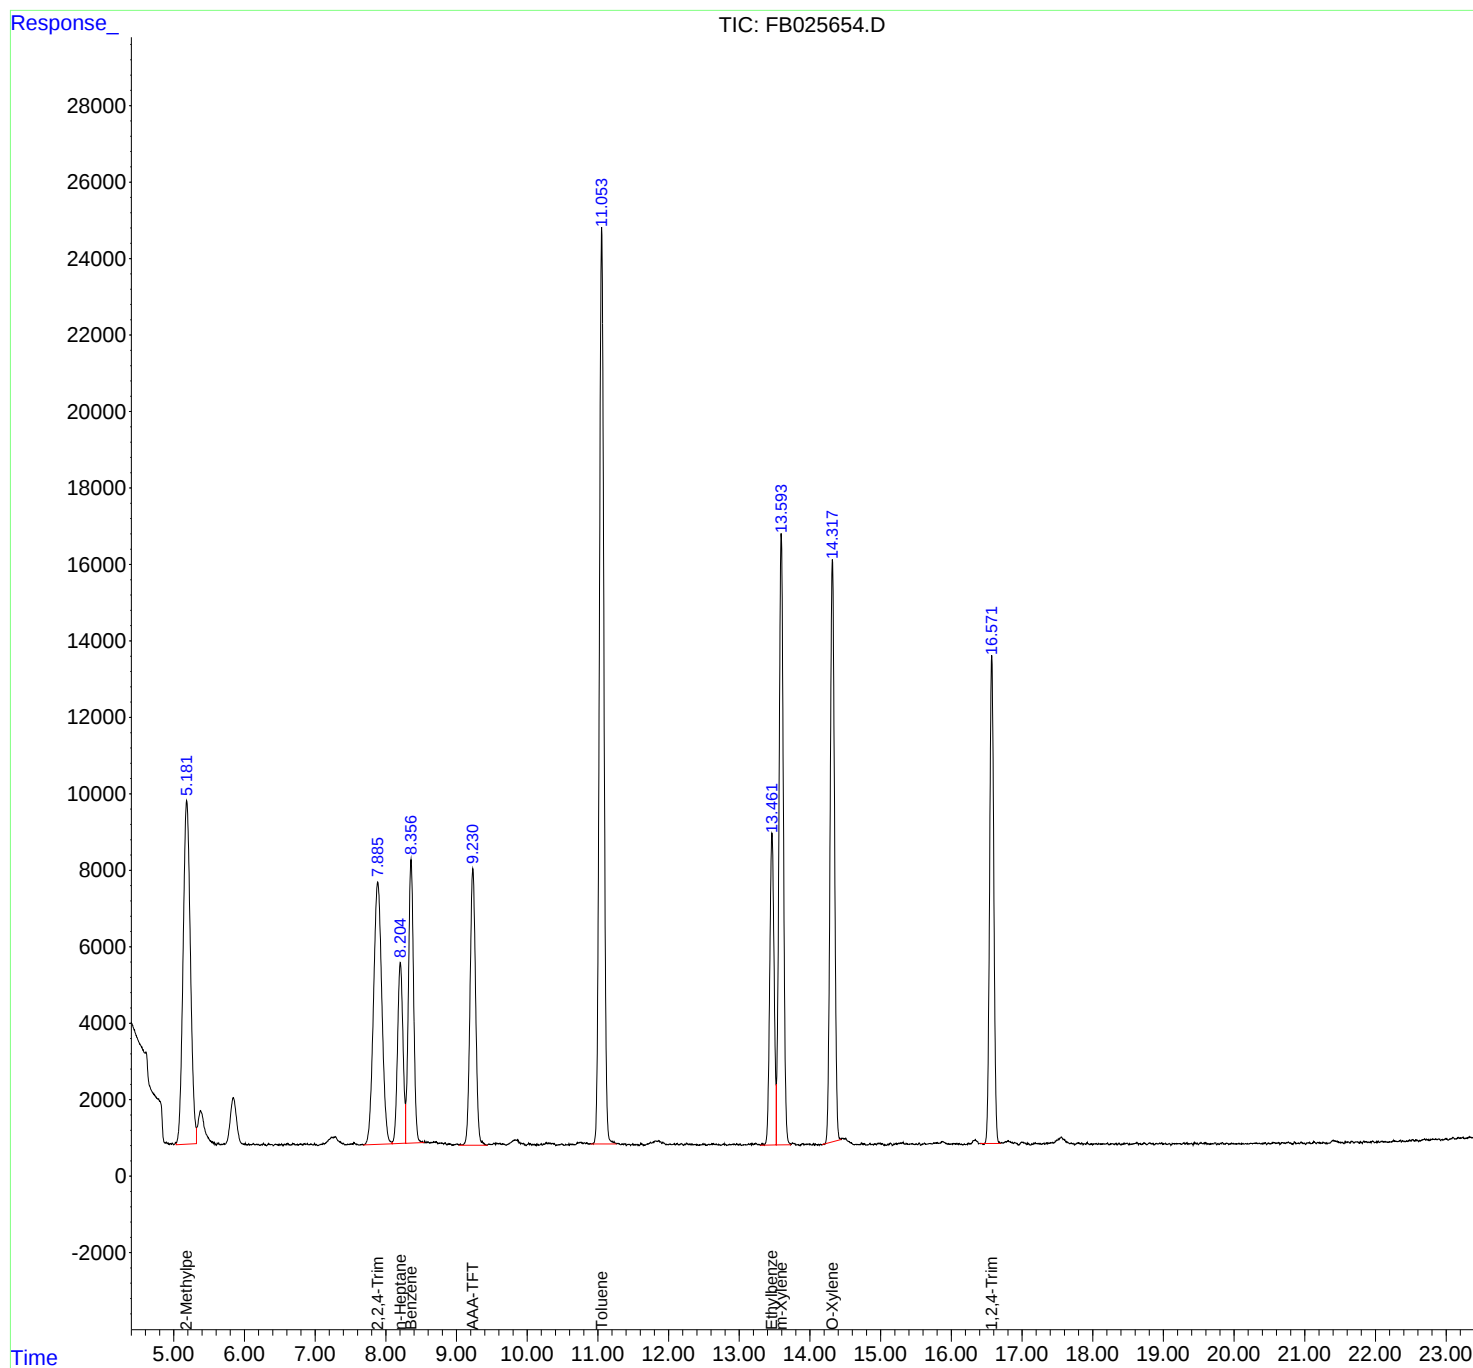


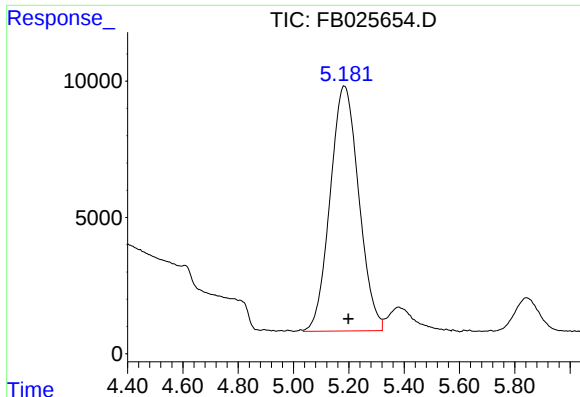

#1 2-Methylpentane


R.T.: 5.183 min
Delta R.T.: -0.015 min
Response: 646614
Conc: 26.73 ng/ml

Instrument :
FID_B
ClientSampleId :

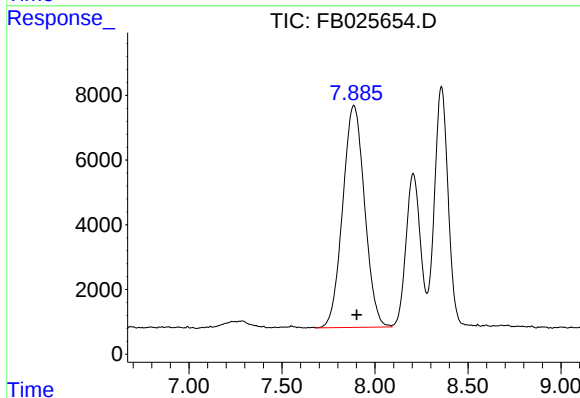


#2 2,2,4-Trimethylpentane

R.T.: 7.886 min
Delta R.T.: -0.016 min
Response: 560434
Conc: 30.13 ng/ml

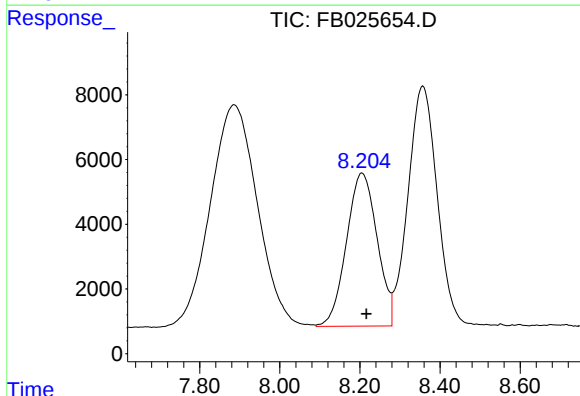


#3 n-Heptane

R.T.: 8.205 min
Delta R.T.: -0.011 min
Response: 251101
Conc: 8.57 ng/ml

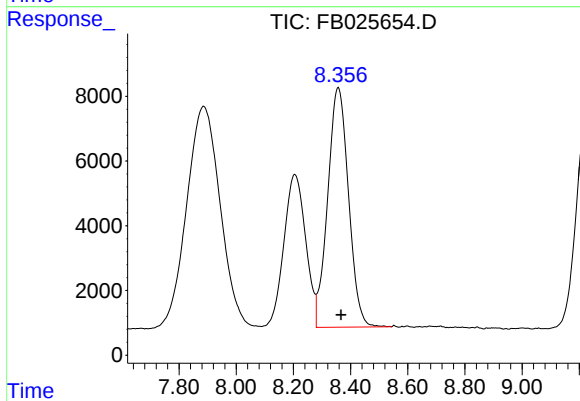

#4 Benzene


R.T.: 8.358 min
Delta R.T.: -0.009 min
Response: 374773
Conc: 9.70 ng/ml

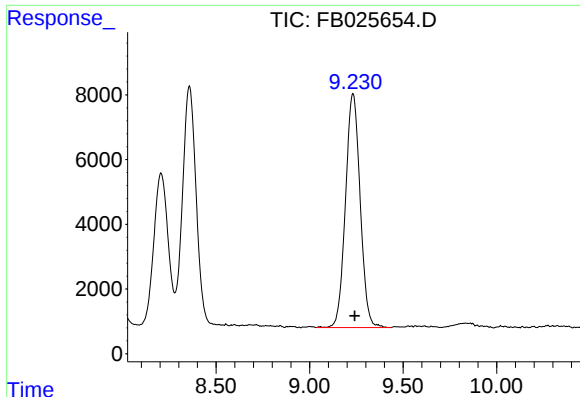

#5 AAA-TFT


R.T.: 9.232 min
Delta R.T.: -0.009 min
Response: 393919
Conc: 20.03 ng/ml

Instrument :
FID_B
ClientSampleId :

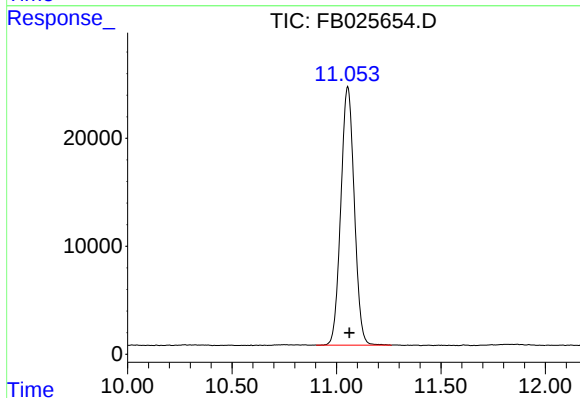


#6 Toluene

R.T.: 11.054 min
Delta R.T.: -0.008 min
Response: 1072162
Conc: 29.71 ng/ml

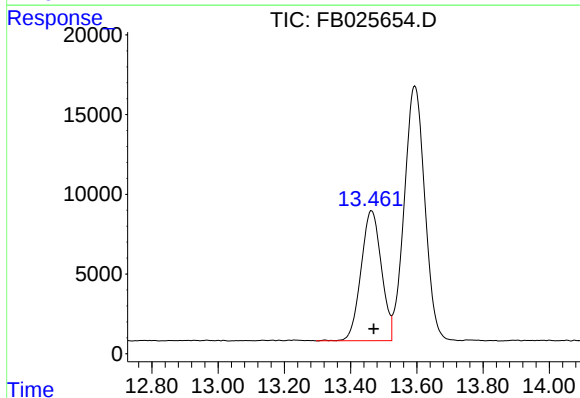


#7 Ethylbenzene

R.T.: 13.464 min
Delta R.T.: -0.007 min
Response: 347926
Conc: 10.15 ng/ml

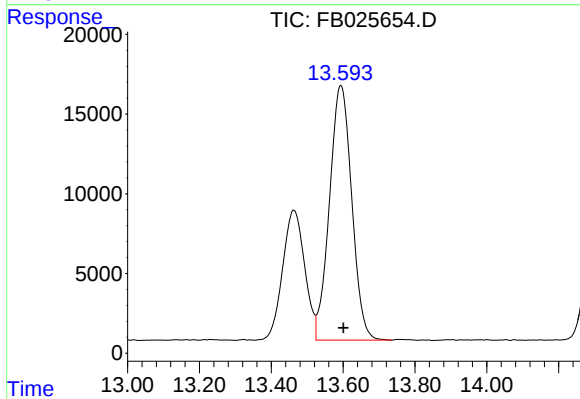

#8 m-Xylene


R.T.: 13.594 min
Delta R.T.: -0.007 min
Response: 688093
Conc: 20.24 ng/ml

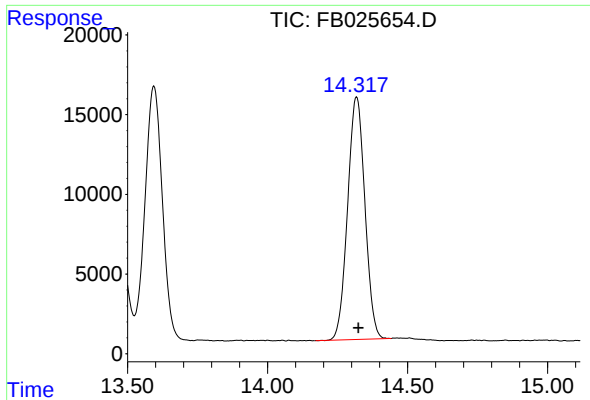

#9 O-Xylene

R.T.: 14.318 min
Delta R.T.: -0.007 min
Response: 652677
Conc: 20.03 ng/ml

Instrument :
FID_B
ClientSampleId :

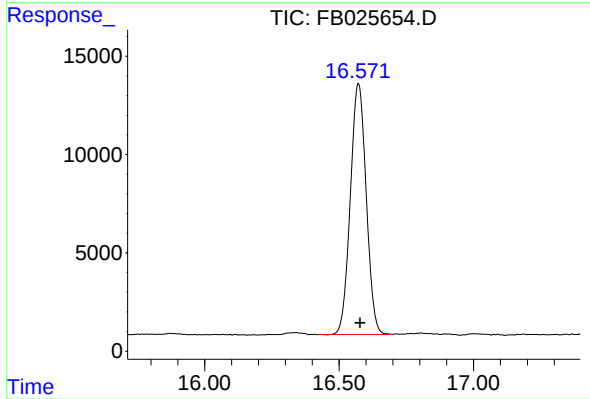

#10 1,2,4-Trimethylbenzene

R.T.: 16.572 min
Delta R.T.: -0.006 min
Response: 522541
Conc: 19.88 ng/ml