

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042721\
 Data File : FB025660.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2021 16:31
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 28 03:35:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.230	399051	20.292 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.174	654501	27.055 ng/ml
2) t 2,2,4-Trimethylpentane	7.882	568515	30.568 ng/ml
3) t n-Heptane	8.203	258552	8.825 ng/ml
4) t Benzene	8.354	361676	9.361 ng/ml
6) t Toluene	11.054	1051405	29.130 ng/ml
7) t Ethylbenzene	13.465	337817	9.853 ng/ml
8) t m-Xylene	13.595	674030	19.829 ng/ml
9) t O-Xylene	14.319	629214	19.314 ng/ml
10) t 1,2,4-Trimethylbenzene	16.573	530424	20.177 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042721\
Data File : FB025660.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2021 16:31
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 28 03:35:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

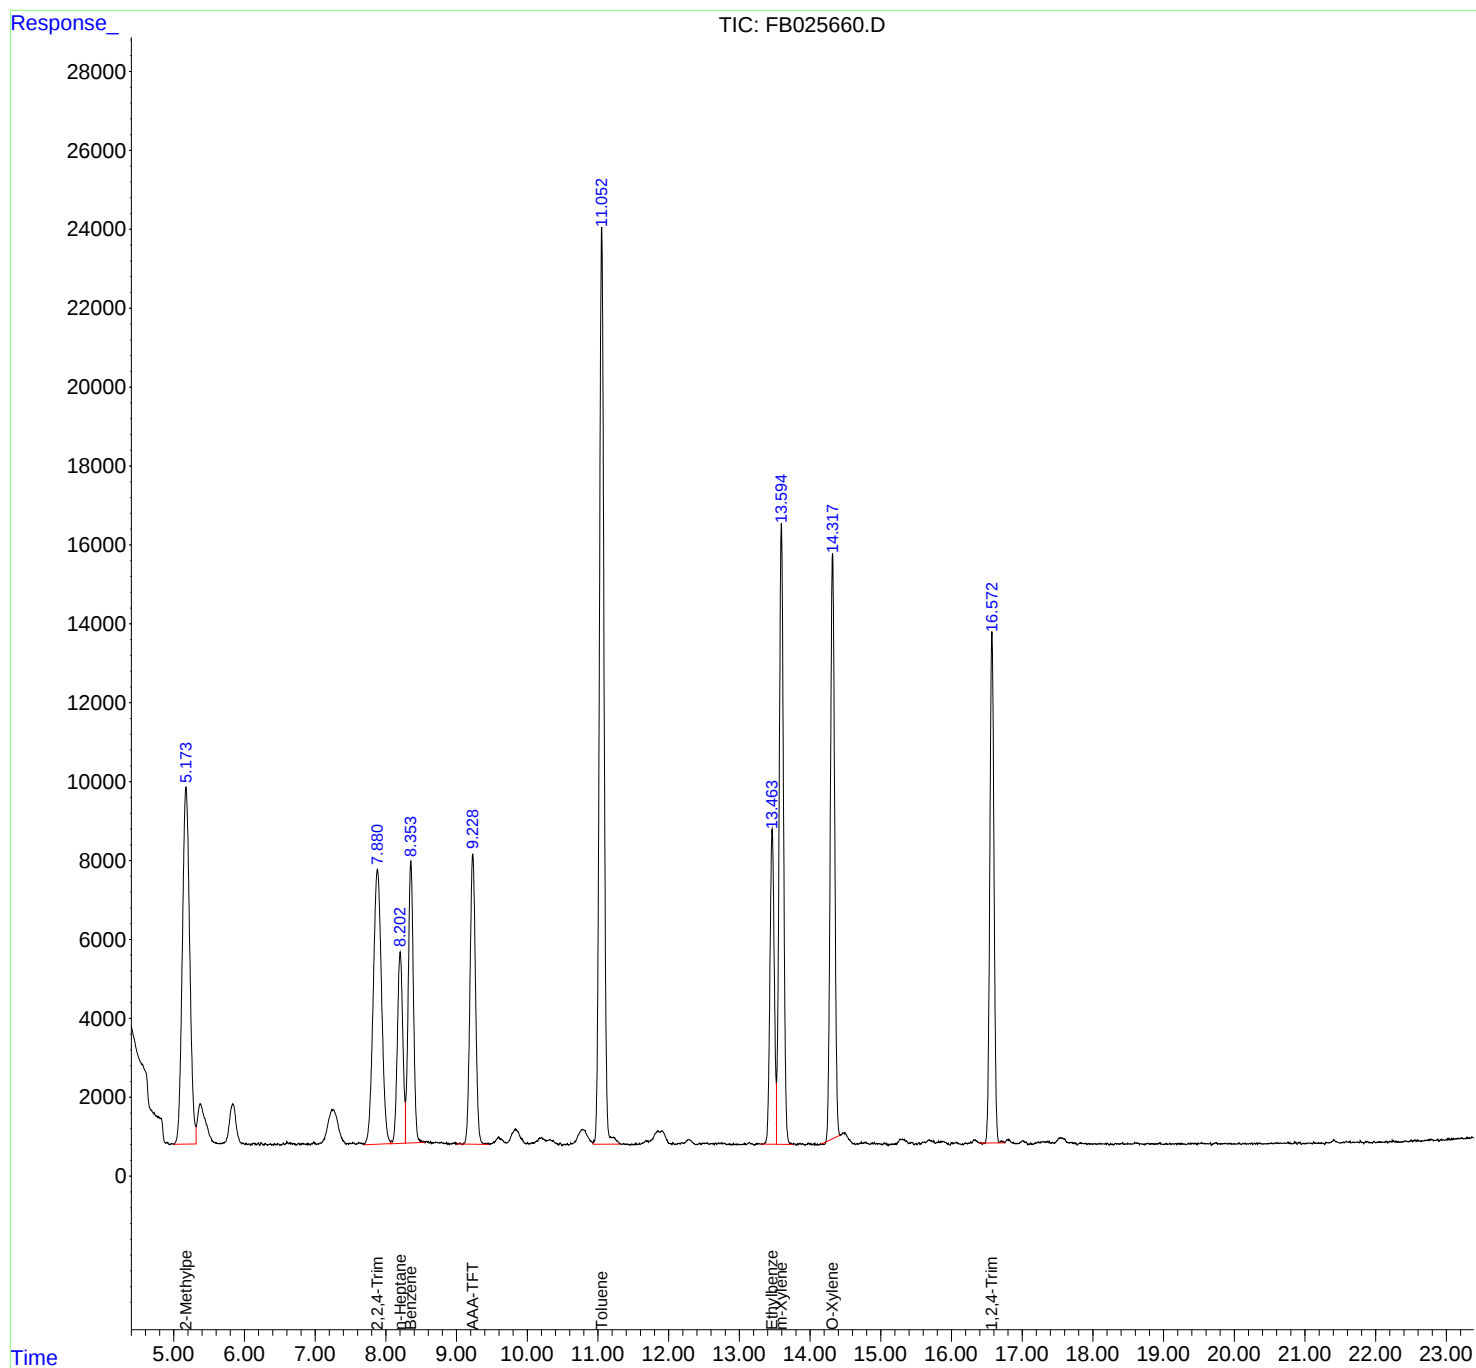


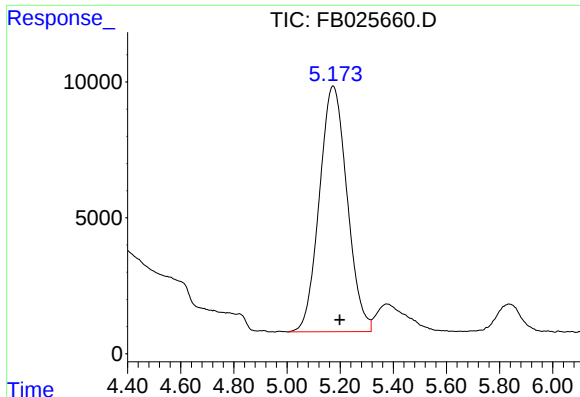

#1 2-Methylpentane


R.T.: 5.174 min
Delta R.T.: -0.024 min
Response: 654501
Conc: 27.05 ng/ml

Instrument :
FID_B
ClientSampleId :

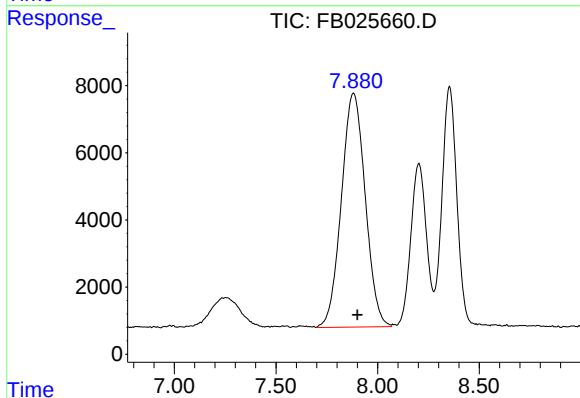


#2 2,2,4-Trimethylpentane

R.T.: 7.882 min
Delta R.T.: -0.020 min
Response: 568515
Conc: 30.57 ng/ml

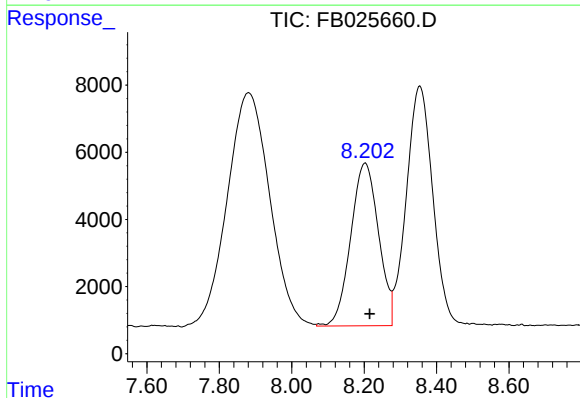


#3 n-Heptane

R.T.: 8.203 min
Delta R.T.: -0.013 min
Response: 258552
Conc: 8.82 ng/ml

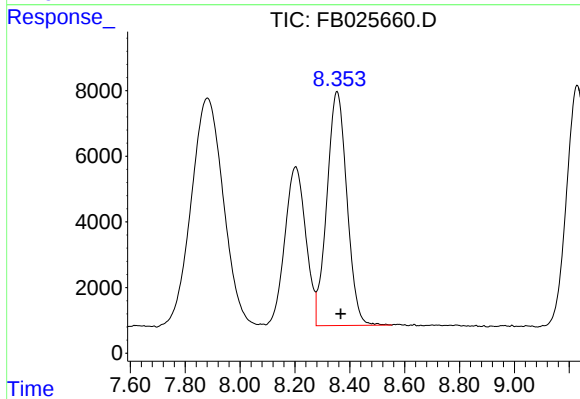

#4 Benzene


R.T.: 8.354 min
Delta R.T.: -0.013 min
Response: 361676
Conc: 9.36 ng/ml

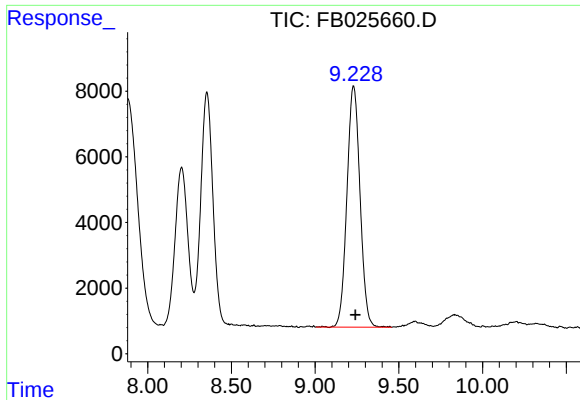

#5 AAA-TFT


R.T.: 9.230 min
Delta R.T.: -0.011 min
Response: 399051
Conc: 20.29 ng/ml

Instrument :
FID_B
ClientSampleId :

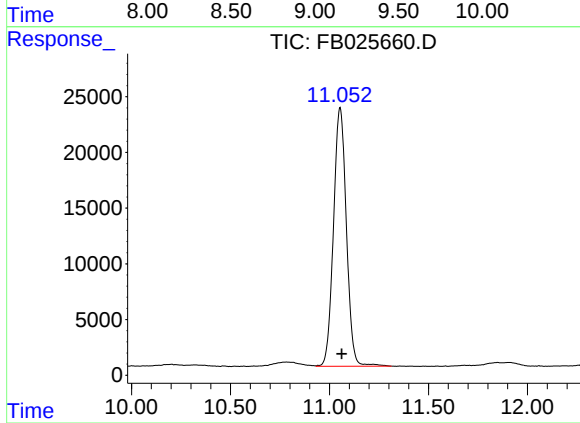


#6 Toluene

R.T.: 11.054 min
Delta R.T.: -0.008 min
Response: 1051405
Conc: 29.13 ng/ml

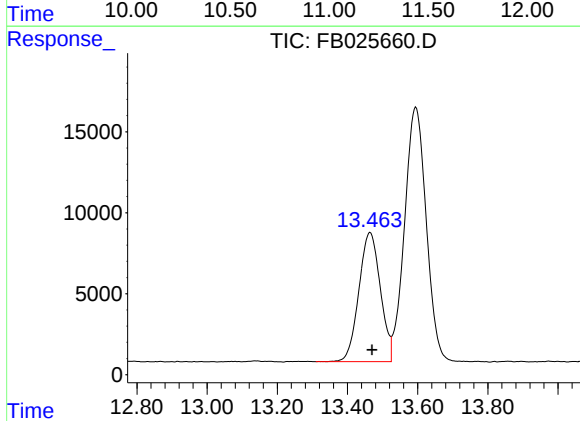


#7 Ethylbenzene

R.T.: 13.465 min
Delta R.T.: -0.006 min
Response: 337817
Conc: 9.85 ng/ml

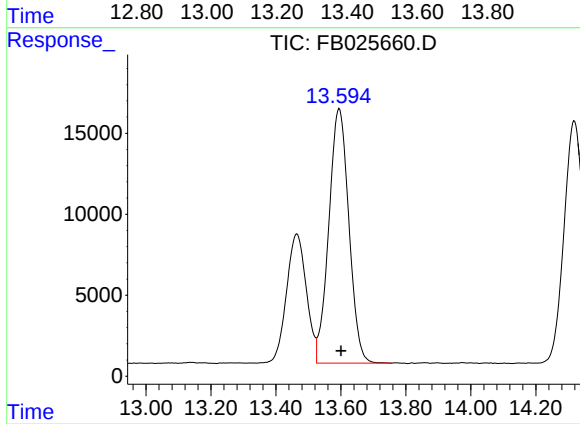

#8 m-Xylene


R.T.: 13.595 min
Delta R.T.: -0.006 min
Response: 674030
Conc: 19.83 ng/ml

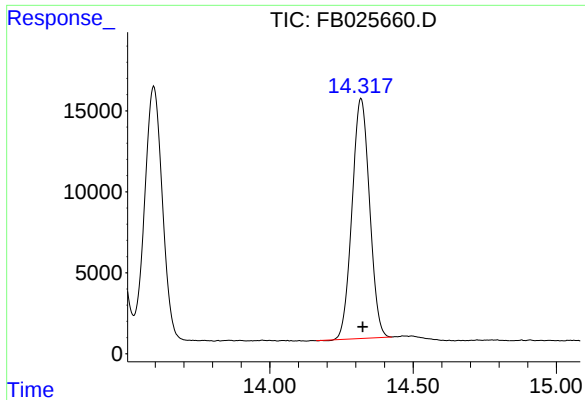

#9 O-Xylene

R.T.: 14.319 min
Delta R.T.: -0.006 min
Response: 629214
Conc: 19.31 ng/ml

Instrument :
FID_B
ClientSampleId :

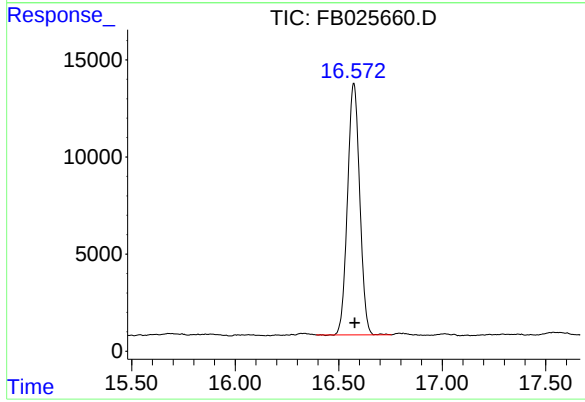

#10 1,2,4-Trimethylbenzene

R.T.: 16.573 min
Delta R.T.: -0.005 min
Response: 530424
Conc: 20.18 ng/ml