

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042721\
 Data File : FB025650.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2021 9:47
 Operator : DD/AJ
 Sample : BSF0427S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0427S1

Integration File: Calibration.e
 Quant Time: Apr 28 03:34:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.238	404466	20.567 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.209	712370	29.447 ng/ml
2) t 2,2,4-Trimethylpentane	7.898	660391	35.509 ng/ml
3) t n-Heptane	8.216	295603	10.089 ng/ml
4) t Benzene	8.368	374888	9.703 ng/ml
6) t Toluene	11.058	1082616	29.995 ng/ml
7) t Ethylbenzene	13.464	351609	10.256 ng/ml
8) t m-Xylene	13.595	701369	20.633 ng/ml
9) t O-Xylene	14.318	654016	20.075 ng/ml
10) t 1,2,4-Trimethylbenzene	16.571	549311	20.896 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042721\
Data File : FB025650.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2021 9:47
Operator : DD/AJ
Sample : BSF0427S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0427S1

Integration File: Calibration.e
Quant Time: Apr 28 03:34:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

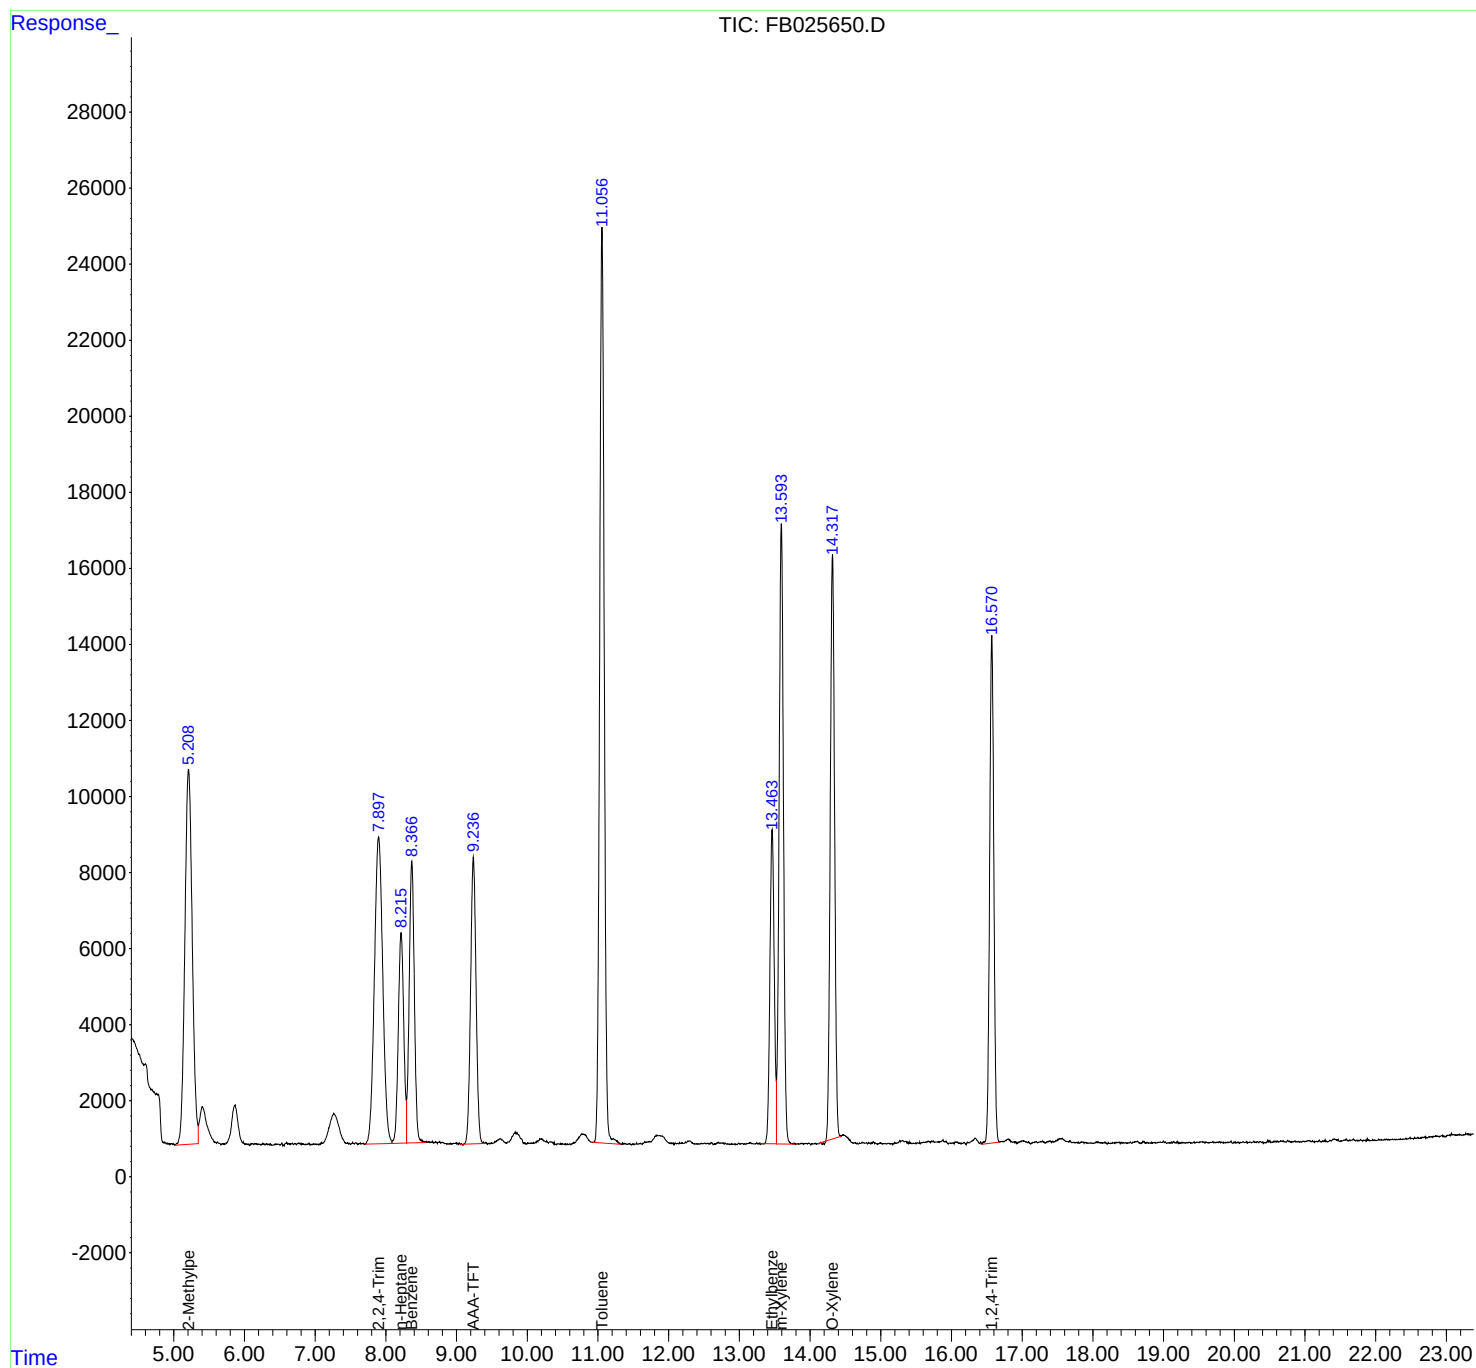


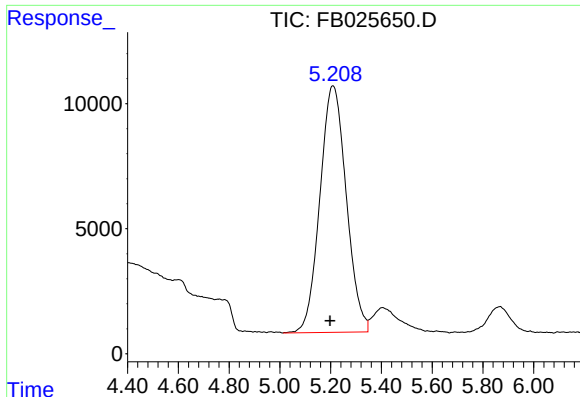

#1 2-Methylpentane


R.T.: 5.209 min
Delta R.T.: 0.011 min
Response: 712370
Conc: 29.45 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S1

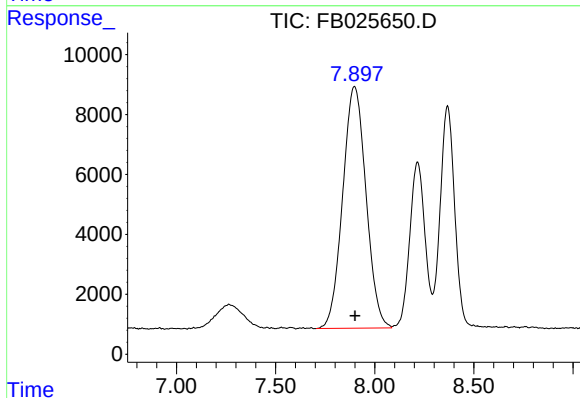


#2 2,2,4-Trimethylpentane

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 660391
Conc: 35.51 ng/ml

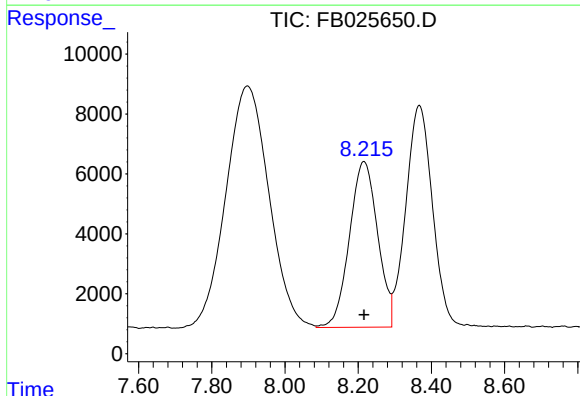


#3 n-Heptane

R.T.: 8.216 min
Delta R.T.: 0.000 min
Response: 295603
Conc: 10.09 ng/ml

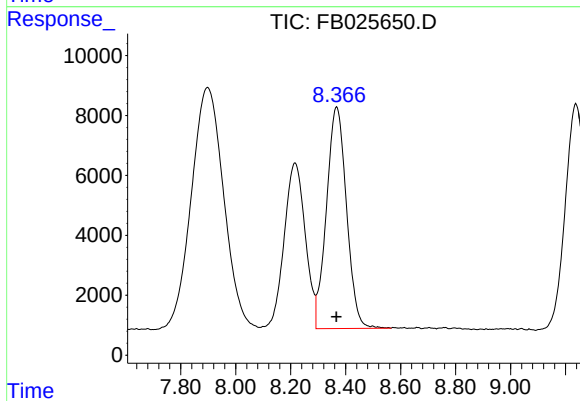

#4 Benzene


R.T.: 8.368 min
Delta R.T.: 0.001 min
Response: 374888
Conc: 9.70 ng/ml

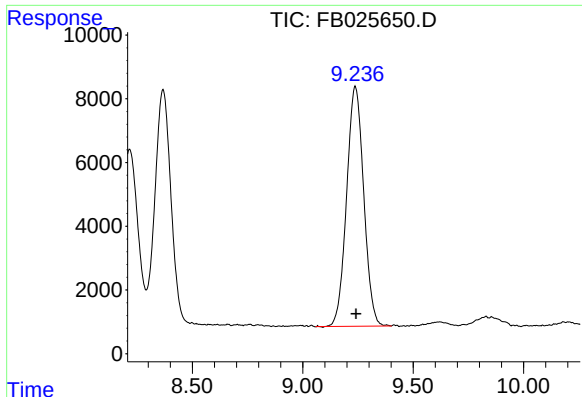

#5 AAA-TFT


R.T.: 9.238 min
Delta R.T.: -0.003 min
Response: 404466
Conc: 20.57 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S1

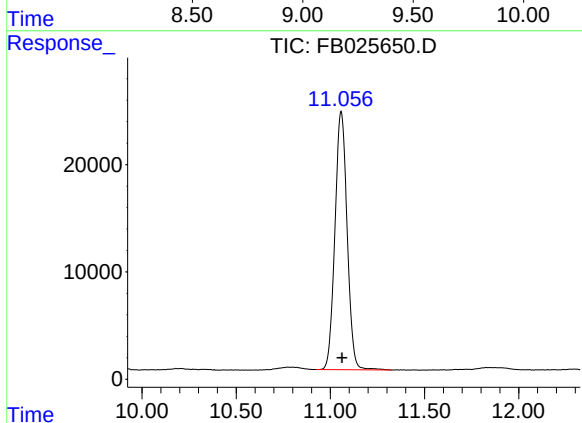


#6 Toluene

R.T.: 11.058 min
Delta R.T.: -0.005 min
Response: 1082616
Conc: 30.00 ng/ml

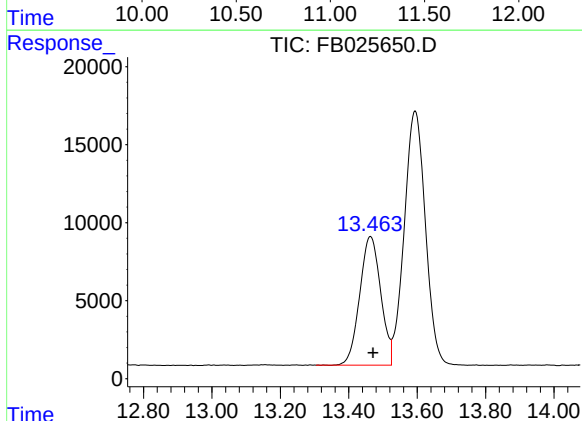


#7 Ethylbenzene

R.T.: 13.464 min
Delta R.T.: -0.007 min
Response: 351609
Conc: 10.26 ng/ml

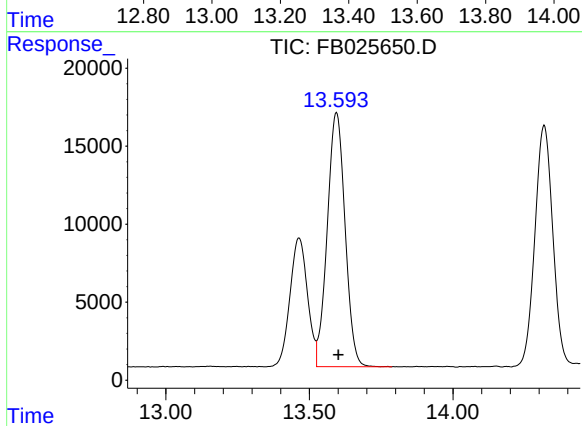

#8 m-Xylene


R.T.: 13.595 min
Delta R.T.: -0.006 min
Response: 701369
Conc: 20.63 ng/ml

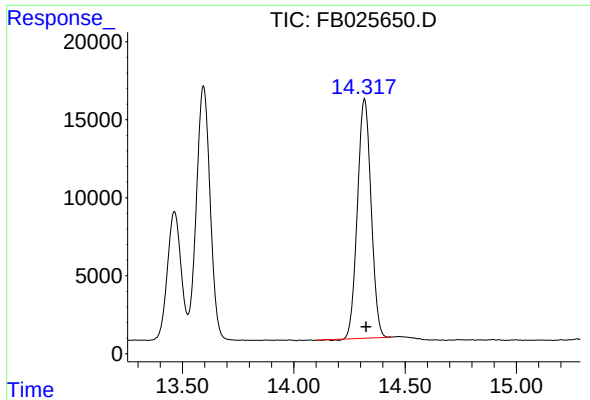

#9 O-Xylene

R.T.: 14.318 min
Delta R.T.: -0.007 min
Response: 654016
Conc: 20.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S1

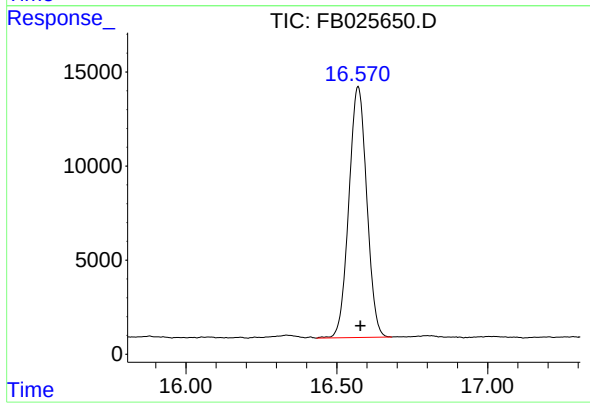

#10 1,2,4-Trimethylbenzene

R.T.: 16.571 min
Delta R.T.: -0.007 min
Response: 549311
Conc: 20.90 ng/ml