

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
 Data File : FB027085.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2022 12:39
 Operator : AJ/MA
 Sample : N2431-05MS 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 28 04:07:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	325290	28.773 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	425344	22.596 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	388050	19.397 ng/ml
3) t n-Heptane	7.747	230870	11.802 ng/ml
4) t Benzene	7.884	215686	9.773 ng/ml
6) t Toluene	10.618	700509	33.972 ng/ml
7) t Ethylbenzene	13.055	326770	17.102 ng/ml
8) t m-Xylene	13.187	476254	25.212 ng/ml
9) t O-Xylene	13.915	429148	23.692 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	500217	27.139 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
Data File : FB027085.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2022 12:39
Operator : AJ/MA
Sample : N2431-05MS 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 28 04:07:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

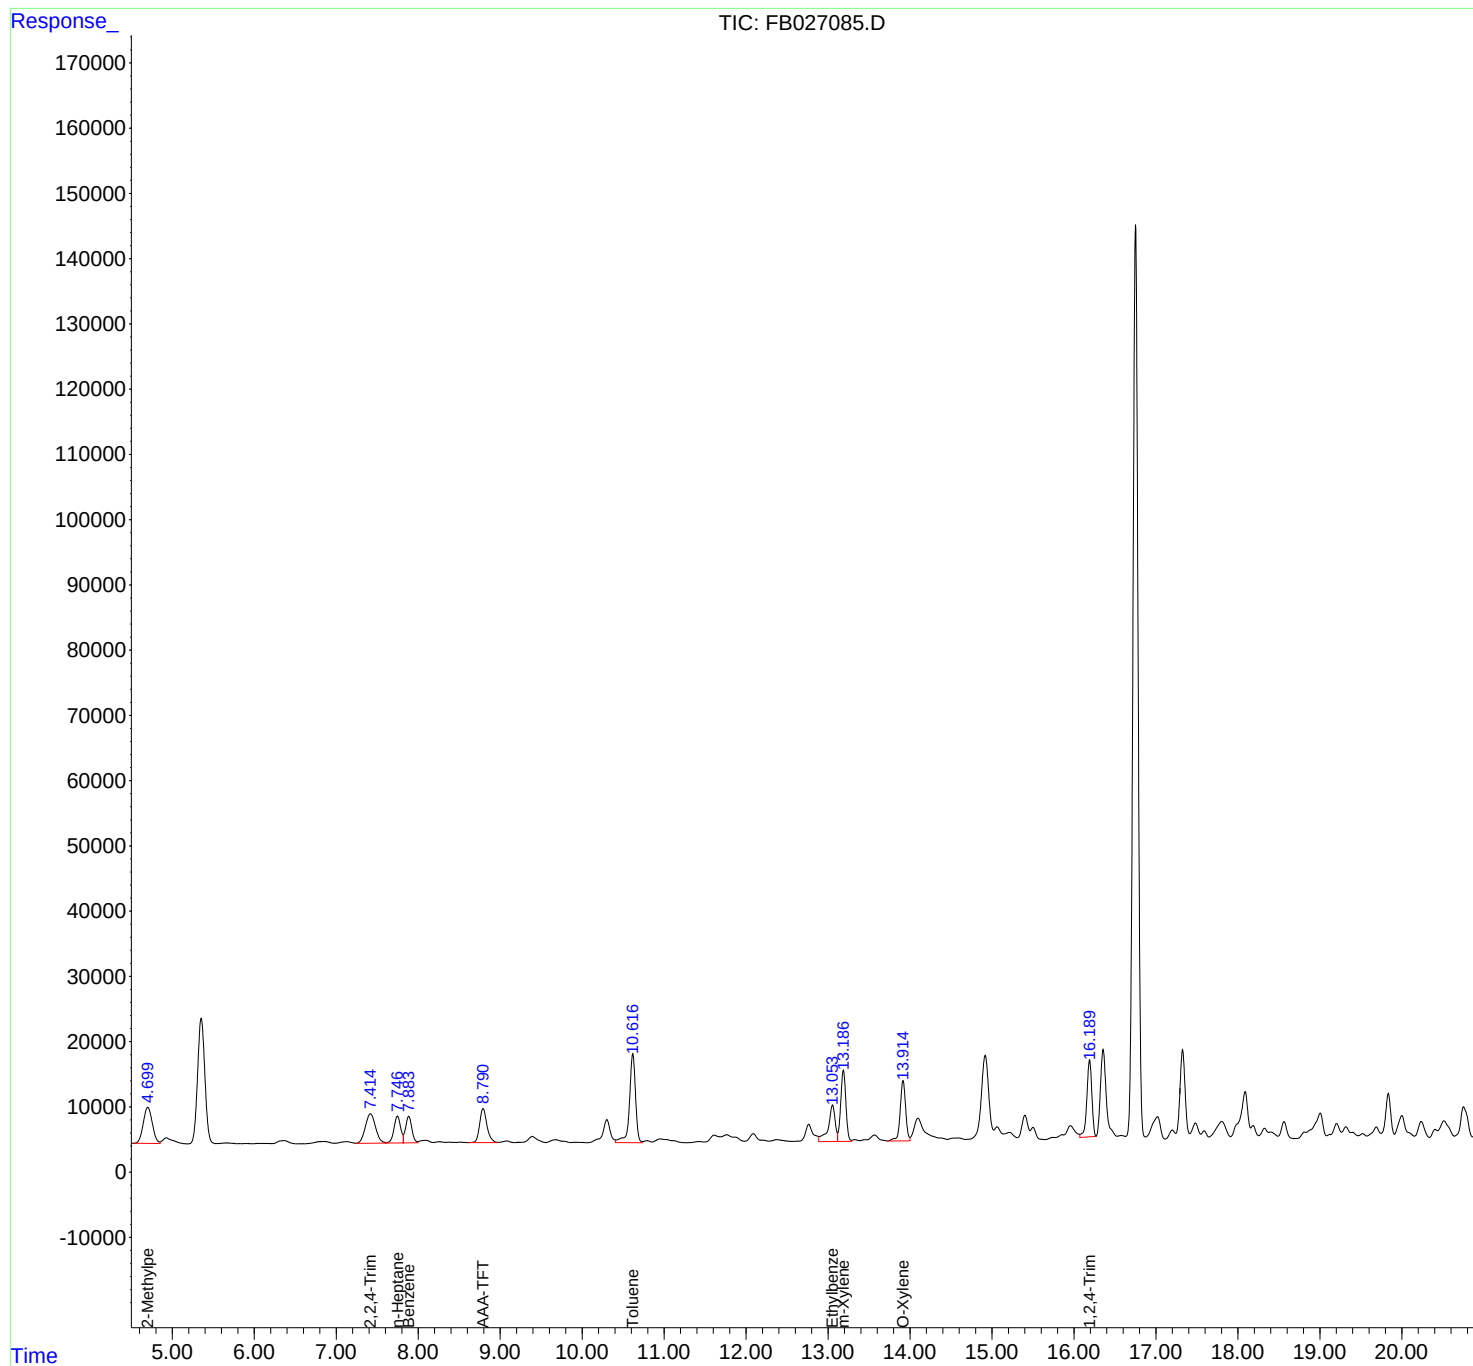


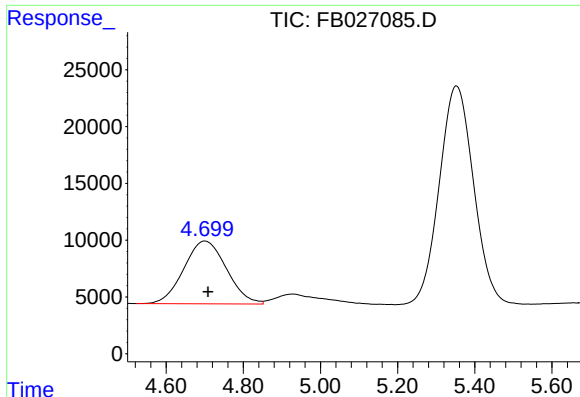

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.008 min
Response: 425344
Conc: 22.60 ng/ml

Instrument :
FID_B
ClientSampleId :

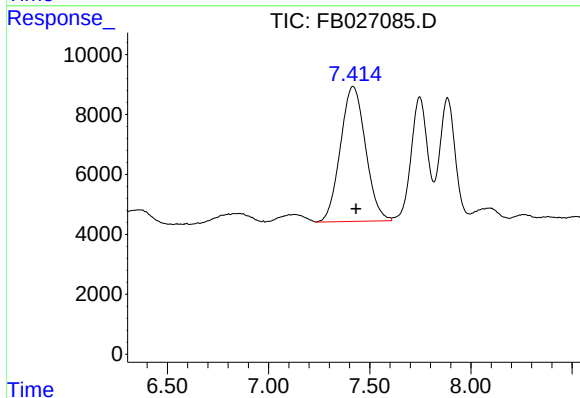


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.017 min
Response: 388050
Conc: 19.40 ng/ml

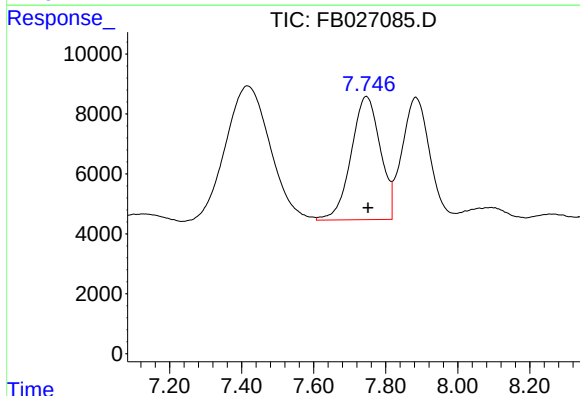


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.004 min
Response: 230870
Conc: 11.80 ng/ml

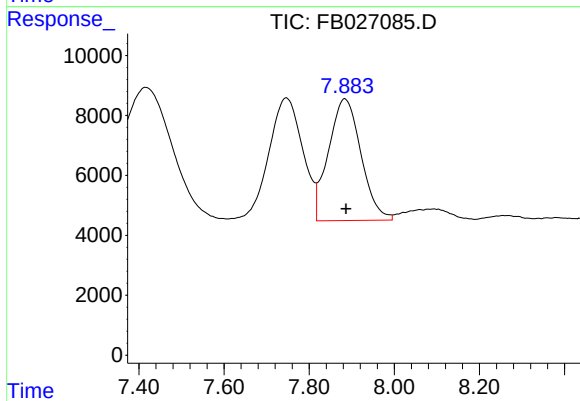

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.003 min
Response: 215686
Conc: 9.77 ng/ml

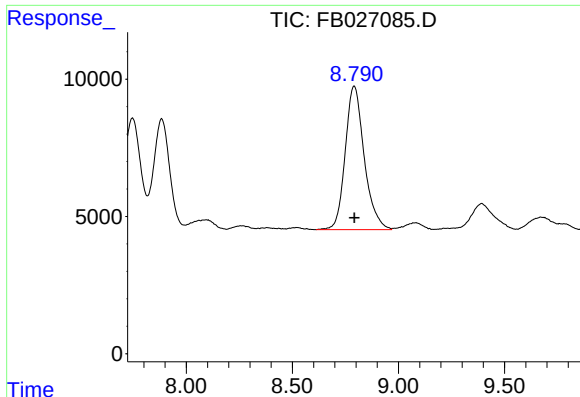

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 325290
Conc: 28.77 ng/ml

Instrument :
FID_B
ClientSampleId :

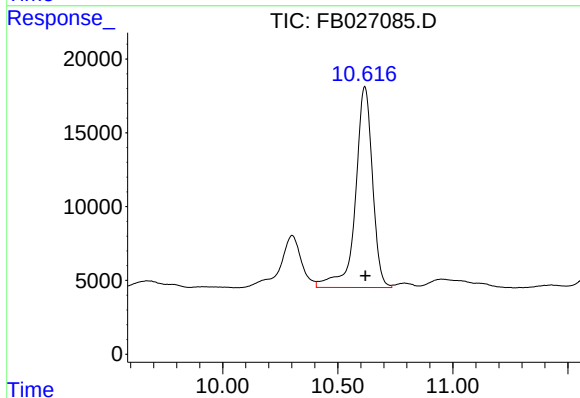


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 700509
Conc: 33.97 ng/ml

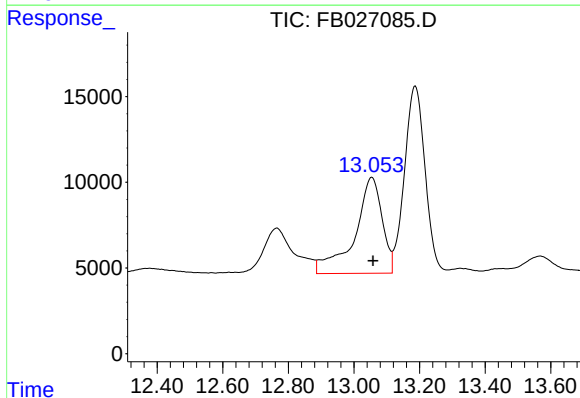


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.003 min
Response: 326770
Conc: 17.10 ng/ml

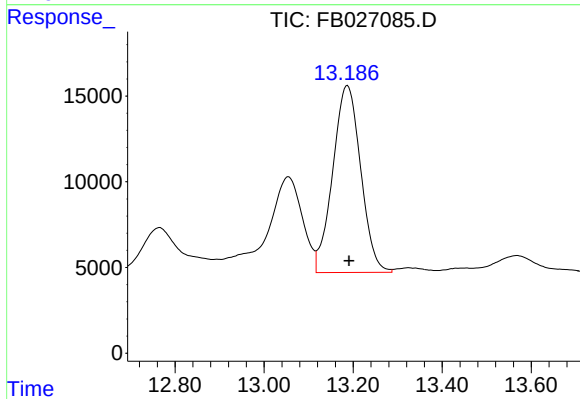

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.004 min
Response: 476254
Conc: 25.21 ng/ml

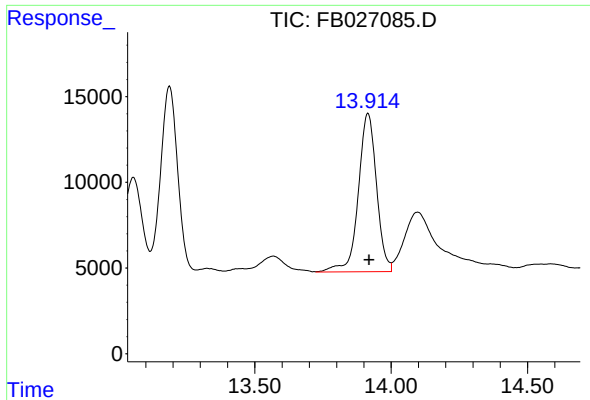

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.003 min
Response: 429148
Conc: 23.69 ng/ml

Instrument :
FID_B
ClientSampleId :

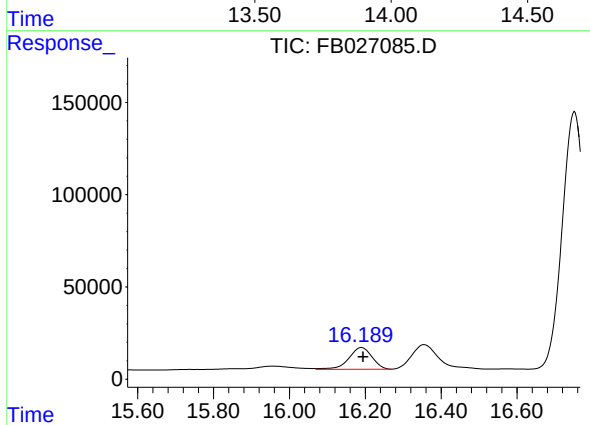

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 500217
Conc: 27.14 ng/ml