

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
 Data File : FB027086.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2022 13:15
 Operator : AJ/MA
 Sample : N2431-05MSD 50X
 Misc : 5.03G/5.00 ML MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 28 04:07:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	321712	28.456 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.698	377462	20.053 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	349860	17.488 ng/ml
3) t n-Heptane	7.746	241619	12.352 ng/ml
4) t Benzene	7.884	218846	9.916 ng/ml
6) t Toluene	10.617	706056	34.241 ng/ml
7) t Ethylbenzene	13.054	342122	17.906 ng/ml
8) t m-Xylene	13.186	496856	26.303 ng/ml
9) t O-Xylene	13.914	423407	23.375 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	529634	28.735 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
Data File : FB027086.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2022 13:15
Operator : AJ/MA
Sample : N2431-05MSD 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 28 04:07:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

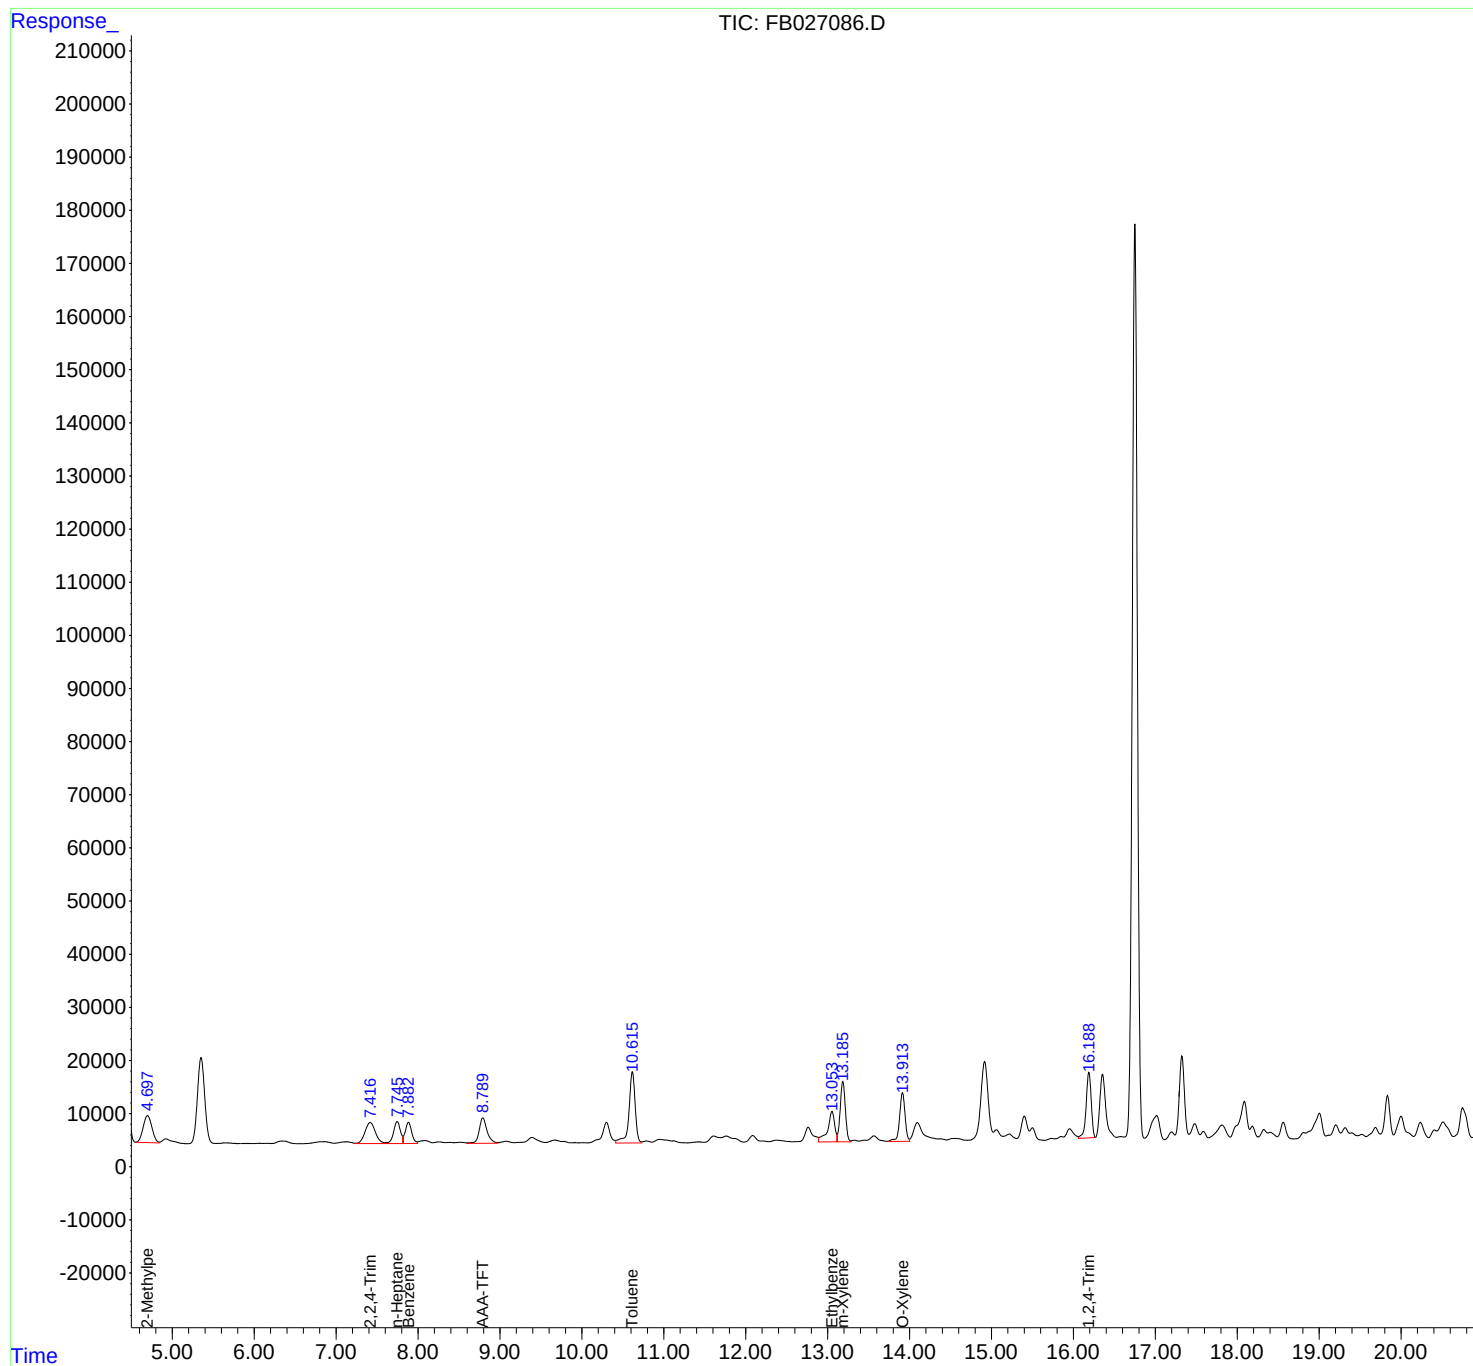


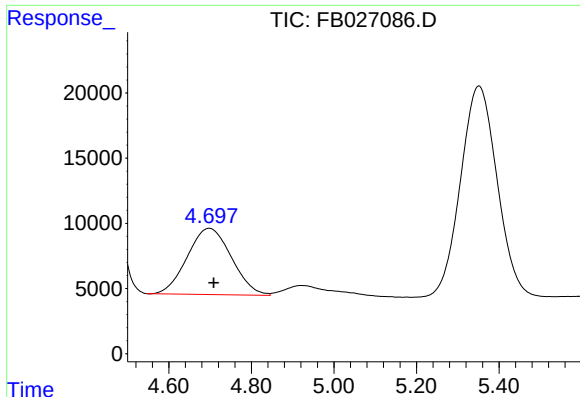

#1 2-Methylpentane


R.T.: 4.698 min
Delta R.T.: -0.011 min
Response: 377462
Conc: 20.05 ng/ml

Instrument :
FID_B
ClientSampleId :

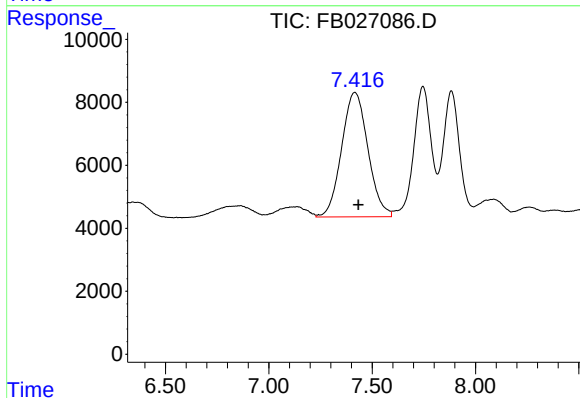


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.016 min
Response: 349860
Conc: 17.49 ng/ml

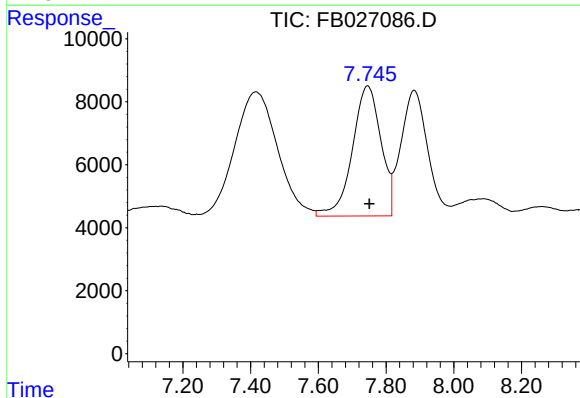


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.005 min
Response: 241619
Conc: 12.35 ng/ml

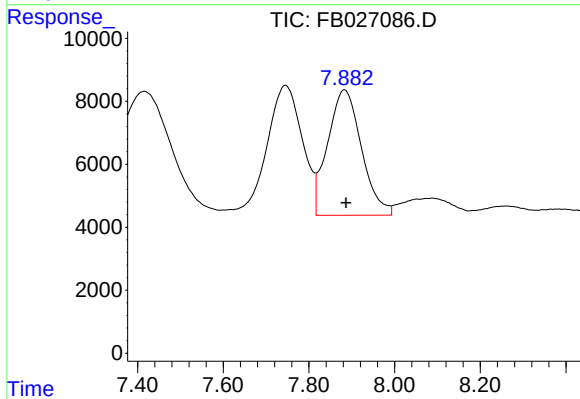

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.003 min
Response: 218846
Conc: 9.92 ng/ml

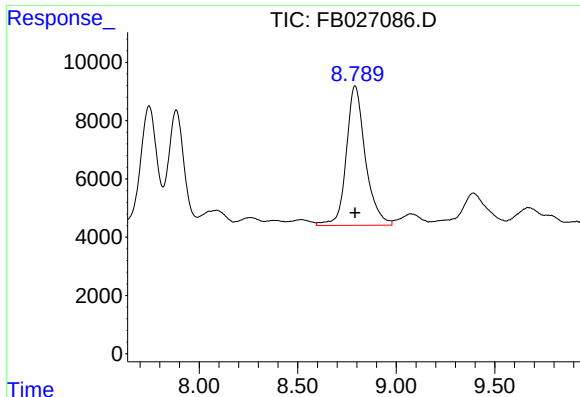

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 321712
Conc: 28.46 ng/ml

Instrument :
FID_B
ClientSampleId :

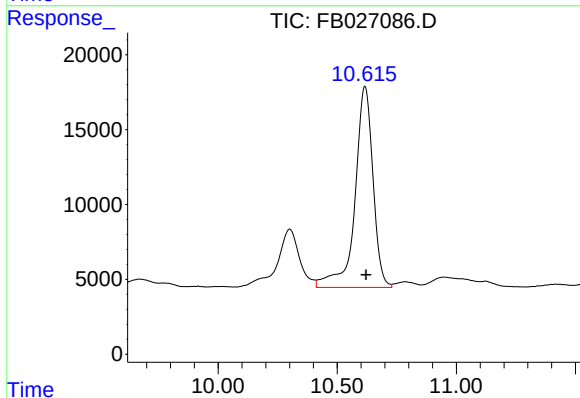


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.004 min
Response: 706056
Conc: 34.24 ng/ml

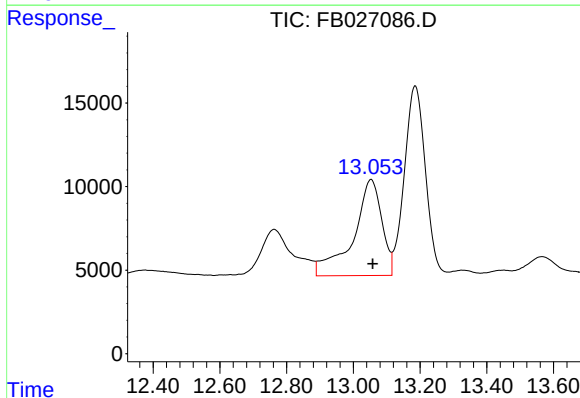


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.005 min
Response: 342122
Conc: 17.91 ng/ml

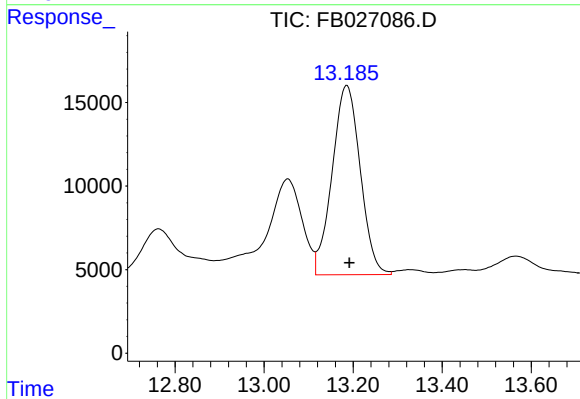

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 496856
Conc: 26.30 ng/ml

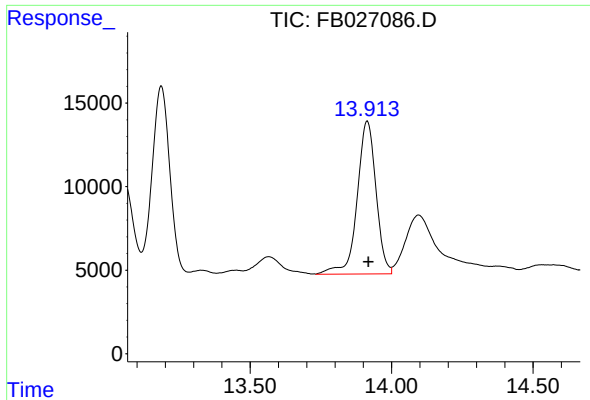

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.004 min
Response: 423407
Conc: 23.38 ng/ml

Instrument :
FID_B
ClientSampleId :

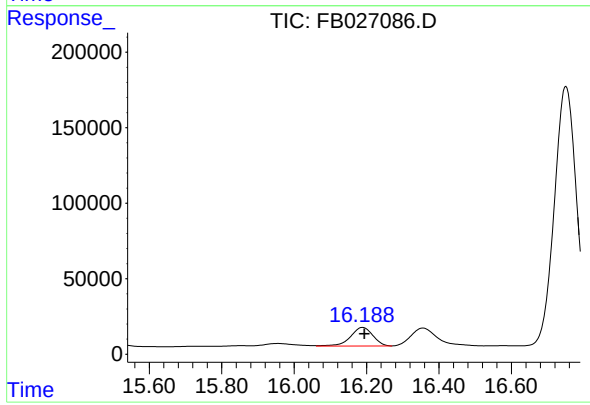

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 529634
Conc: 28.73 ng/ml