

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
 Data File : FB027090.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2022 17:15
 Operator : AJ/MA
 Sample : N2514-05 50X
 Misc : 5.01G/5.00 ML MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 28 04:09:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	520544	46.044 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	310250	16.482 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	471024	23.545 ng/ml
3) t n-Heptane	7.743	213174	10.898 ng/ml
4) t Benzene	7.876	211111	9.566 ng/ml
6) t Toluene	10.614	548145	26.583 ng/ml
7) t Ethylbenzene	13.041	405640	21.230 ng/ml
8) t m-Xylene	13.183	307436	16.275 ng/ml
9) t O-Xylene	13.910	438348	24.200 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	350532	19.018 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
Data File : FB027090.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2022 17:15
Operator : AJ/MA
Sample : N2514-05 50X
Misc : 5.01G/5.00 ML MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 28 04:09:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

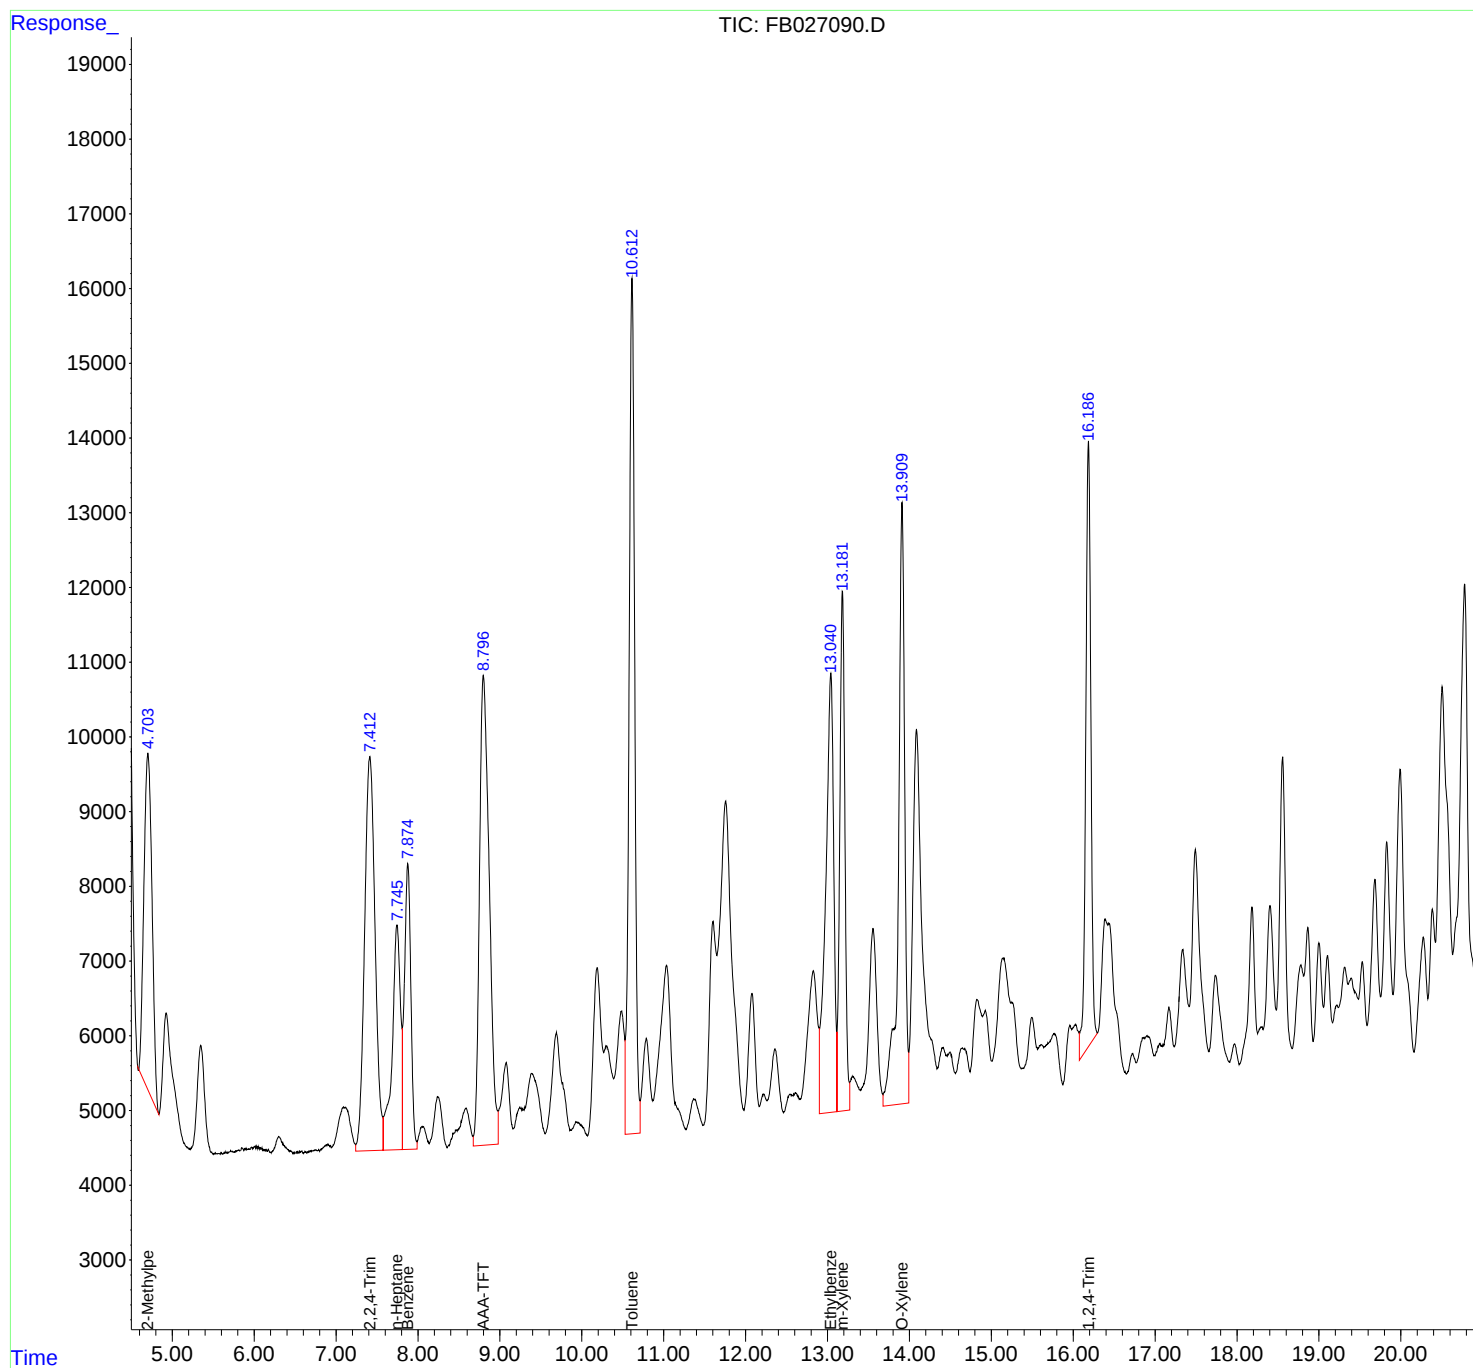


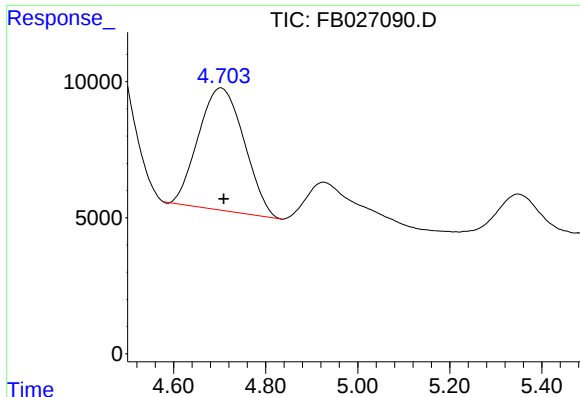

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.006 min
Response: 310250
Conc: 16.48 ng/ml

Instrument :
FID_B
ClientSampleId :

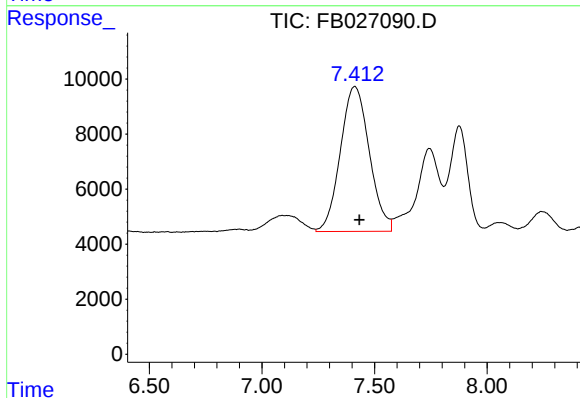


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.020 min
Response: 471024
Conc: 23.54 ng/ml

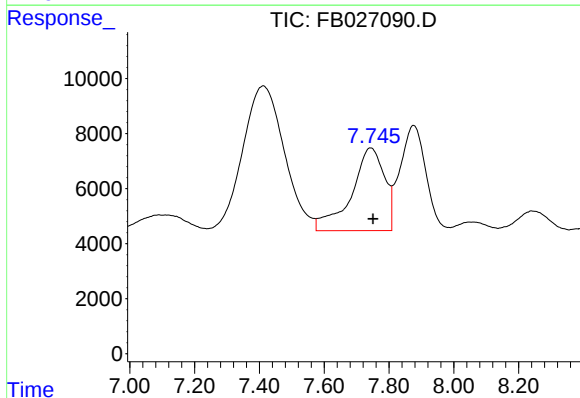


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.007 min
Response: 213174
Conc: 10.90 ng/ml

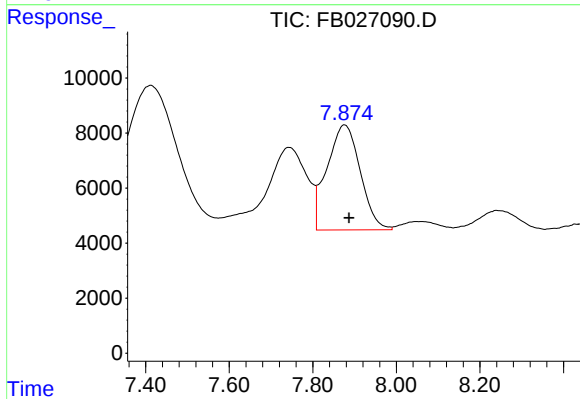

#4 Benzene


R.T.: 7.876 min
Delta R.T.: -0.011 min
Response: 211111
Conc: 9.57 ng/ml

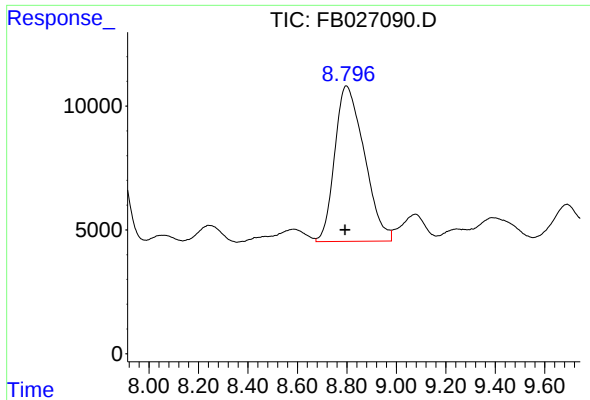

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.006 min
Response: 520544
Conc: 46.04 ng/ml

Instrument :
FID_B
ClientSampleId :

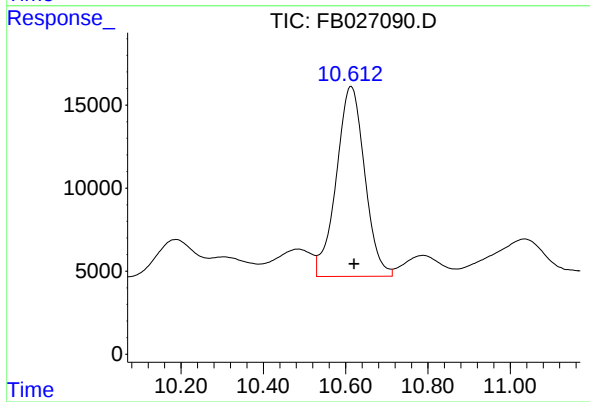


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.007 min
Response: 548145
Conc: 26.58 ng/ml

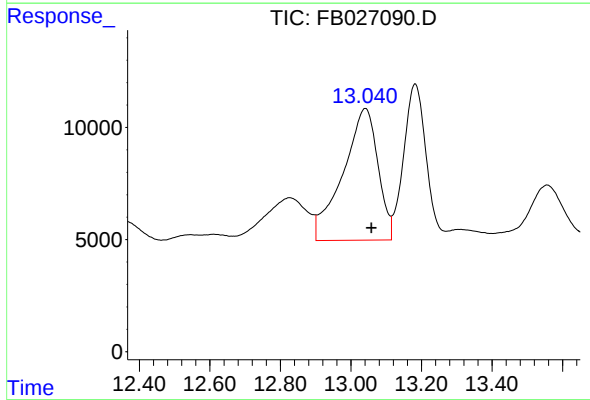


#7 Ethylbenzene

R.T.: 13.041 min
Delta R.T.: -0.017 min
Response: 405640
Conc: 21.23 ng/ml

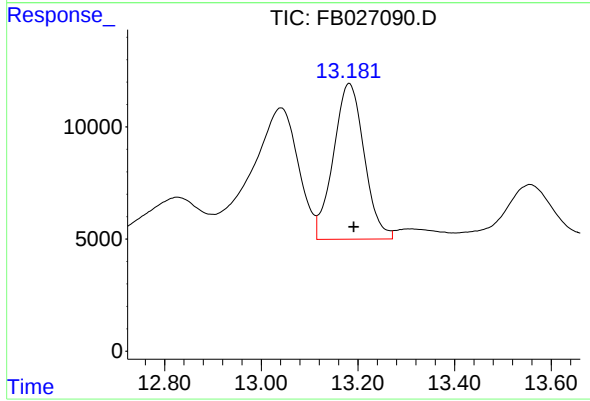

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: -0.009 min
Response: 307436
Conc: 16.28 ng/ml

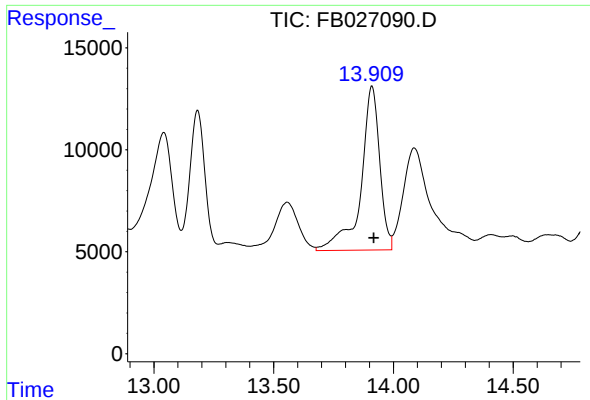

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.008 min
Response: 438348
Conc: 24.20 ng/ml

Instrument :
FID_B
ClientSampleId :

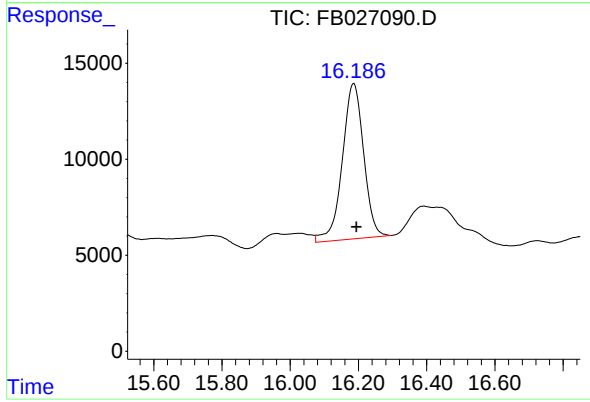

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.008 min
Response: 350532
Conc: 19.02 ng/ml