

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
 Data File : FB027091.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2022 17:51
 Operator : AJ/MA
 Sample : N2431-05
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 28 04:09:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.850	37969	3.359 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.694	21998	1.169 ng/ml
2) t 2,2,4-Trimethylpentane	7.365	8474	0.424 ng/ml
3) t n-Heptane	7.749	102007	5.215 ng/ml
4) t Benzene	7.900	3369	0.153 ng/ml
6) t Toluene	10.623	26323	1.277 ng/ml
7) t Ethylbenzene	13.039	10222	0.535 ng/ml
8) t m-Xylene	13.176	2793	0.148 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
Data File : FB027091.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2022 17:51
Operator : AJ/MA
Sample : N2431-05
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 28 04:09:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

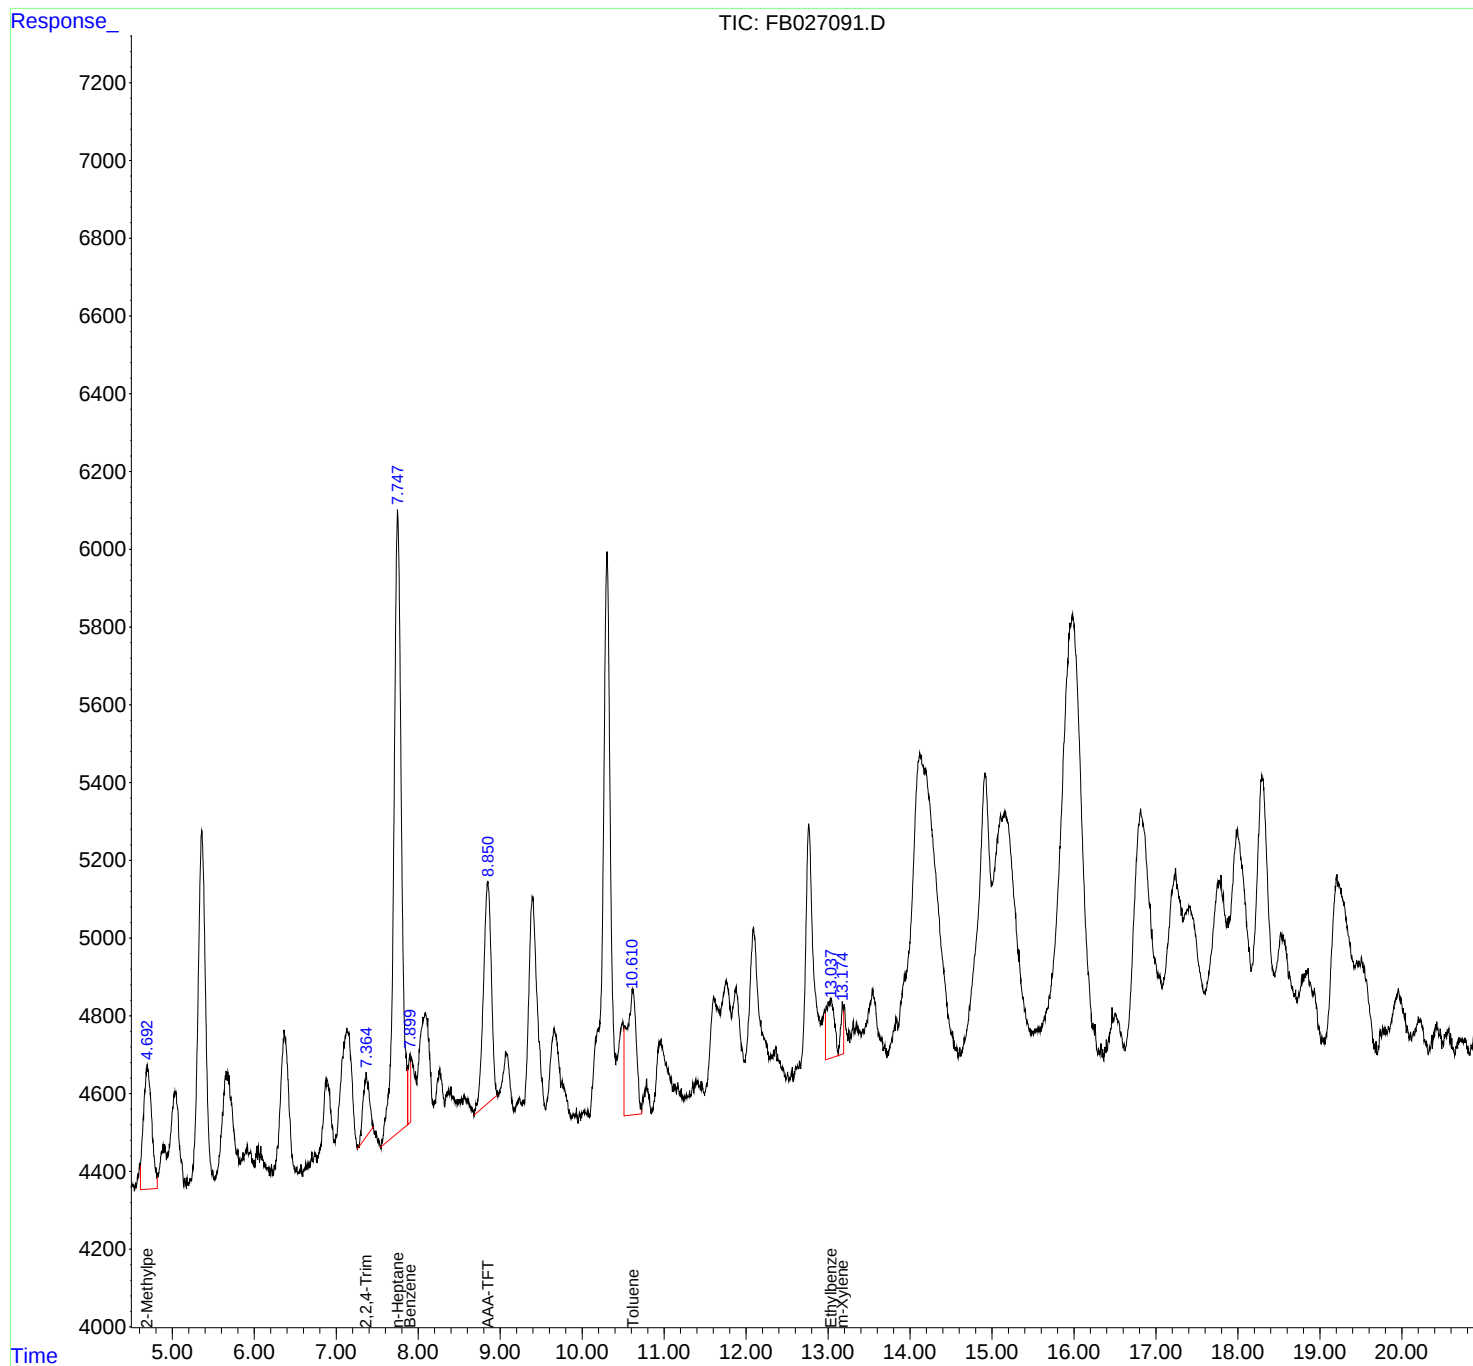


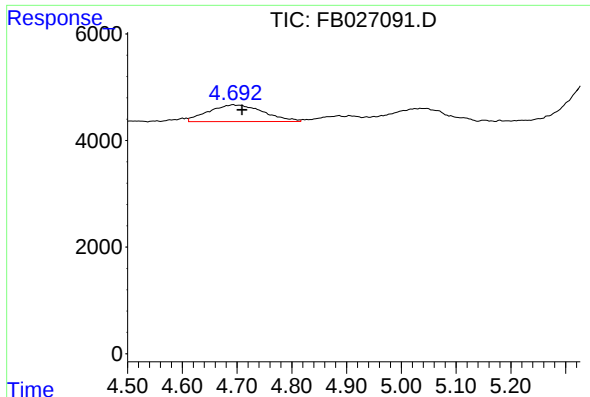

#1 2-Methylpentane


R.T.: 4.694 min
Delta R.T.: -0.015 min
Response: 21998
Conc: 1.17 ng/ml

Instrument :
FID_B
ClientSampleId :

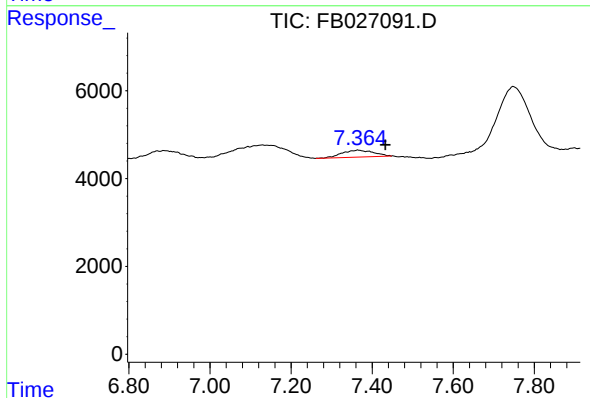


#2 2,2,4-Trimethylpentane

R.T.: 7.365 min
Delta R.T.: -0.068 min
Response: 8474
Conc: 0.42 ng/ml

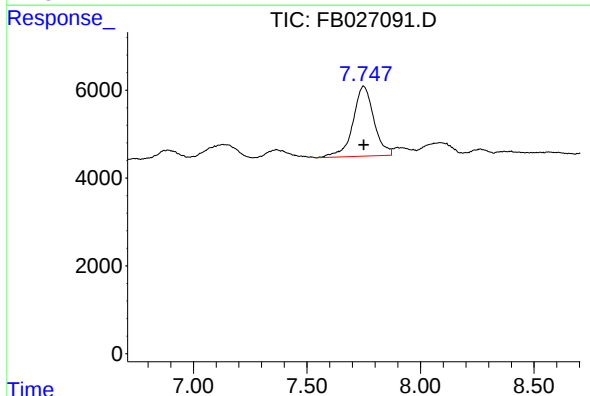


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 102007
Conc: 5.21 ng/ml

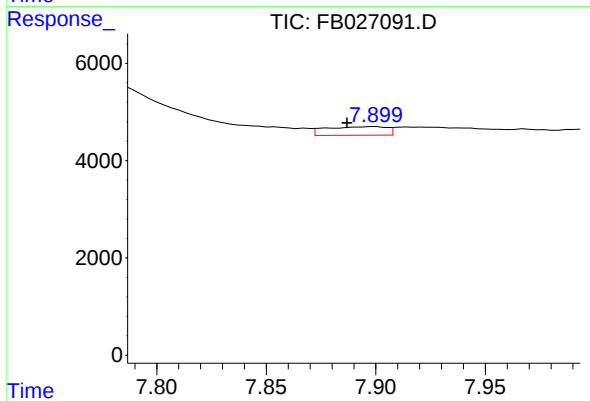

#4 Benzene


R.T.: 7.900 min
Delta R.T.: 0.013 min
Response: 3369
Conc: 0.15 ng/ml

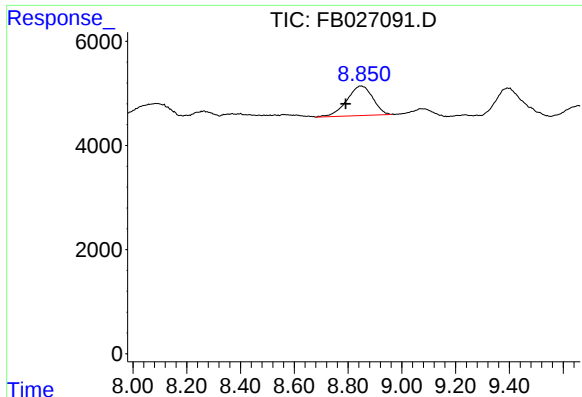

#5 AAA-TFT


R.T.: 8.850 min
Delta R.T.: 0.058 min
Response: 37969
Conc: 3.36 ng/ml

Instrument :
FID_B
ClientSampleId :

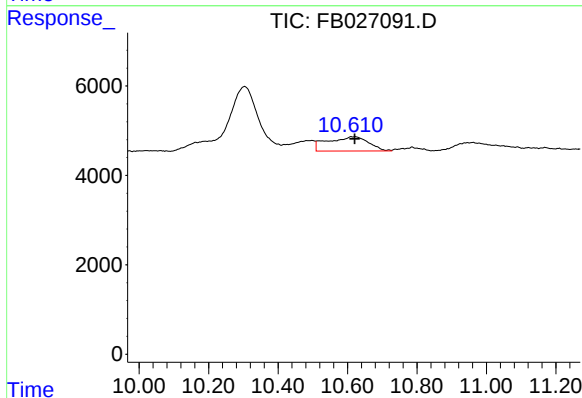


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.002 min
Response: 26323
Conc: 1.28 ng/ml

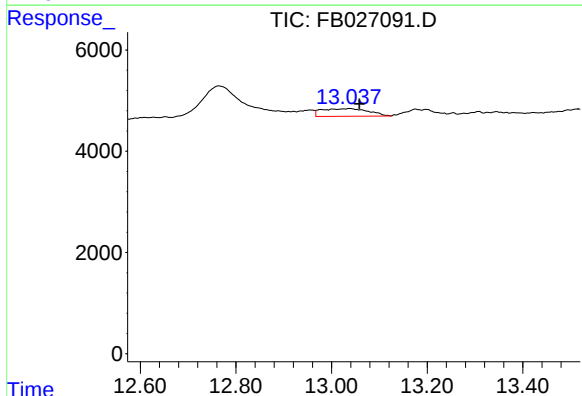

#7 Ethylbenzene

R.T.: 13.039 min
Delta R.T.: -0.019 min
Response: 10222
Conc: 0.54 ng/ml

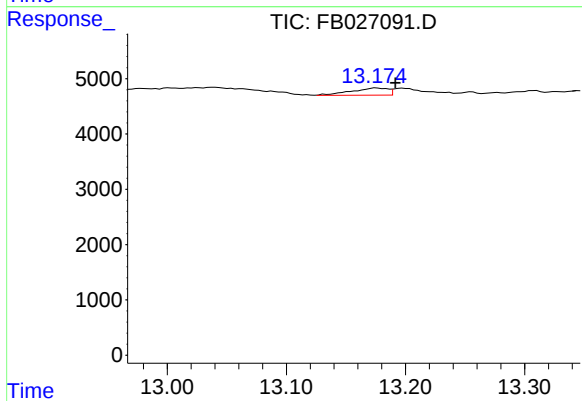

#8 m-Xylene

R.T.: 13.176 min
Delta R.T.: -0.015 min
Response: 2793
Conc: 0.15 ng/ml