

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
 Data File : FB027092.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2022 18:27
 Operator : AJ/MA
 Sample : N2431-05
 Misc : 5.05G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 28 04:09:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.846	811505	71.780 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	368203	19.561 ng/ml
2) t 2,2,4-Trimethylpentane	7.373	228755	11.435 ng/ml
3) t n-Heptane	7.748	1854666	94.811 ng/ml
4) t Benzene	7.904	280740	12.721 ng/ml
6) t Toluene	10.618	1084669	52.603 ng/ml
7) t Ethylbenzene	13.051	728504	38.128 ng/ml
8) t m-Xylene	13.183	507384	26.860 ng/ml
9) t O-Xylene	13.913	300898	16.612 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	351414	19.066 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
Data File : FB027092.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2022 18:27
Operator : AJ/MA
Sample : N2431-05
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 28 04:09:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

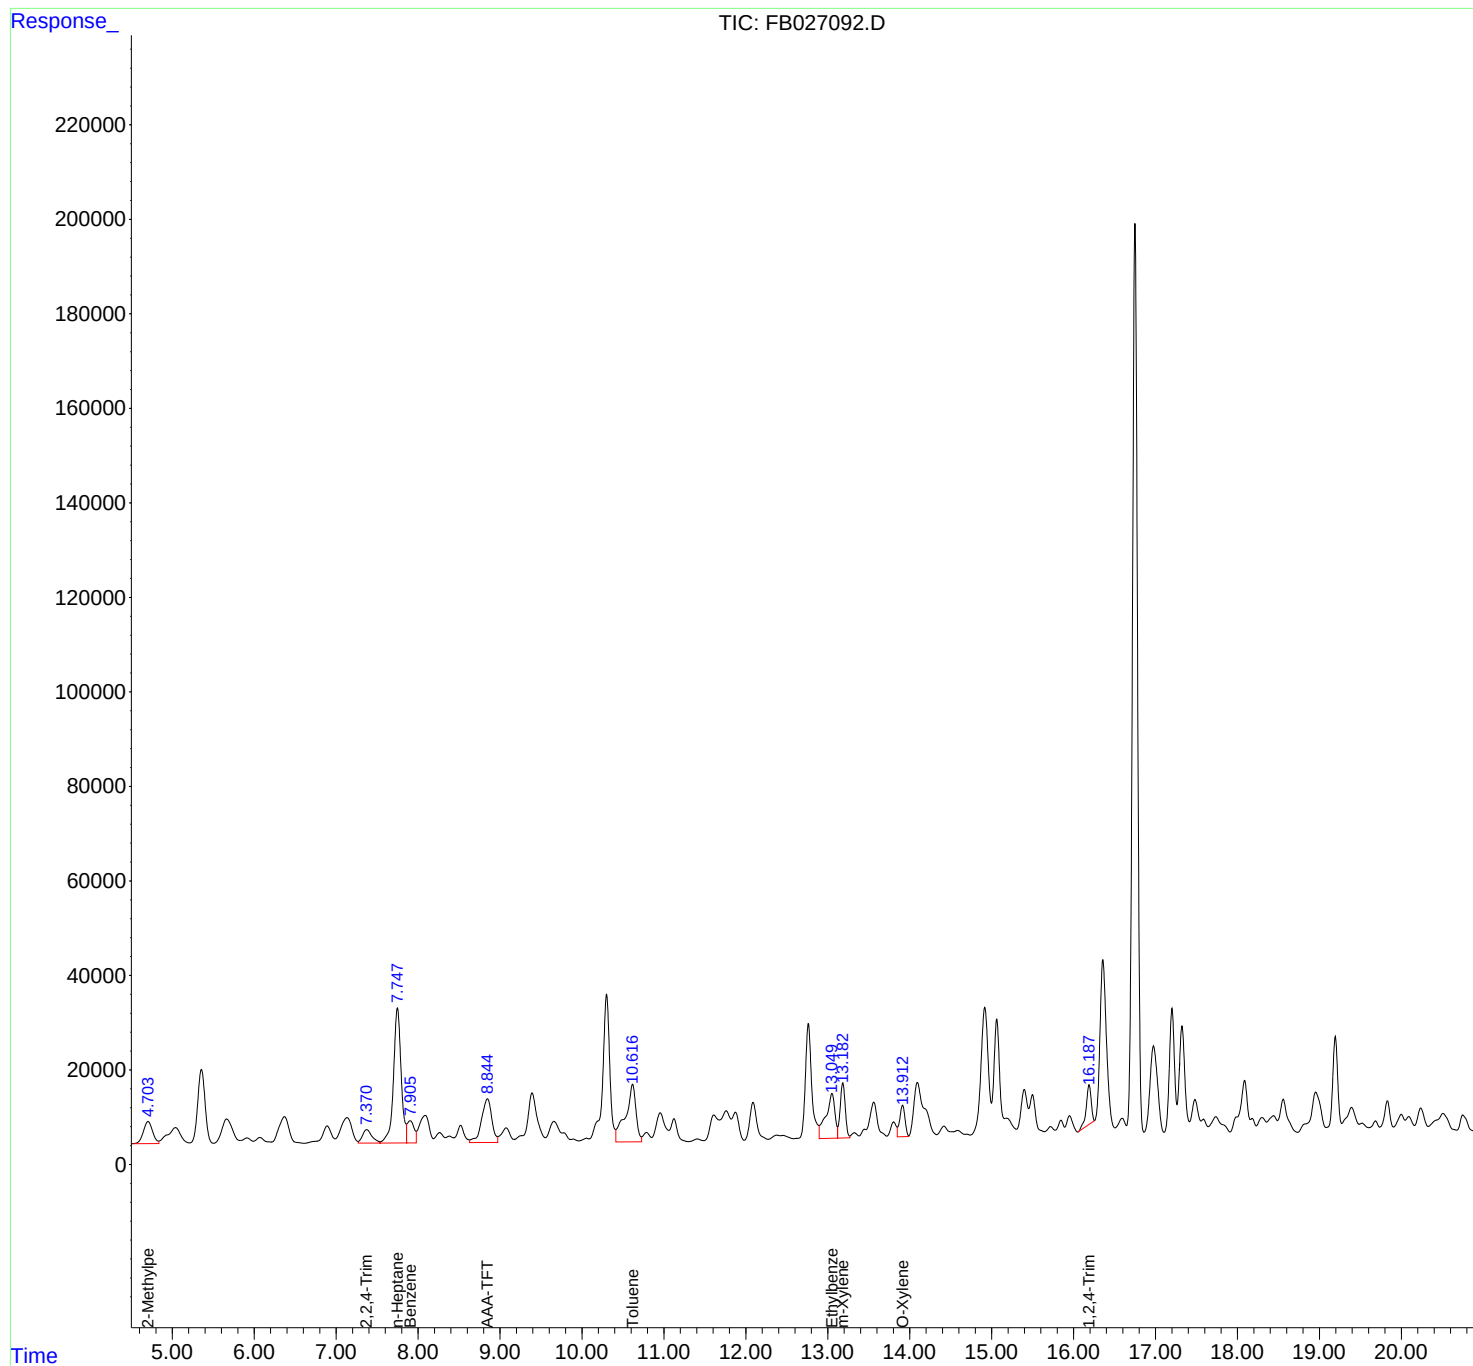


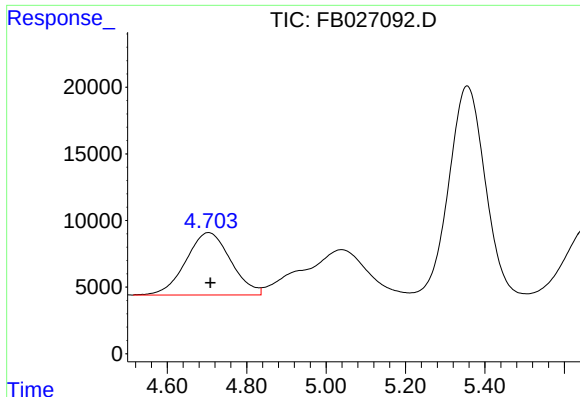

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.004 min
Response: 368203
Conc: 19.56 ng/ml

Instrument : FID_B
ClientSampleId :

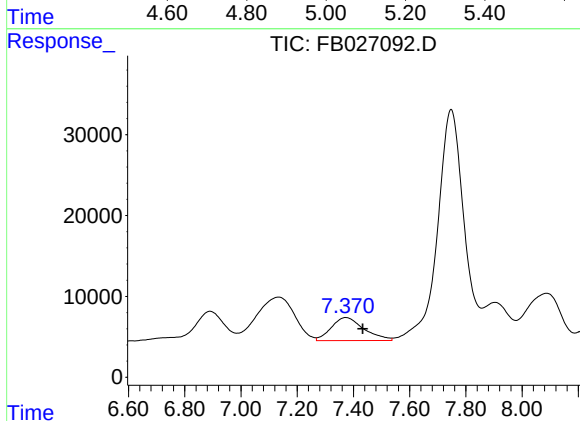


#2 2,2,4-Trimethylpentane

R.T.: 7.373 min
Delta R.T.: -0.060 min
Response: 228755
Conc: 11.43 ng/ml

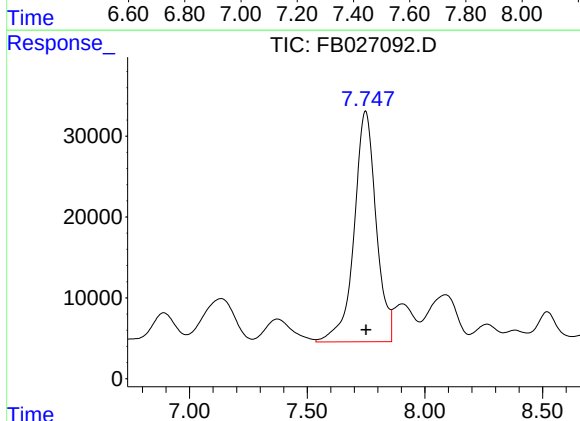


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 1854666
Conc: 94.81 ng/ml

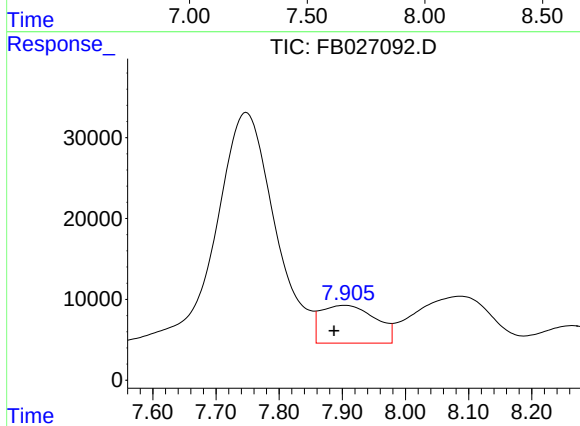

#4 Benzene


R.T.: 7.904 min
Delta R.T.: 0.017 min
Response: 280740
Conc: 12.72 ng/ml

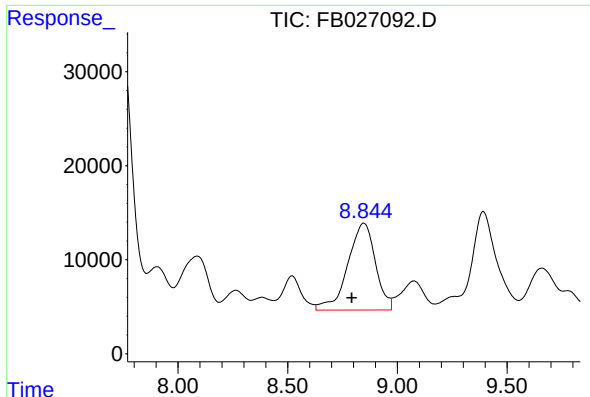

#5 AAA-TFT


R.T.: 8.846 min
Delta R.T.: 0.054 min
Response: 811505
Conc: 71.78 ng/ml

Instrument :
FID_B
ClientSampleId :

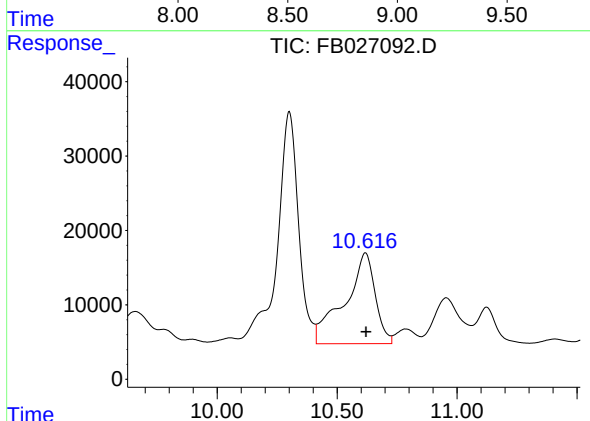


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 1084669
Conc: 52.60 ng/ml

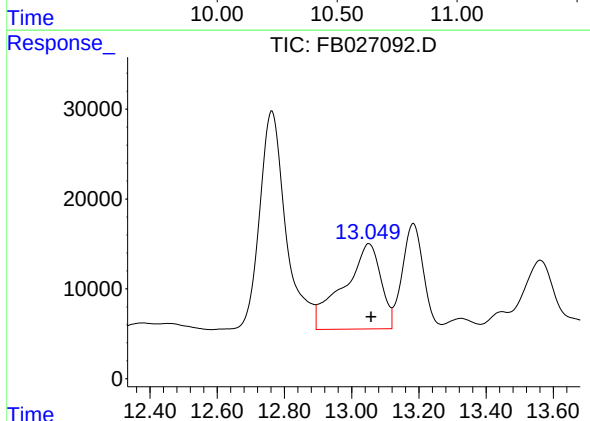


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: -0.007 min
Response: 728504
Conc: 38.13 ng/ml

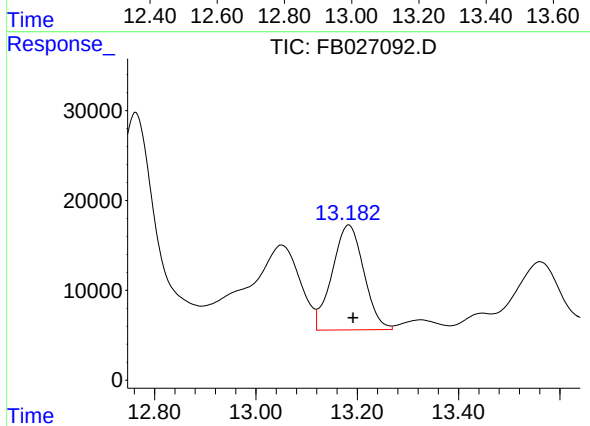

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: -0.008 min
Response: 507384
Conc: 26.86 ng/ml

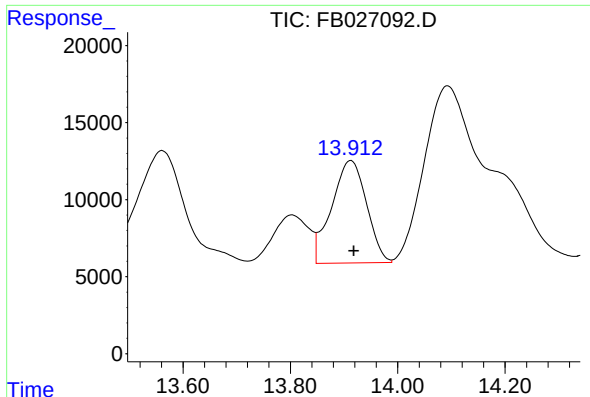

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.006 min
Response: 300898
Conc: 16.61 ng/ml

Instrument :
FID_B
ClientSampleId :

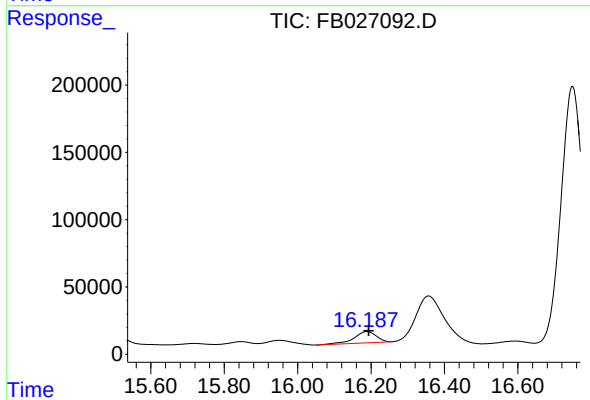

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 351414
Conc: 19.07 ng/ml