

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
 Data File : FB027083.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2022 11:22
 Operator : AJ/MA
 Sample : BSF0427S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0427S1

Integration File: autoint1.e
 Quant Time: Apr 28 04:07:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	260527	23.044 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	445908	23.689 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	503653	25.176 ng/ml
3) t n-Heptane	7.747	152802	7.811 ng/ml
4) t Benzene	7.884	194059	8.793 ng/ml
6) t Toluene	10.617	562009	27.256 ng/ml
7) t Ethylbenzene	13.055	183055	9.581 ng/ml
8) t m-Xylene	13.187	353904	18.735 ng/ml
9) t O-Xylene	13.914	348623	19.246 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	358645	19.458 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
Data File : FB027083.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2022 11:22
Operator : AJ/MA
Sample : BSF0427S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0427S1

Integration File: autoint1.e
Quant Time: Apr 28 04:07:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

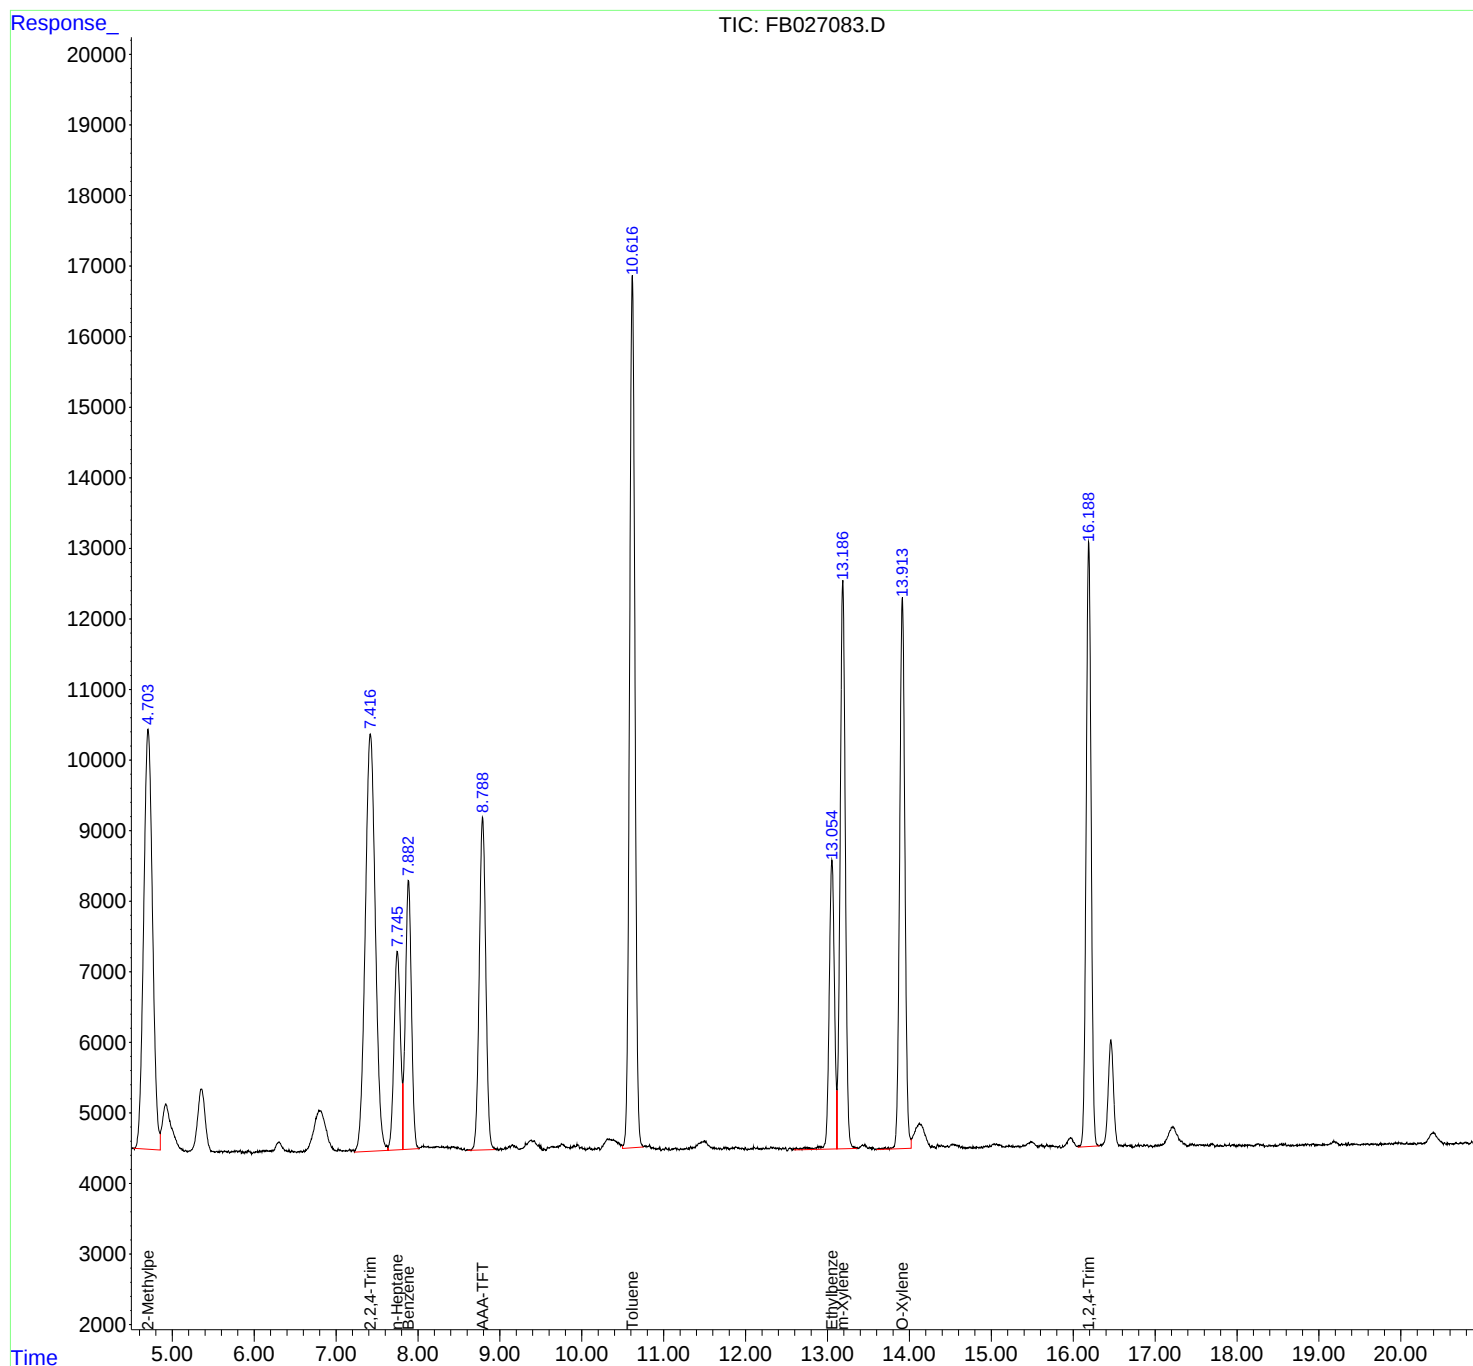


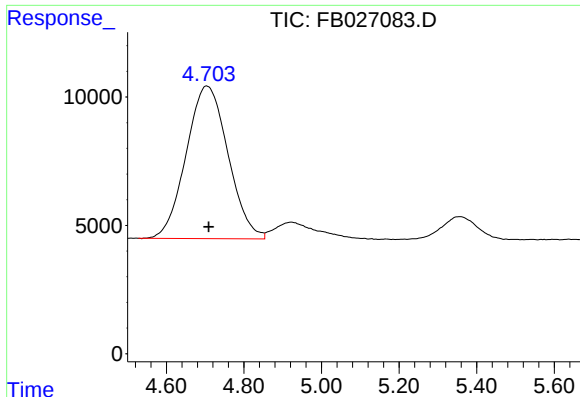

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.005 min
Response: 445908
Conc: 23.69 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S1

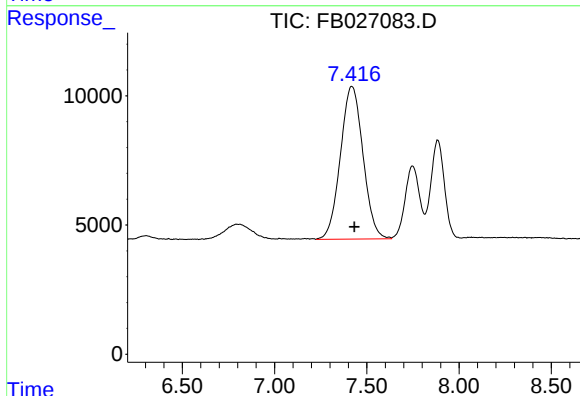


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.015 min
Response: 503653
Conc: 25.18 ng/ml

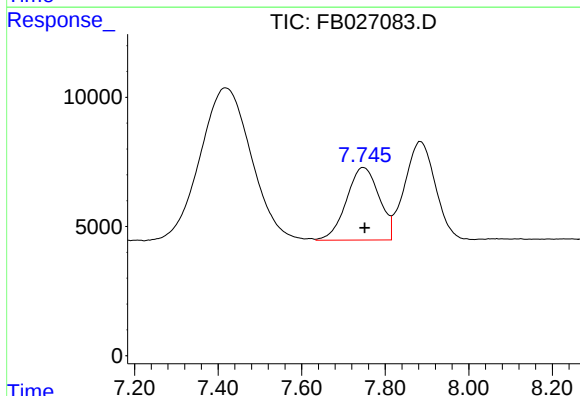


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.004 min
Response: 152802
Conc: 7.81 ng/ml

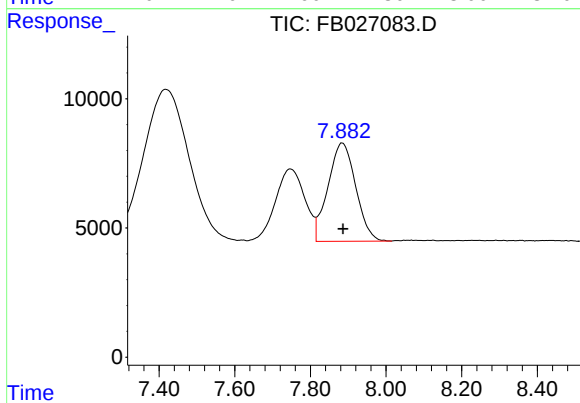

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.003 min
Response: 194059
Conc: 8.79 ng/ml

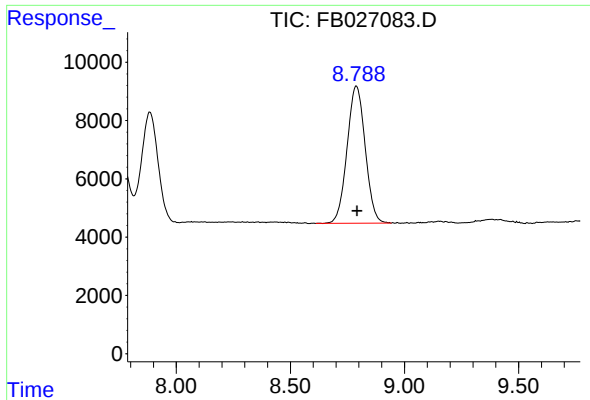

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 260527
Conc: 23.04 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S1

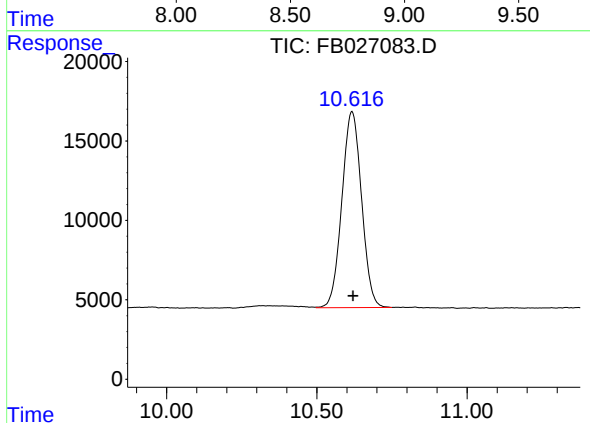


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.003 min
Response: 562009
Conc: 27.26 ng/ml

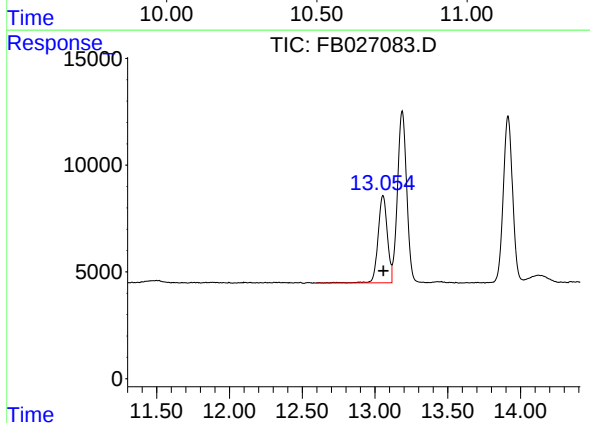


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.004 min
Response: 183055
Conc: 9.58 ng/ml

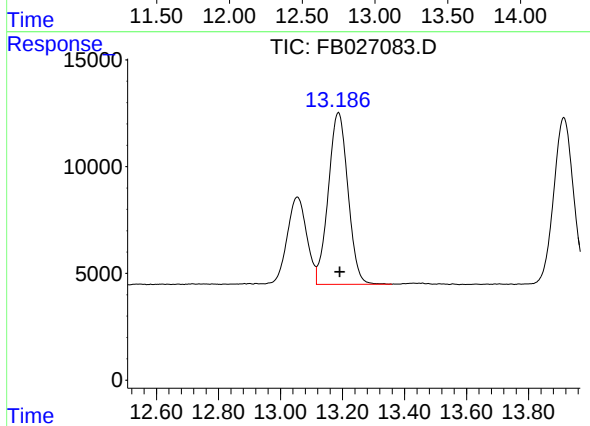

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.004 min
Response: 353904
Conc: 18.74 ng/ml

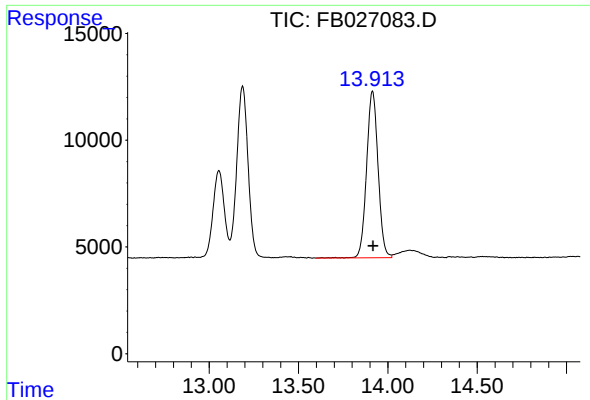

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.004 min
Response: 348623
Conc: 19.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S1

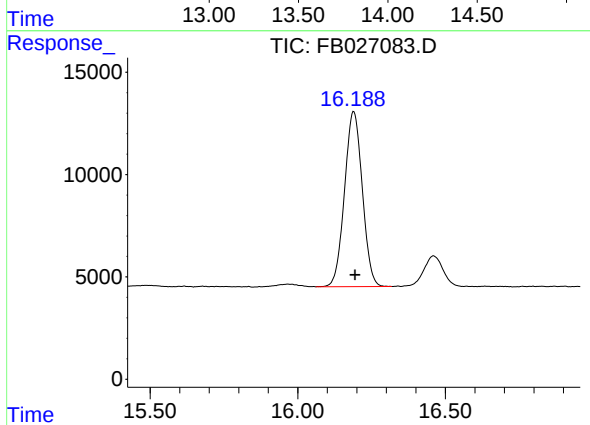

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 358645
Conc: 19.46 ng/ml