

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
 Data File : FB027088.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2022 14:33
 Operator : AJ/MA
 Sample : BSF0427S2
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0427S2

Integration File: autoint1.e
 Quant Time: Apr 28 04:07:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	204151	18.058 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	448439	23.823 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	503747	25.180 ng/ml
3) t n-Heptane	7.748	152418	7.792 ng/ml
4) t Benzene	7.885	197719	8.959 ng/ml
6) t Toluene	10.618	556908	27.008 ng/ml
7) t Ethylbenzene	13.055	174048	9.109 ng/ml
8) t m-Xylene	13.188	346758	18.357 ng/ml
9) t O-Xylene	13.915	359841	19.866 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	356173	19.324 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
Data File : FB027088.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2022 14:33
Operator : AJ/MA
Sample : BSF0427S2
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0427S2

Integration File: autoint1.e
Quant Time: Apr 28 04:07:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

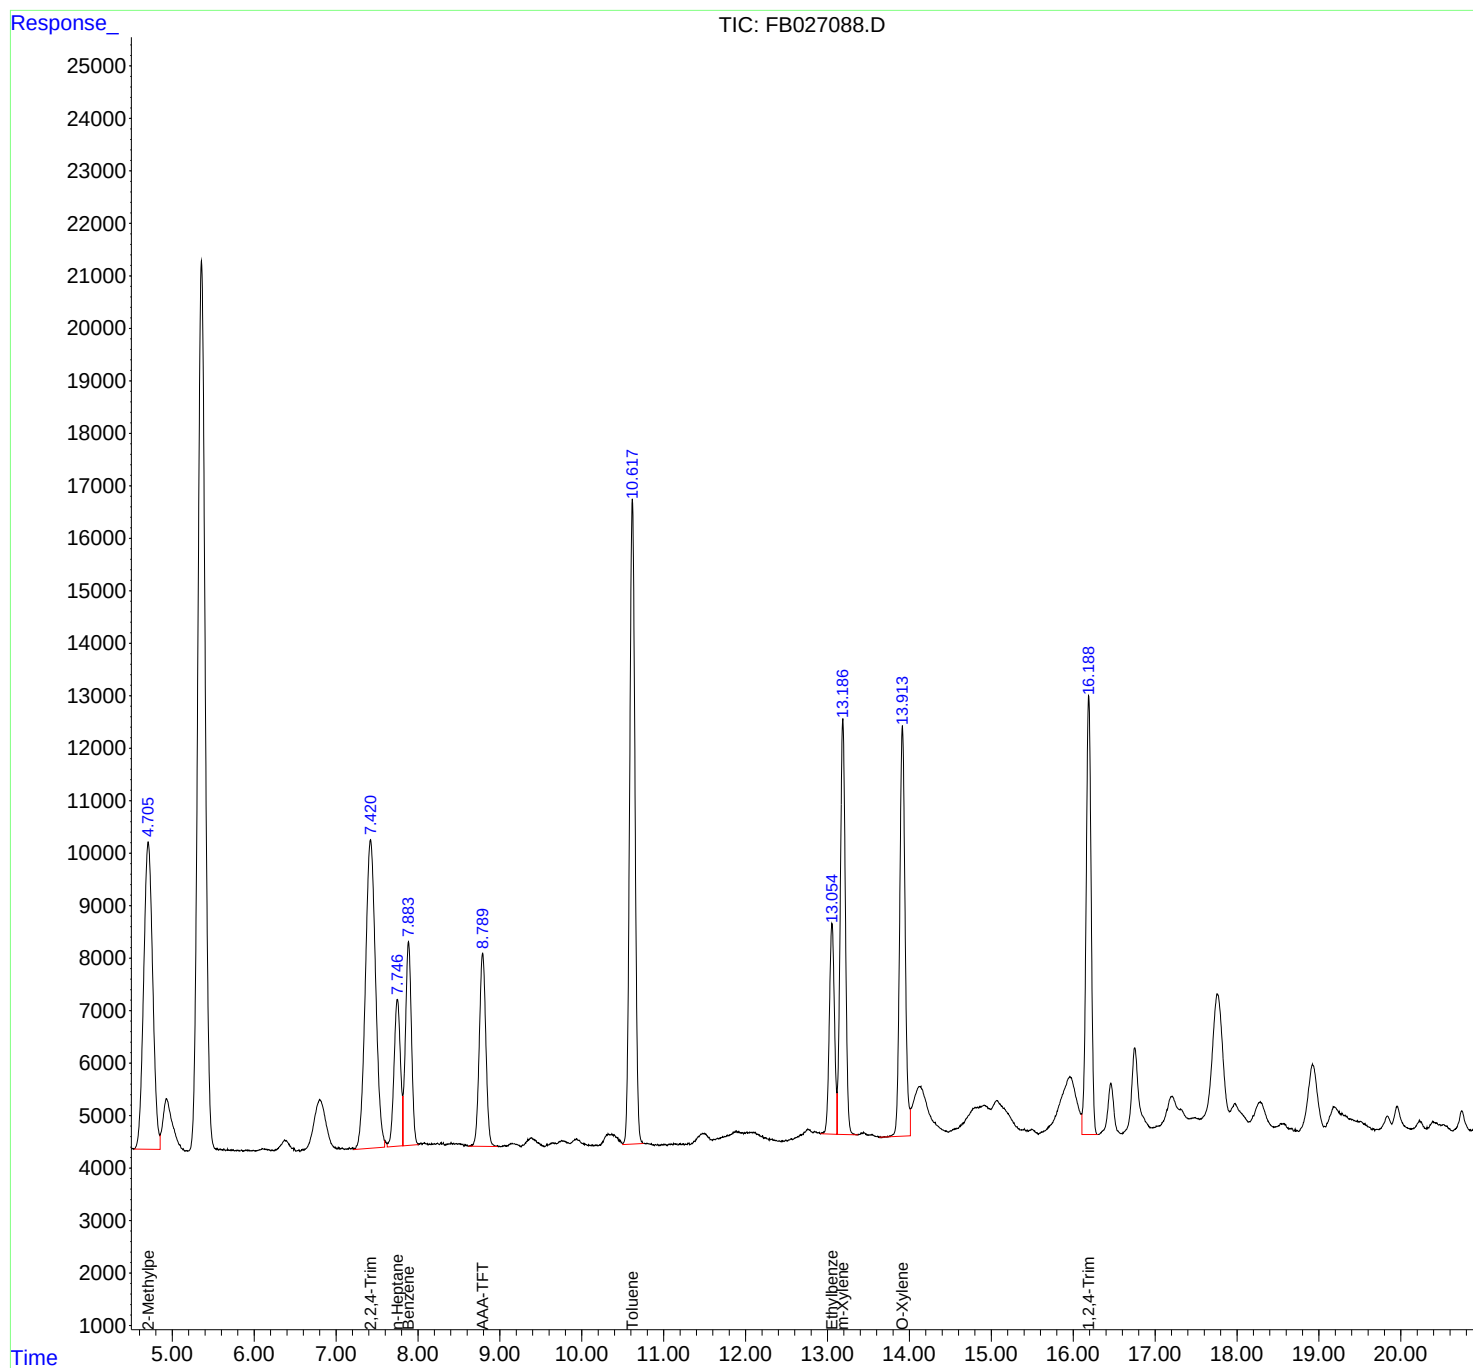


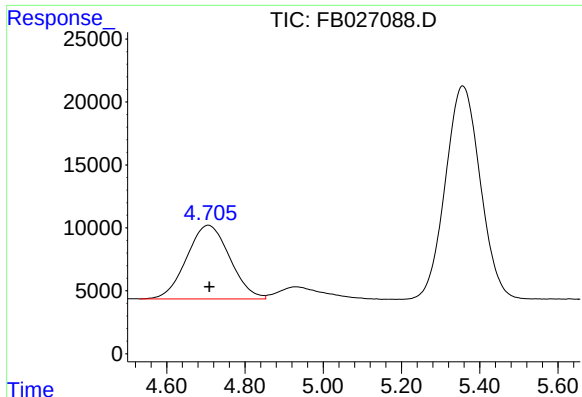

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.002 min
Response: 448439
Conc: 23.82 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S2

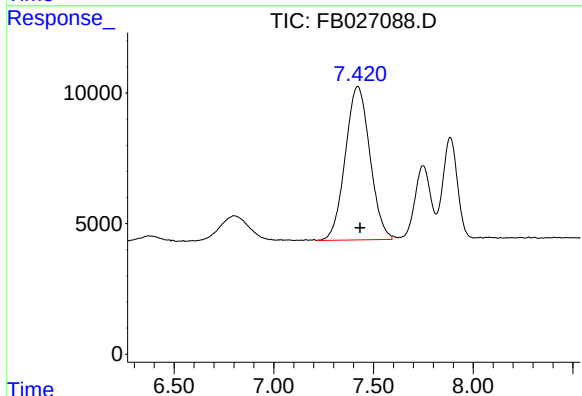


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: -0.012 min
Response: 503747
Conc: 25.18 ng/ml

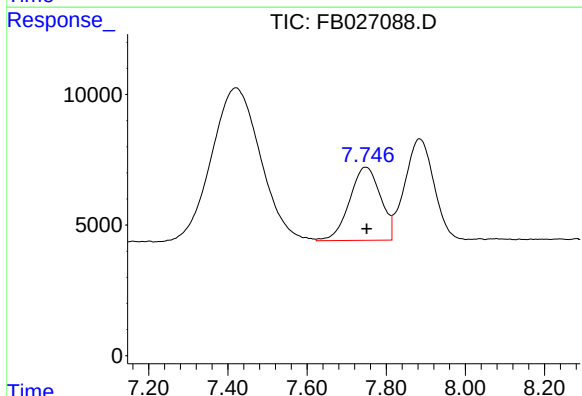


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 152418
Conc: 7.79 ng/ml

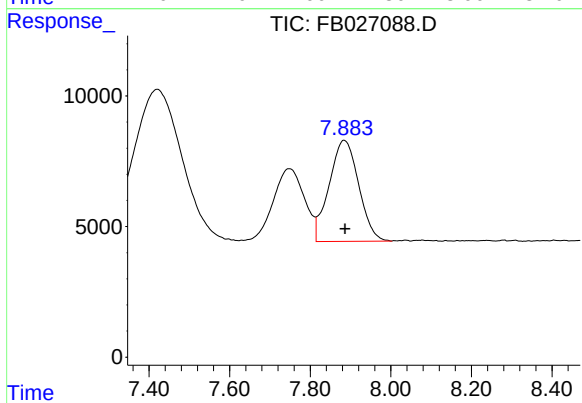

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 197719
Conc: 8.96 ng/ml

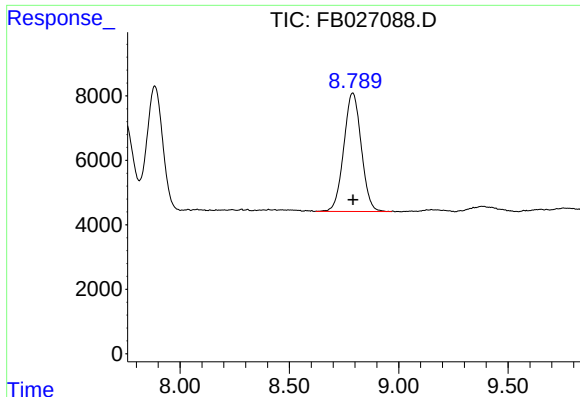

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 204151
Conc: 18.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S2

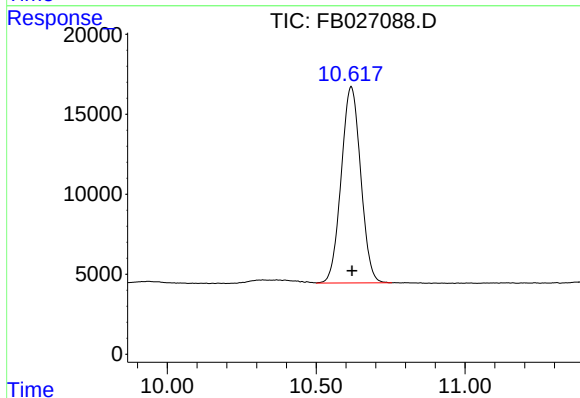


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 556908
Conc: 27.01 ng/ml

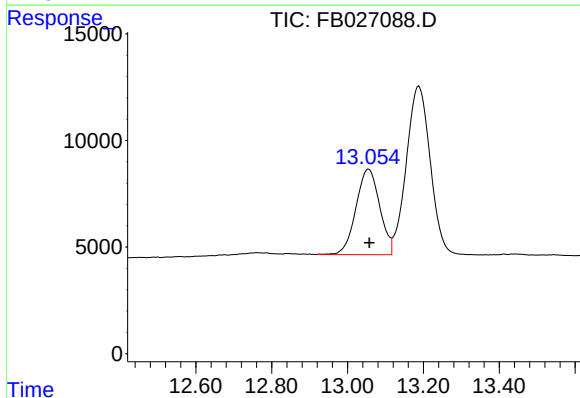


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.003 min
Response: 174048
Conc: 9.11 ng/ml

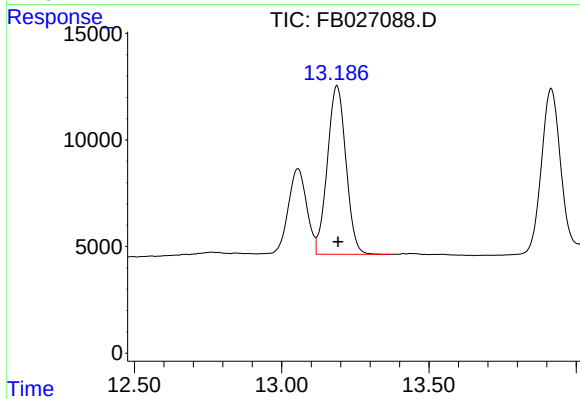

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.004 min
Response: 346758
Conc: 18.36 ng/ml

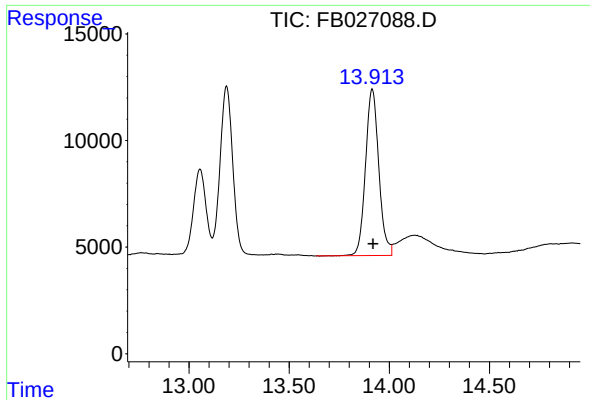

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.003 min
Response: 359841
Conc: 19.87 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S2

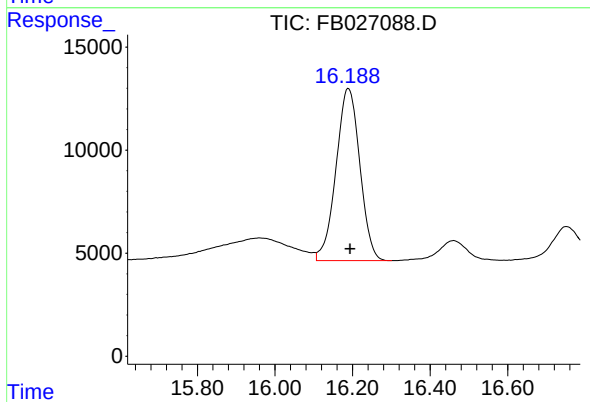

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 356173
Conc: 19.32 ng/ml