

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
 Data File : FB027093.D
 Signal(s) : FID2B.CH
 Acq On : 27 Apr 2022 19:03
 Operator : AJ/MA
 Sample : BSF0427S3
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0427S3

Integration File: autoint1.e
 Quant Time: Apr 28 04:09:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	252629	22.346 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	403116	21.415 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	447734	22.380 ng/ml
3) t n-Heptane	7.750	136021	6.953 ng/ml
4) t Benzene	7.885	178867	8.105 ng/ml
6) t Toluene	10.617	512272	24.844 ng/ml
7) t Ethylbenzene	13.054	163718	8.569 ng/ml
8) t m-Xylene	13.187	322006	17.047 ng/ml
9) t O-Xylene	13.915	317620	17.535 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	325006	17.633 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042722\
Data File : FB027093.D
Signal(s) : FID2B.CH
Acq On : 27 Apr 2022 19:03
Operator : AJ/MA
Sample : BSF0427S3
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0427S3

Integration File: autoint1.e
Quant Time: Apr 28 04:09:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

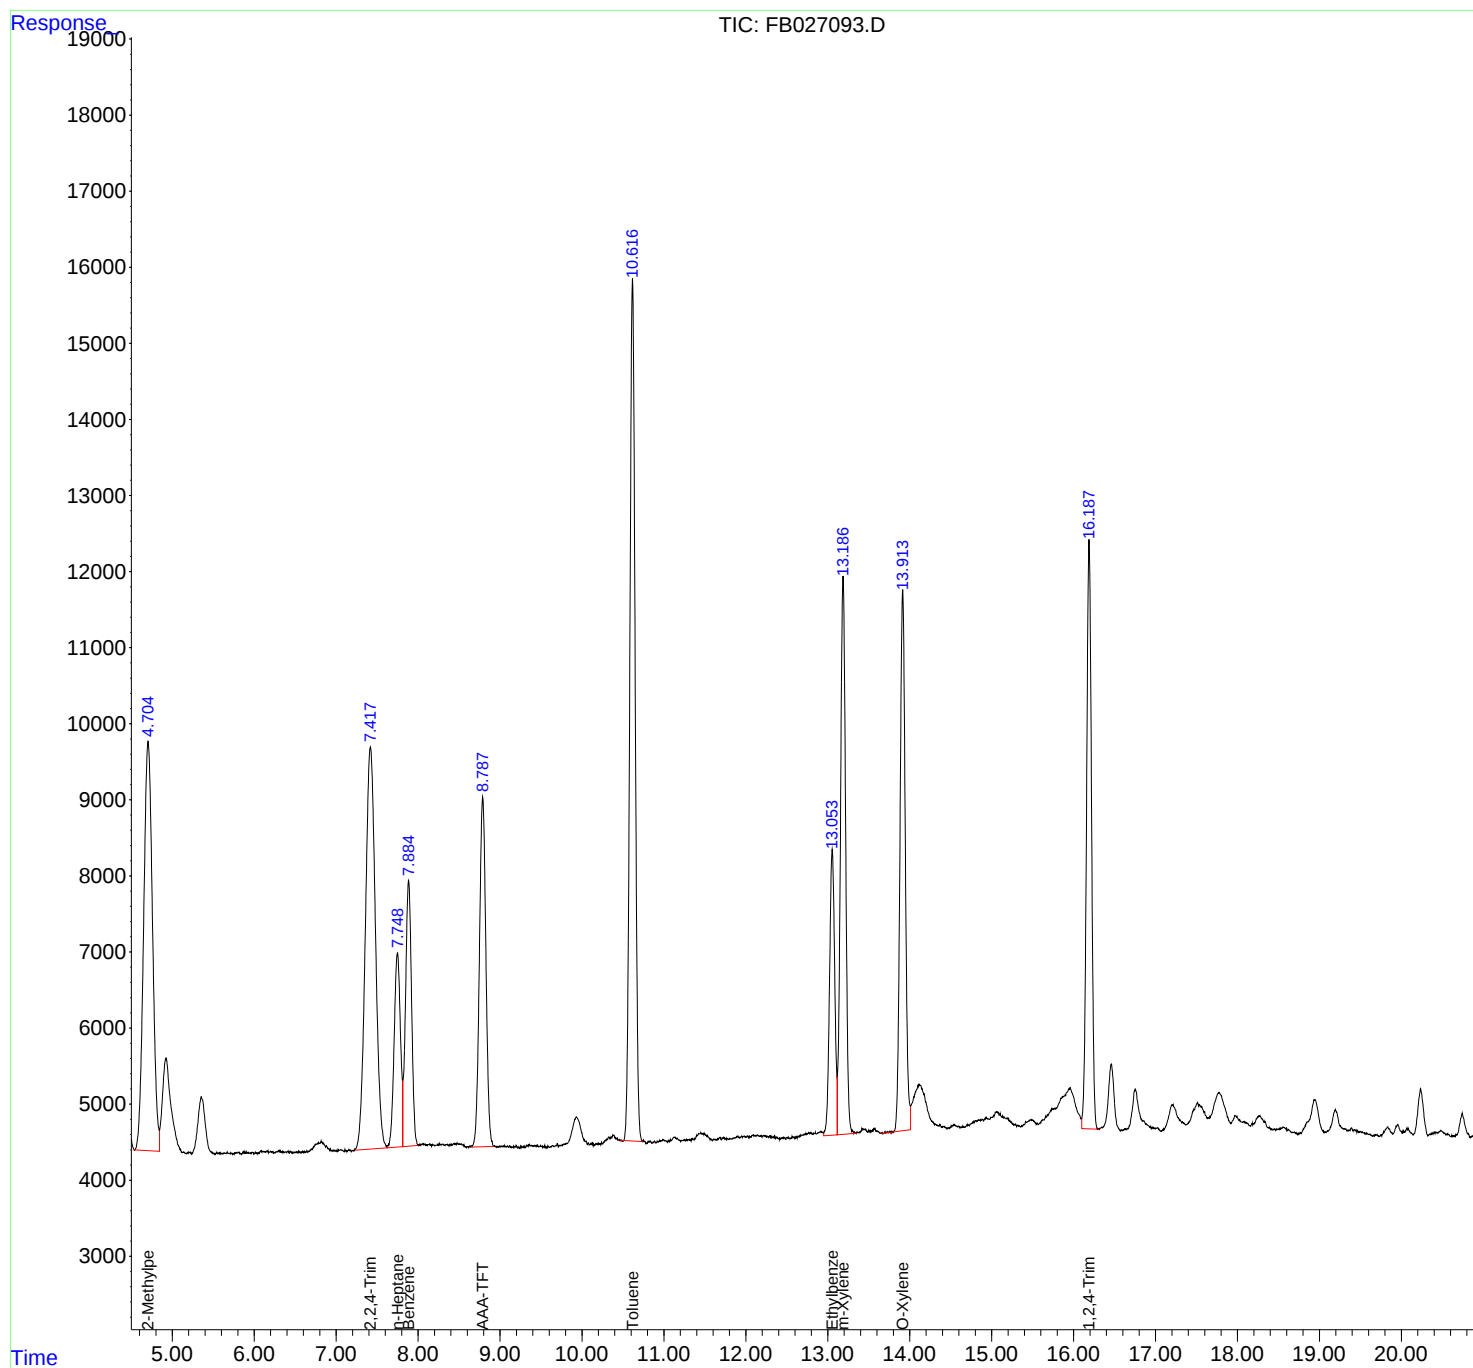


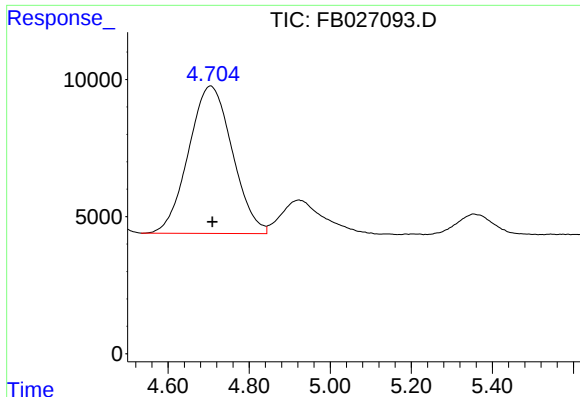

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.003 min
Response: 403116
Conc: 21.42 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S3

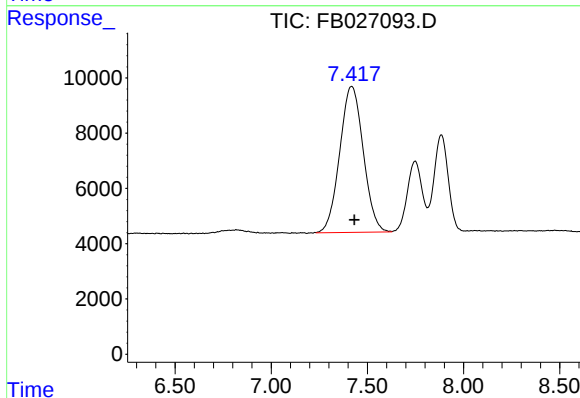


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.014 min
Response: 447734
Conc: 22.38 ng/ml

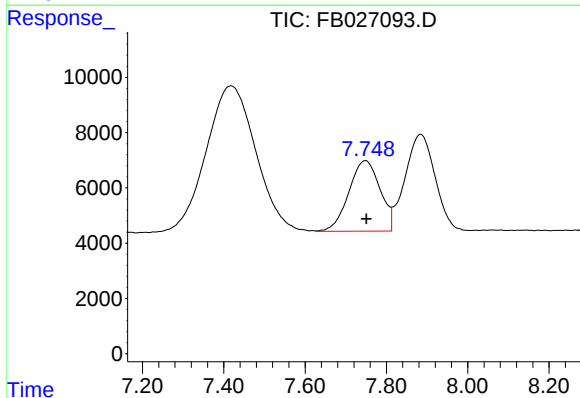


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.001 min
Response: 136021
Conc: 6.95 ng/ml

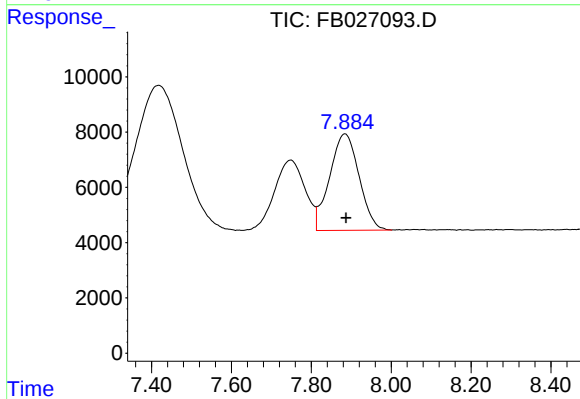

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 178867
Conc: 8.10 ng/ml

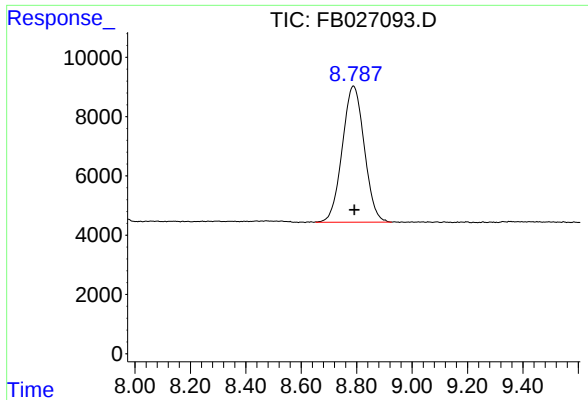

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 252629
Conc: 22.35 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S3

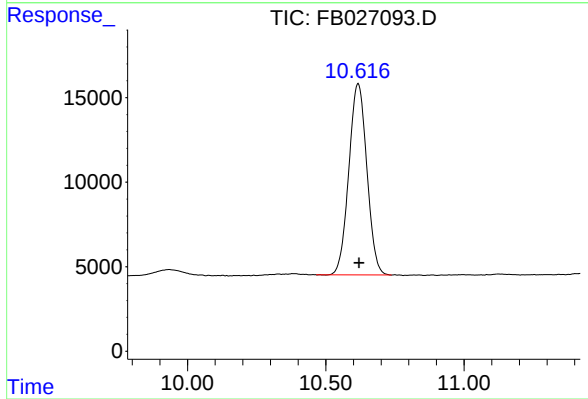


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.004 min
Response: 512272
Conc: 24.84 ng/ml

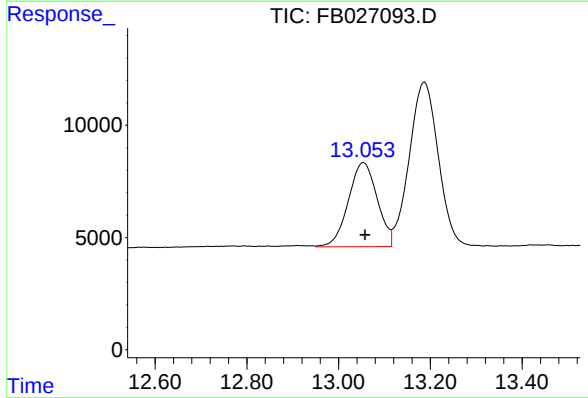


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.004 min
Response: 163718
Conc: 8.57 ng/ml

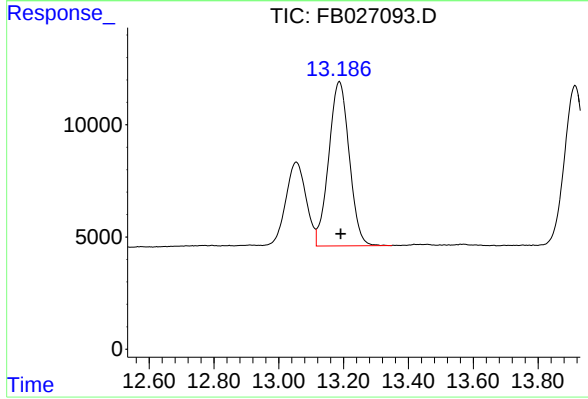

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.004 min
Response: 322006
Conc: 17.05 ng/ml

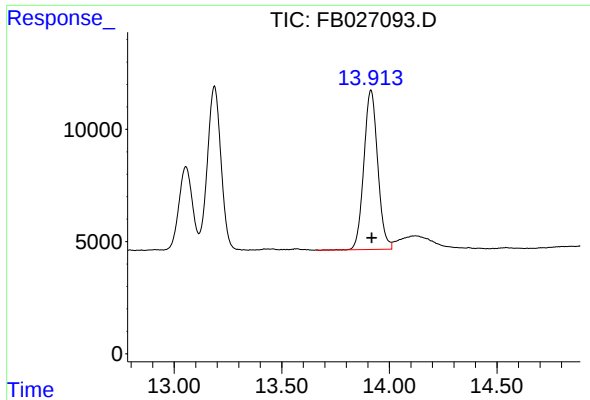

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.004 min
Response: 317620
Conc: 17.53 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0427S3

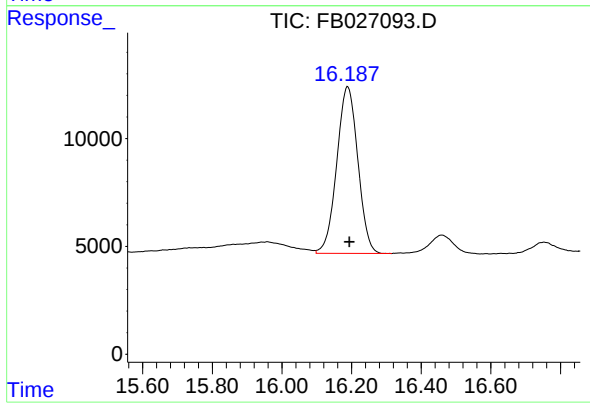

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 325006
Conc: 17.63 ng/ml