

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042821\
 Data File : FB025674.D
 Signal(s) : FID2B.CH
 Acq On : 28 Apr 2021 12:44
 Operator : DD/AJ
 Sample : M2149-14MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 29 00:23:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.243	386069	19.632 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.210	670849	27.730 ng/ml
2) t 2,2,4-Trimethylpentane	7.903	624349	33.571 ng/ml
3) t n-Heptane	8.221	292057	9.968 ng/ml
4) t Benzene	8.372	367931	9.523 ng/ml
6) t Toluene	11.063	1052348	29.157 ng/ml
7) t Ethylbenzene	13.470	345117	10.066 ng/ml
8) t m-Xylene	13.600	690186	20.304 ng/ml
9) t O-Xylene	14.323	641897	19.703 ng/ml
10) t 1,2,4-Trimethylbenzene	16.576	537640	20.452 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042821\
Data File : FB025674.D
Signal(s) : FID2B.CH
Acq On : 28 Apr 2021 12:44
Operator : DD/AJ
Sample : M2149-14MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 29 00:23:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

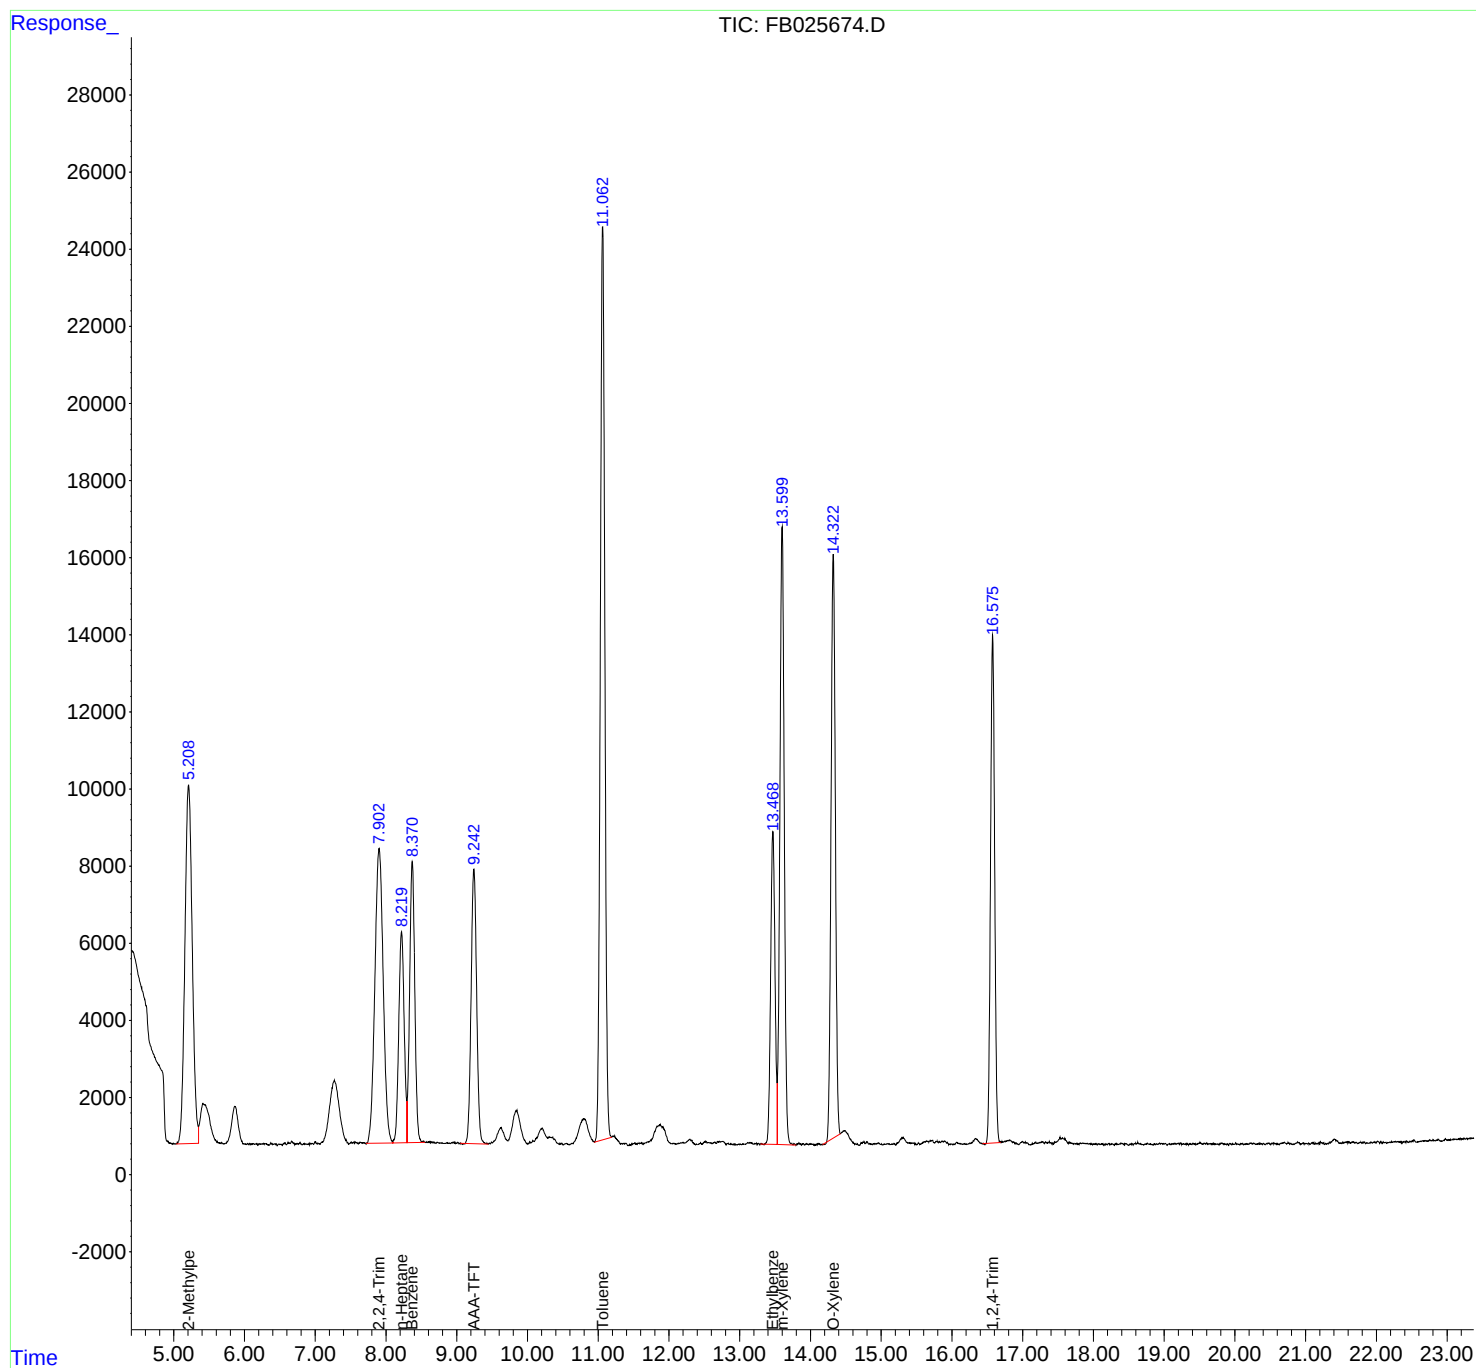


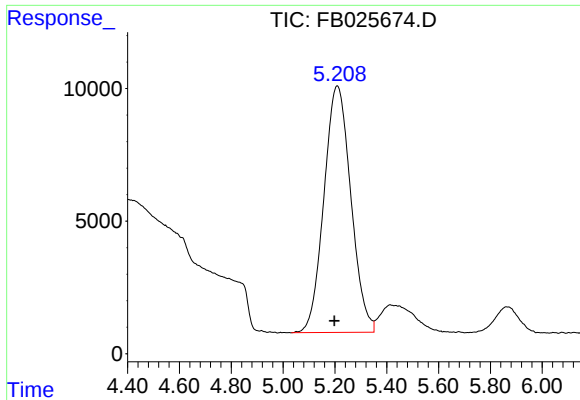

#1 2-Methylpentane


R.T.: 5.210 min
Delta R.T.: 0.012 min
Response: 670849
Conc: 27.73 ng/ml

Instrument :
FID_B
ClientSampleId :

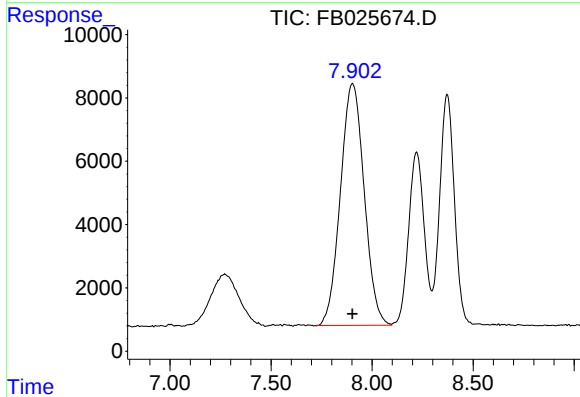


#2 2,2,4-Trimethylpentane

R.T.: 7.903 min
Delta R.T.: 0.002 min
Response: 624349
Conc: 33.57 ng/ml

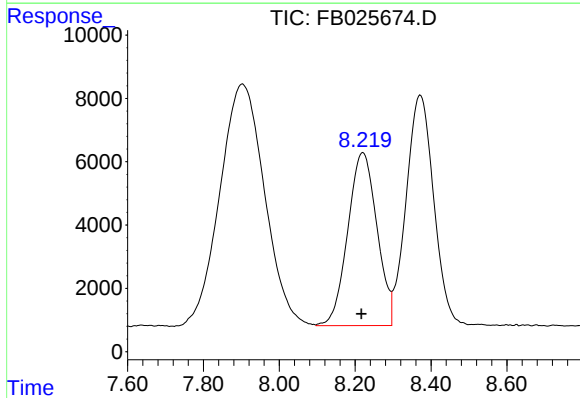


#3 n-Heptane

R.T.: 8.221 min
Delta R.T.: 0.005 min
Response: 292057
Conc: 9.97 ng/ml

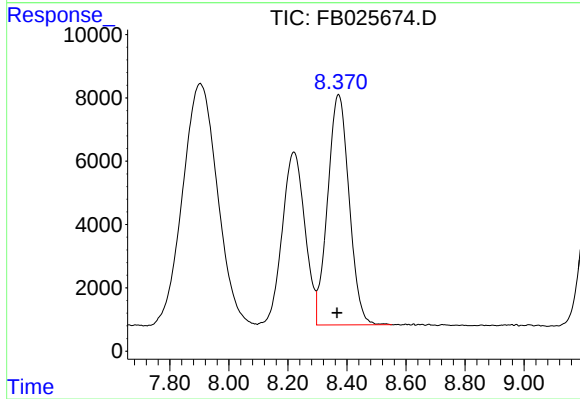

#4 Benzene


R.T.: 8.372 min
Delta R.T.: 0.005 min
Response: 367931
Conc: 9.52 ng/ml

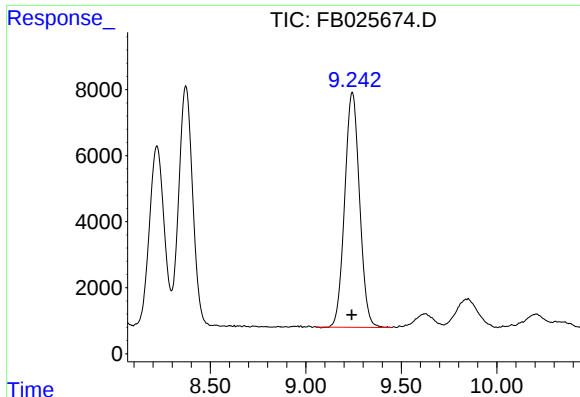

#5 AAA-TFT


R.T.: 9.243 min
Delta R.T.: 0.002 min
Response: 386069
Conc: 19.63 ng/ml

Instrument :
FID_B
ClientSampleId :

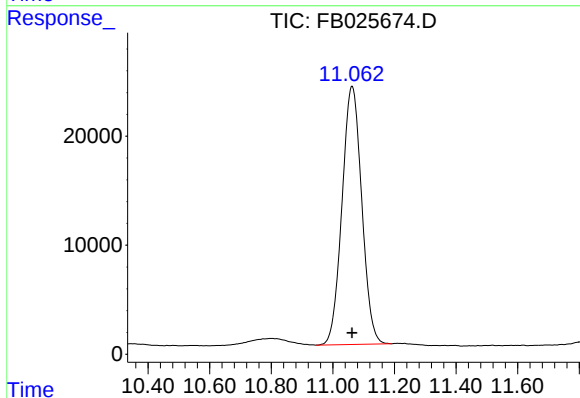


#6 Toluene

R.T.: 11.063 min
Delta R.T.: 0.000 min
Response: 1052348
Conc: 29.16 ng/ml

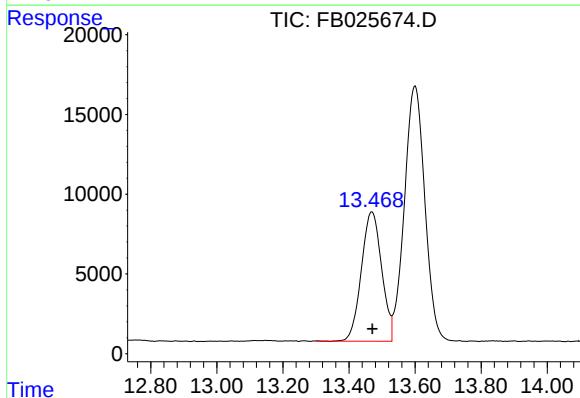


#7 Ethylbenzene

R.T.: 13.470 min
Delta R.T.: 0.000 min
Response: 345117
Conc: 10.07 ng/ml

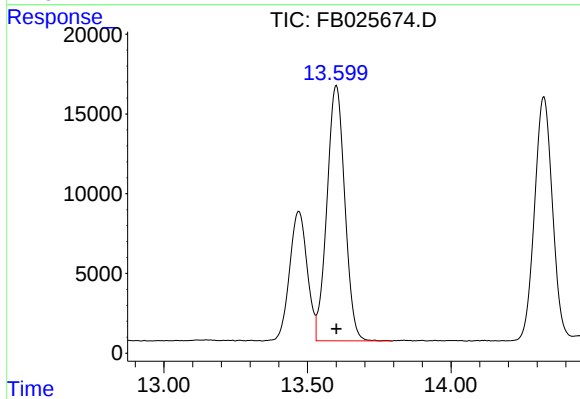

#8 m-Xylene


R.T.: 13.600 min
Delta R.T.: 0.000 min
Response: 690186
Conc: 20.30 ng/ml

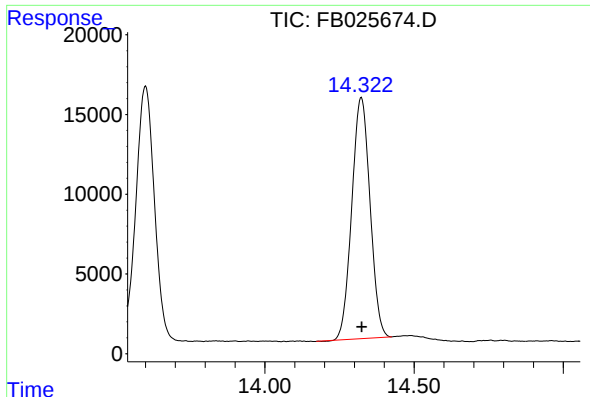

#9 O-Xylene

R.T.: 14.323 min
Delta R.T.: -0.002 min
Response: 641897
Conc: 19.70 ng/ml

Instrument :
FID_B
ClientSampleId :

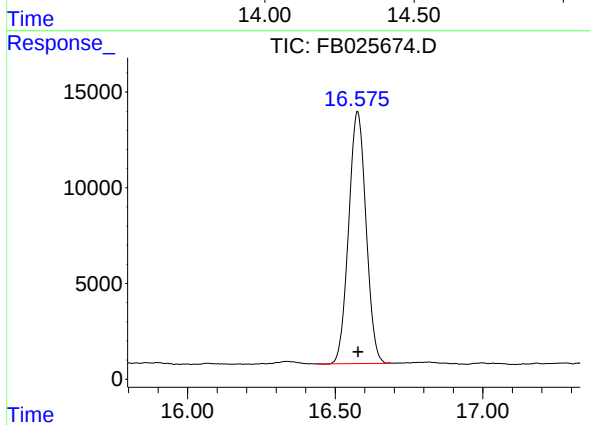

#10 1,2,4-Trimethylbenzene

R.T.: 16.576 min
Delta R.T.: -0.002 min
Response: 537640
Conc: 20.45 ng/ml