

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042821\
 Data File : FB025668.D
 Signal(s) : FID2B.CH
 Acq On : 28 Apr 2021 9:06
 Operator : DD/AJ
 Sample : BSF0428S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0428S1

Integration File: Calibration.e
 Quant Time: Apr 29 00:22:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.242	398189	20.248 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.211	696393	28.786 ng/ml
2) t 2,2,4-Trimethylpentane	7.901	649969	34.948 ng/ml
3) t n-Heptane	8.219	294525	10.052 ng/ml
4) t Benzene	8.371	366465	9.485 ng/ml
6) t Toluene	11.060	1077095	29.842 ng/ml
7) t Ethylbenzene	13.466	347828	10.145 ng/ml
8) t m-Xylene	13.597	690724	20.320 ng/ml
9) t O-Xylene	14.320	639370	19.625 ng/ml
10) t 1,2,4-Trimethylbenzene	16.573	541390	20.595 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042821\
Data File : FB025668.D
Signal(s) : FID2B.CH
Acq On : 28 Apr 2021 9:06
Operator : DD/AJ
Sample : BSF0428S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0428S1

Integration File: Calibration.e
Quant Time: Apr 29 00:22:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

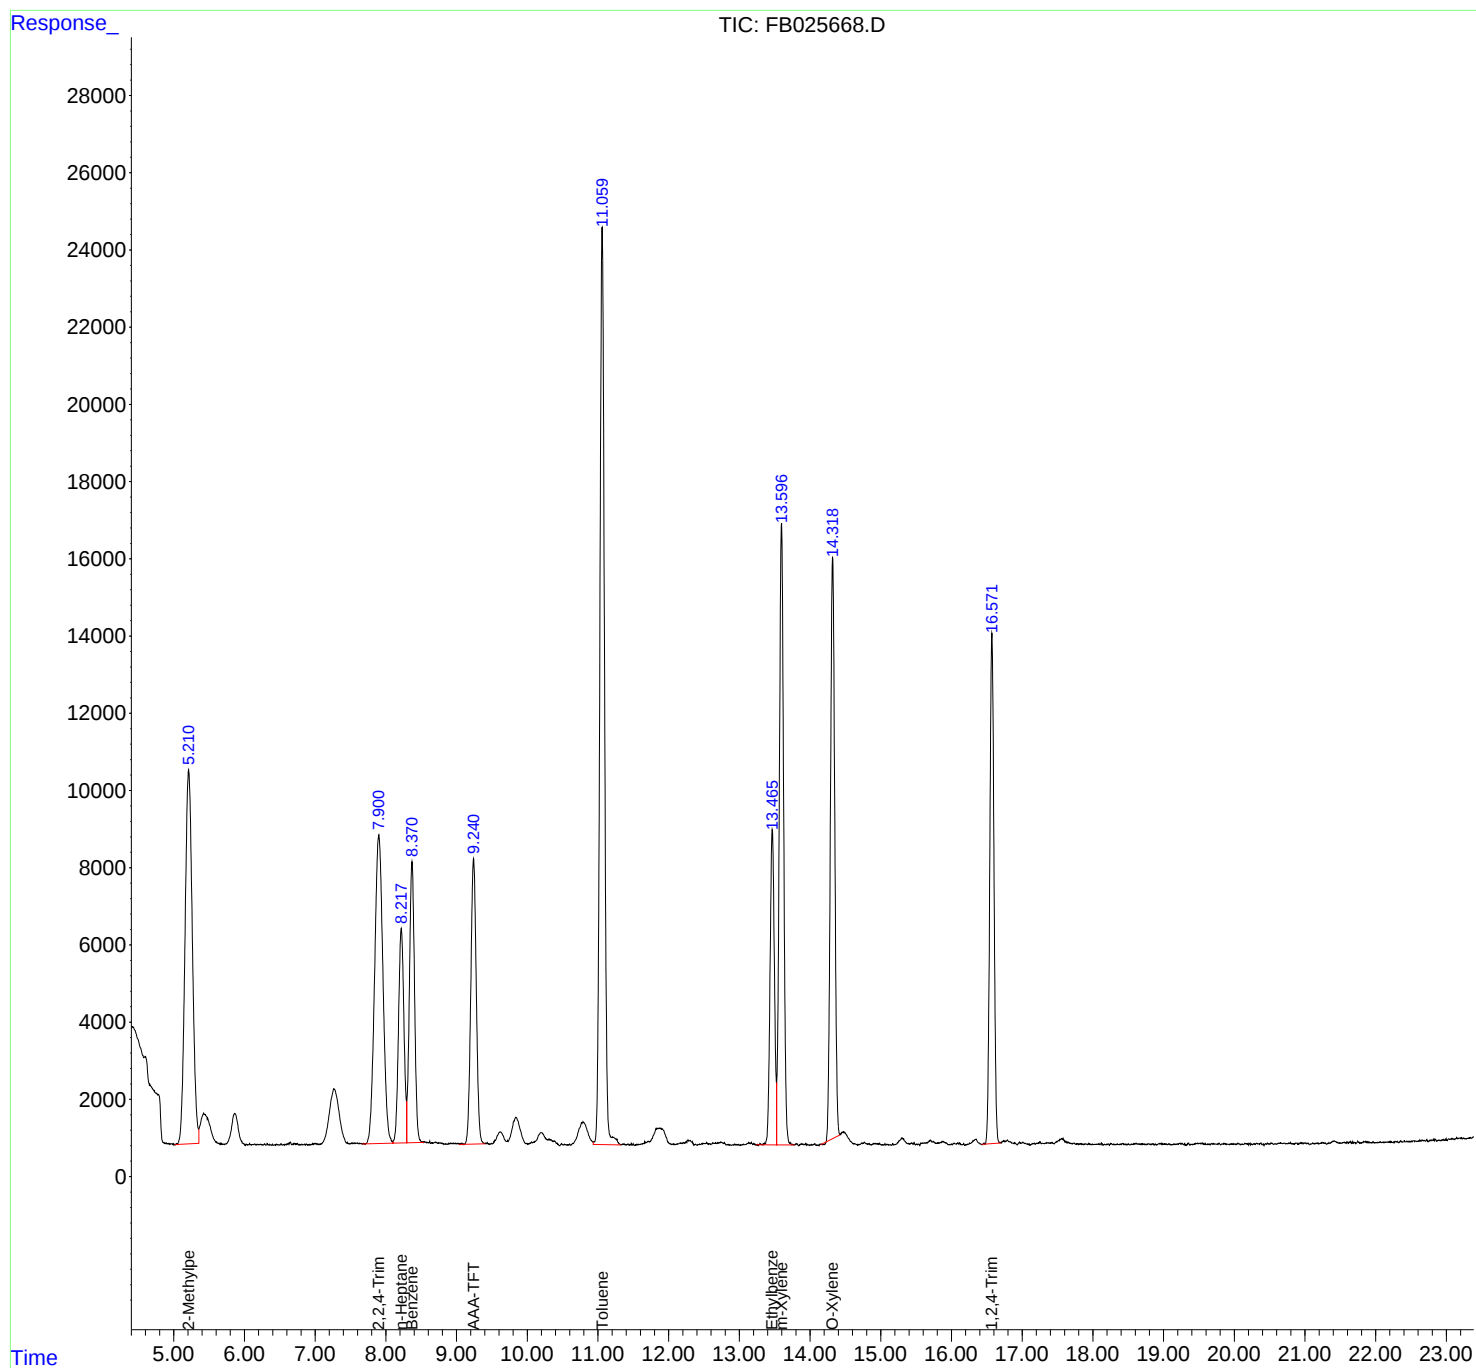


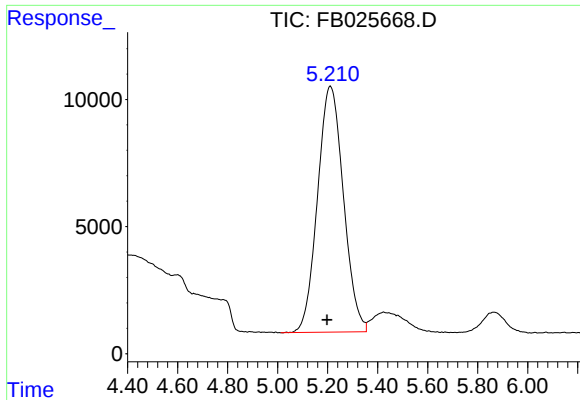

#1 2-Methylpentane


R.T.: 5.211 min
Delta R.T.: 0.013 min
Response: 696393
Conc: 28.79 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0428S1

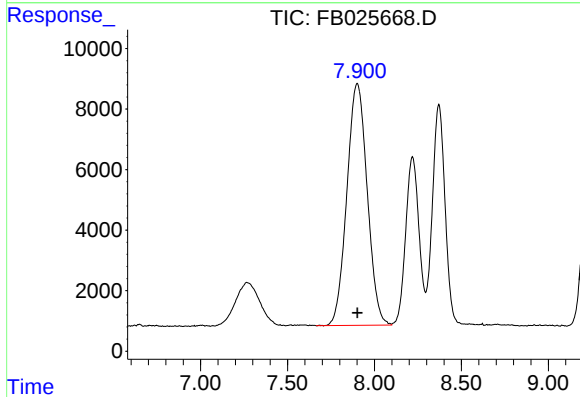


#2 2,2,4-Trimethylpentane

R.T.: 7.901 min
Delta R.T.: 0.000 min
Response: 649969
Conc: 34.95 ng/ml

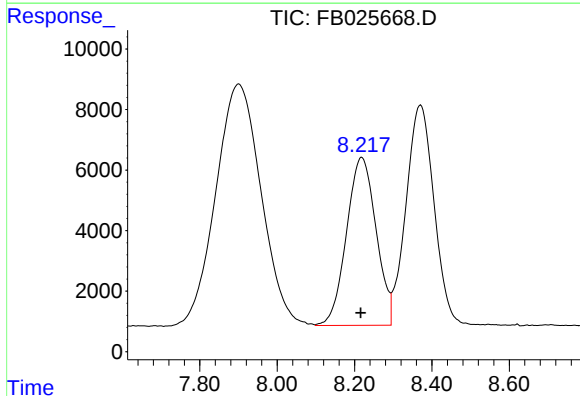


#3 n-Heptane

R.T.: 8.219 min
Delta R.T.: 0.003 min
Response: 294525
Conc: 10.05 ng/ml

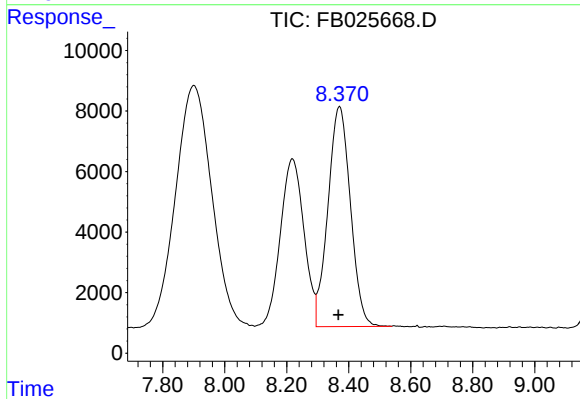

#4 Benzene


R.T.: 8.371 min
Delta R.T.: 0.004 min
Response: 366465
Conc: 9.49 ng/ml

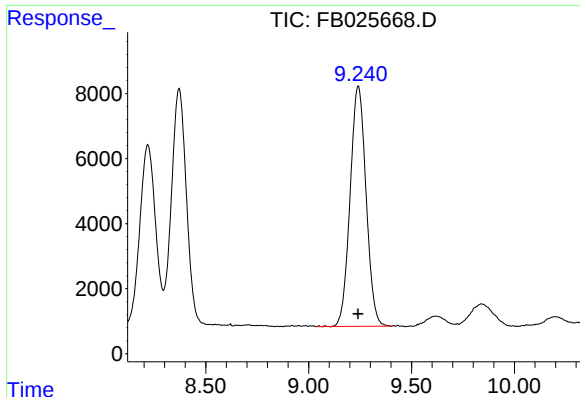

#5 AAA-TFT


R.T.: 9.242 min
Delta R.T.: 0.000 min
Response: 398189
Conc: 20.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0428S1

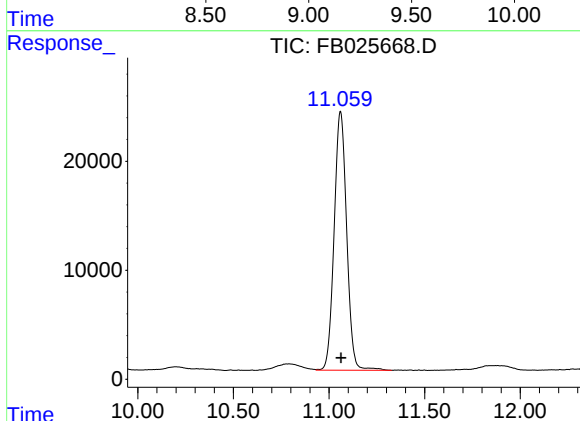


#6 Toluene

R.T.: 11.060 min
Delta R.T.: -0.002 min
Response: 1077095
Conc: 29.84 ng/ml

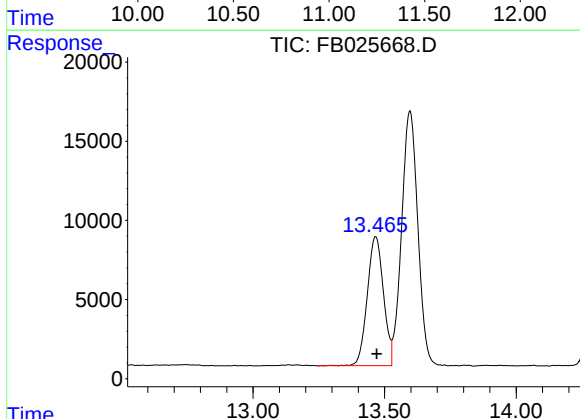


#7 Ethylbenzene

R.T.: 13.466 min
Delta R.T.: -0.004 min
Response: 347828
Conc: 10.15 ng/ml

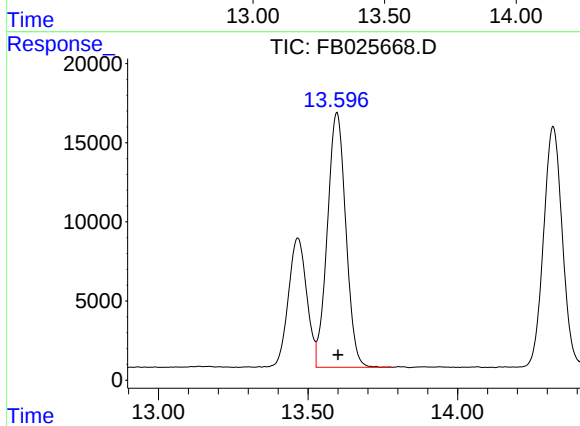

#8 m-Xylene


R.T.: 13.597 min
Delta R.T.: -0.004 min
Response: 690724
Conc: 20.32 ng/ml

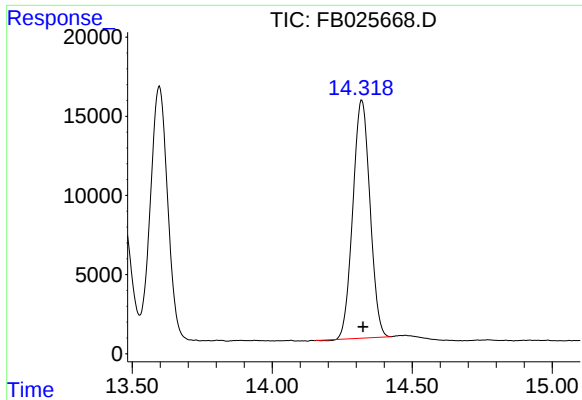

#9 O-Xylene

R.T.: 14.320 min
Delta R.T.: -0.005 min
Response: 639370
Conc: 19.63 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0428S1

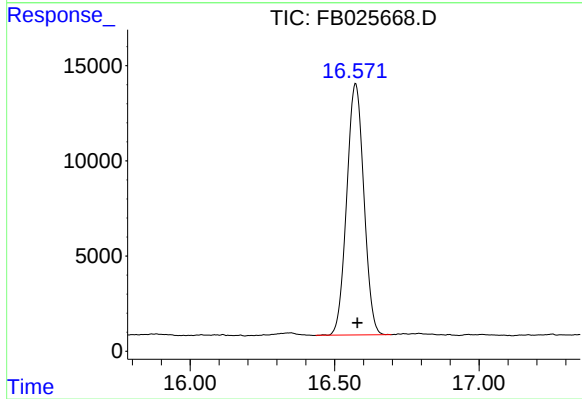

#10 1,2,4-Trimethylbenzene

R.T.: 16.573 min
Delta R.T.: -0.006 min
Response: 541390
Conc: 20.59 ng/ml