

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042822\
 Data File : FB027099.D
 Signal(s) : FID2B.CH
 Acq On : 28 Apr 2022 12:00
 Operator : AJ/MA
 Sample : N2514-05 50X
 Misc : 5.01G/5.00 ML MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 29 02:23:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.818	634800	56.150 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	6215	0.330 ng/ml
2) t 2,2,4-Trimethylpentane	7.376	78105	3.904 ng/ml
3) t n-Heptane	7.789	81752	4.179 ng/ml
6) t Toluene	10.634	56269	2.729 ng/ml
7) t Ethylbenzene	13.007	412957	21.613 ng/ml
9) t O-Xylene	13.916	93789	5.178 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	7978	0.433 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042822\
Data File : FB027099.D
Signal(s) : FID2B.CH
Acq On : 28 Apr 2022 12:00
Operator : AJ/MA
Sample : N2514-05 50X
Misc : 5.01G/5.00 ML MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 29 02:23:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

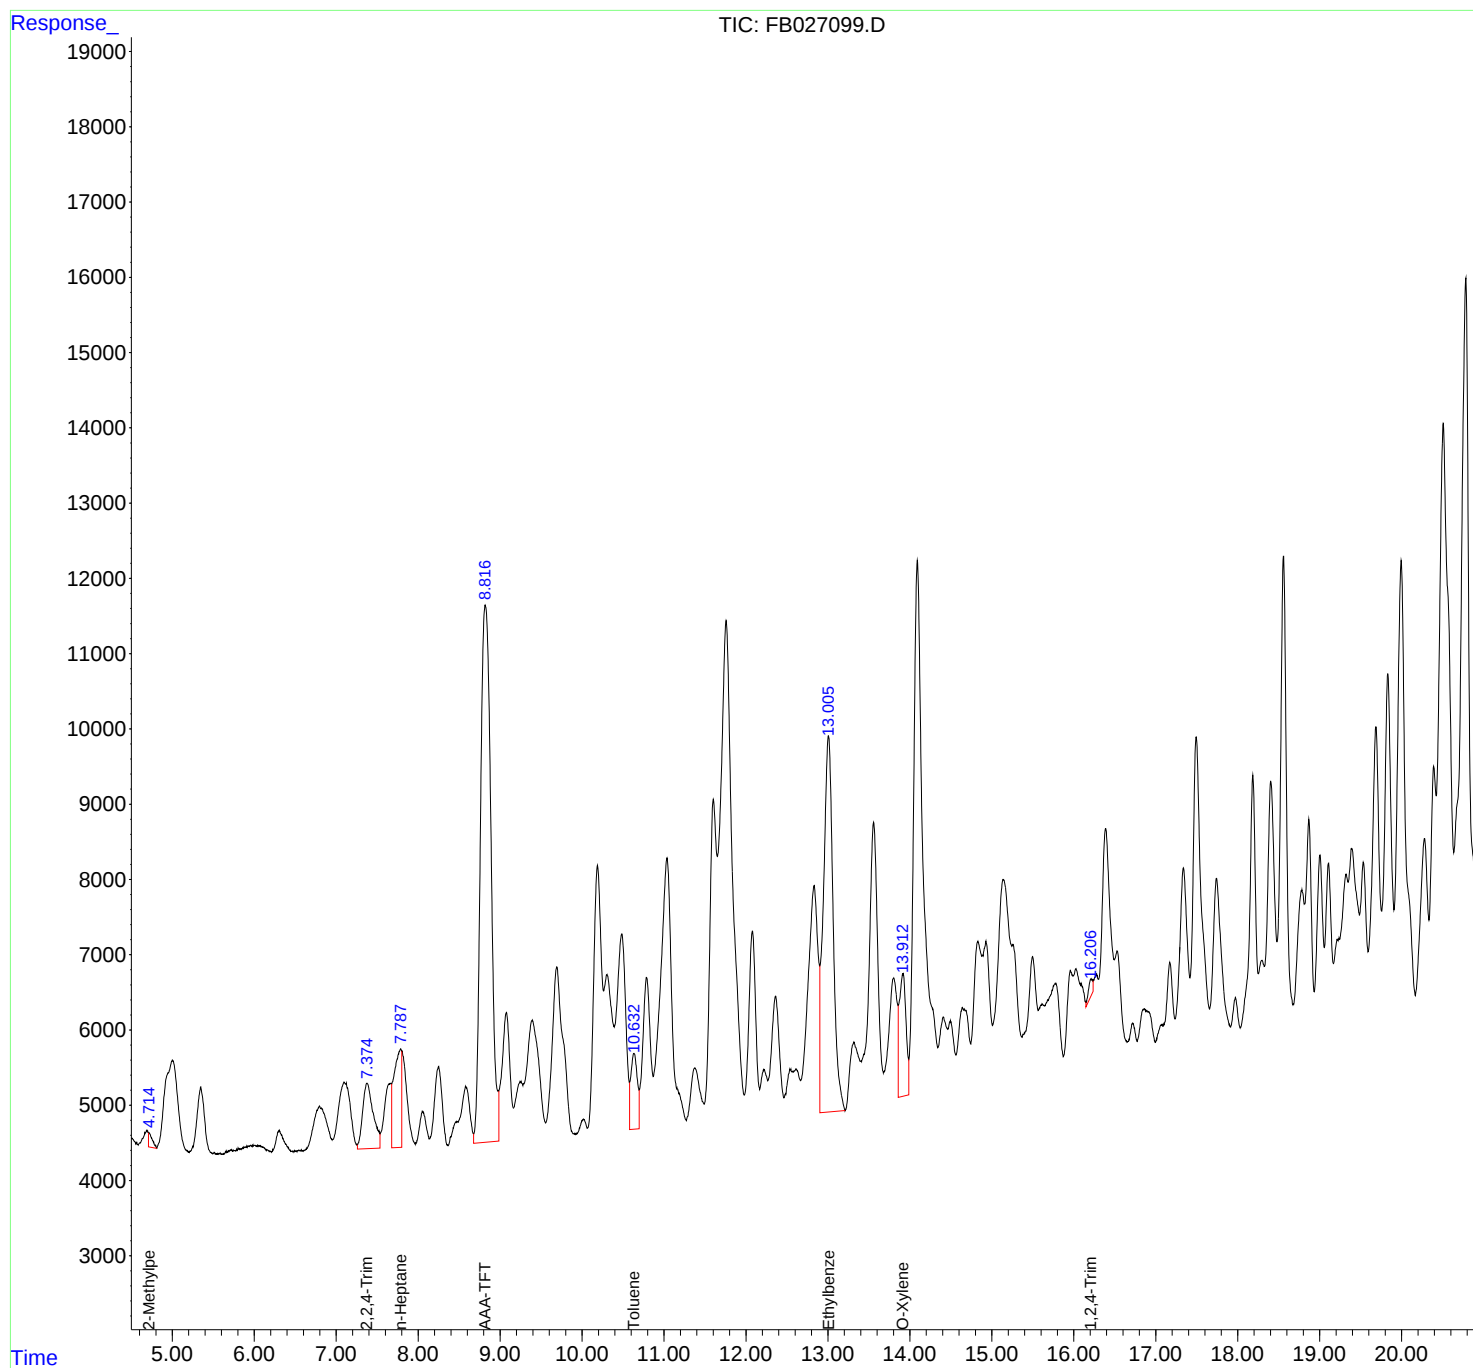


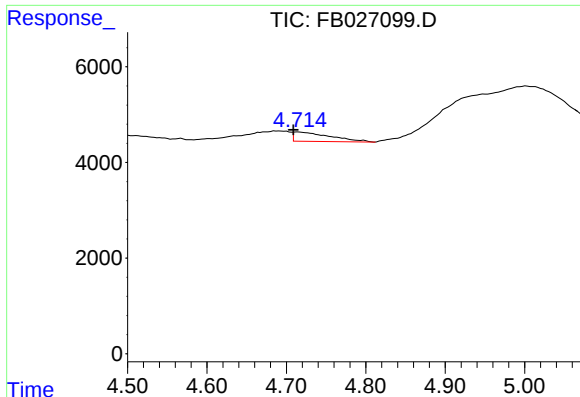

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.006 min
Response: 6215
Conc: 0.33 ng/ml

Instrument :
FID_B
ClientSampleId :

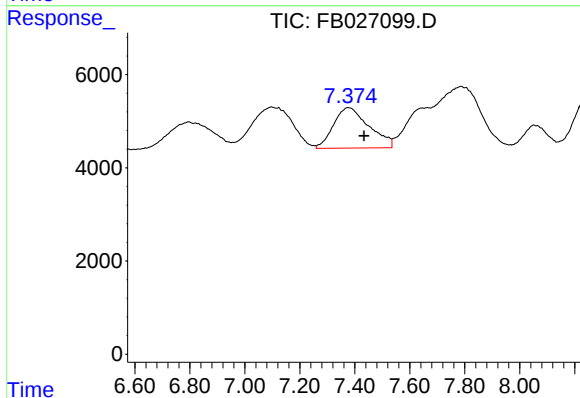


#2 2,2,4-Trimethylpentane

R.T.: 7.376 min
Delta R.T.: -0.057 min
Response: 78105
Conc: 3.90 ng/ml

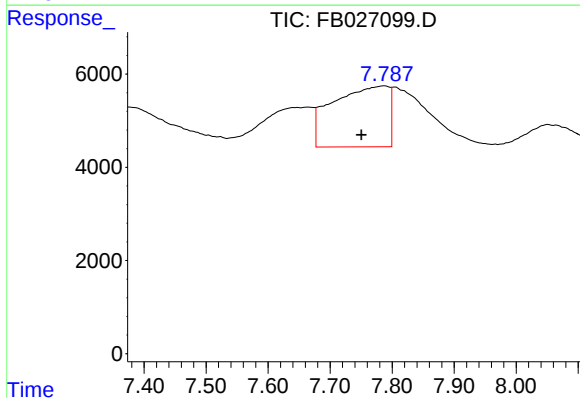


#3 n-Heptane

R.T.: 7.789 min
Delta R.T.: 0.038 min
Response: 81752
Conc: 4.18 ng/ml

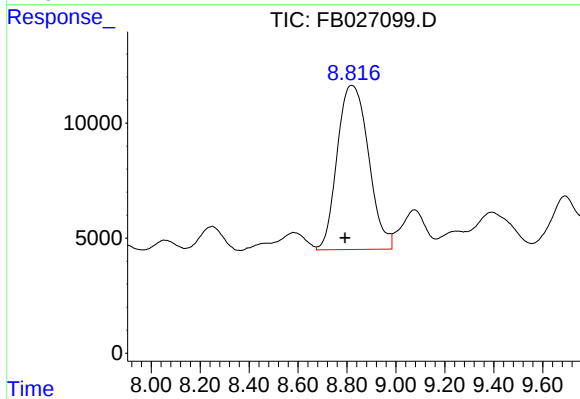

#5 AAA-TFT


R.T.: 8.818 min
Delta R.T.: 0.026 min
Response: 634800
Conc: 56.15 ng/ml

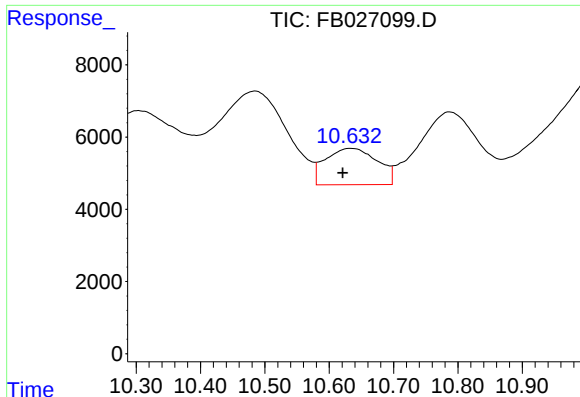

#6 Toluene


R.T.: 10.634 min
Delta R.T.: 0.013 min
Response: 56269
Conc: 2.73 ng/ml

Instrument :
FID_B
ClientSampleId :

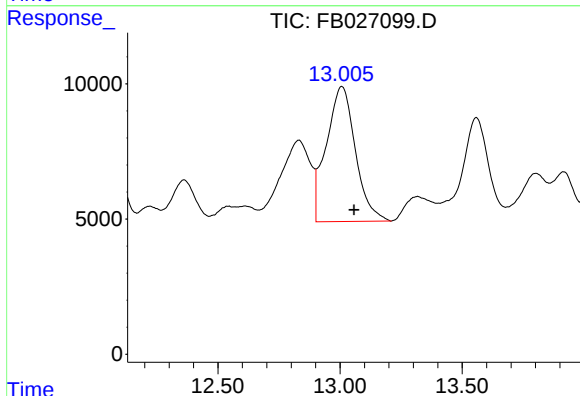


#7 Ethylbenzene

R.T.: 13.007 min
Delta R.T.: -0.051 min
Response: 412957
Conc: 21.61 ng/ml

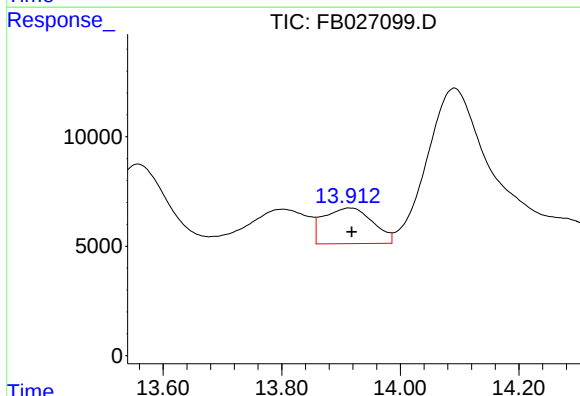

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 93789
Conc: 5.18 ng/ml

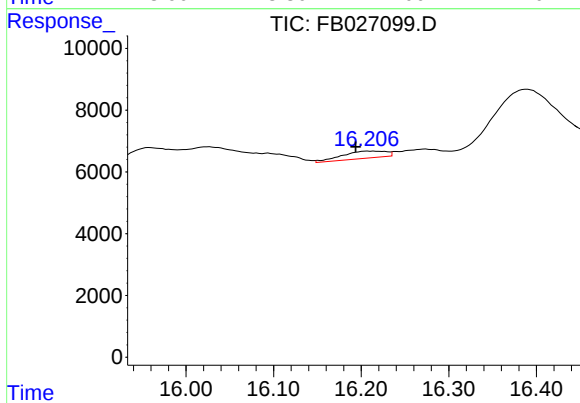

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.017 min
Response: 7978
Conc: 0.43 ng/ml