

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042822\
 Data File : FB027098.D
 Signal(s) : FID2B.CH
 Acq On : 28 Apr 2022 11:09
 Operator : AJ/MA
 Sample : BSF0428S1
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0428S1

Integration File: Calibration.e
 Quant Time: Apr 29 02:23:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	237046	20.967 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	393316	20.895 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	446643	22.326 ng/ml
3) t n-Heptane	7.748	133536	6.826 ng/ml
4) t Benzene	7.884	172742	7.827 ng/ml
6) t Toluene	10.616	495790	24.044 ng/ml
7) t Ethylbenzene	13.054	162712	8.516 ng/ml
8) t m-Xylene	13.186	314345	16.641 ng/ml
9) t O-Xylene	13.913	306415	16.916 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	309750	16.805 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042822\
Data File : FB027098.D
Signal(s) : FID2B.CH
Acq On : 28 Apr 2022 11:09
Operator : AJ/MA
Sample : BSF0428S1
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0428S1

Integration File: Calibration.e
Quant Time: Apr 29 02:23:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

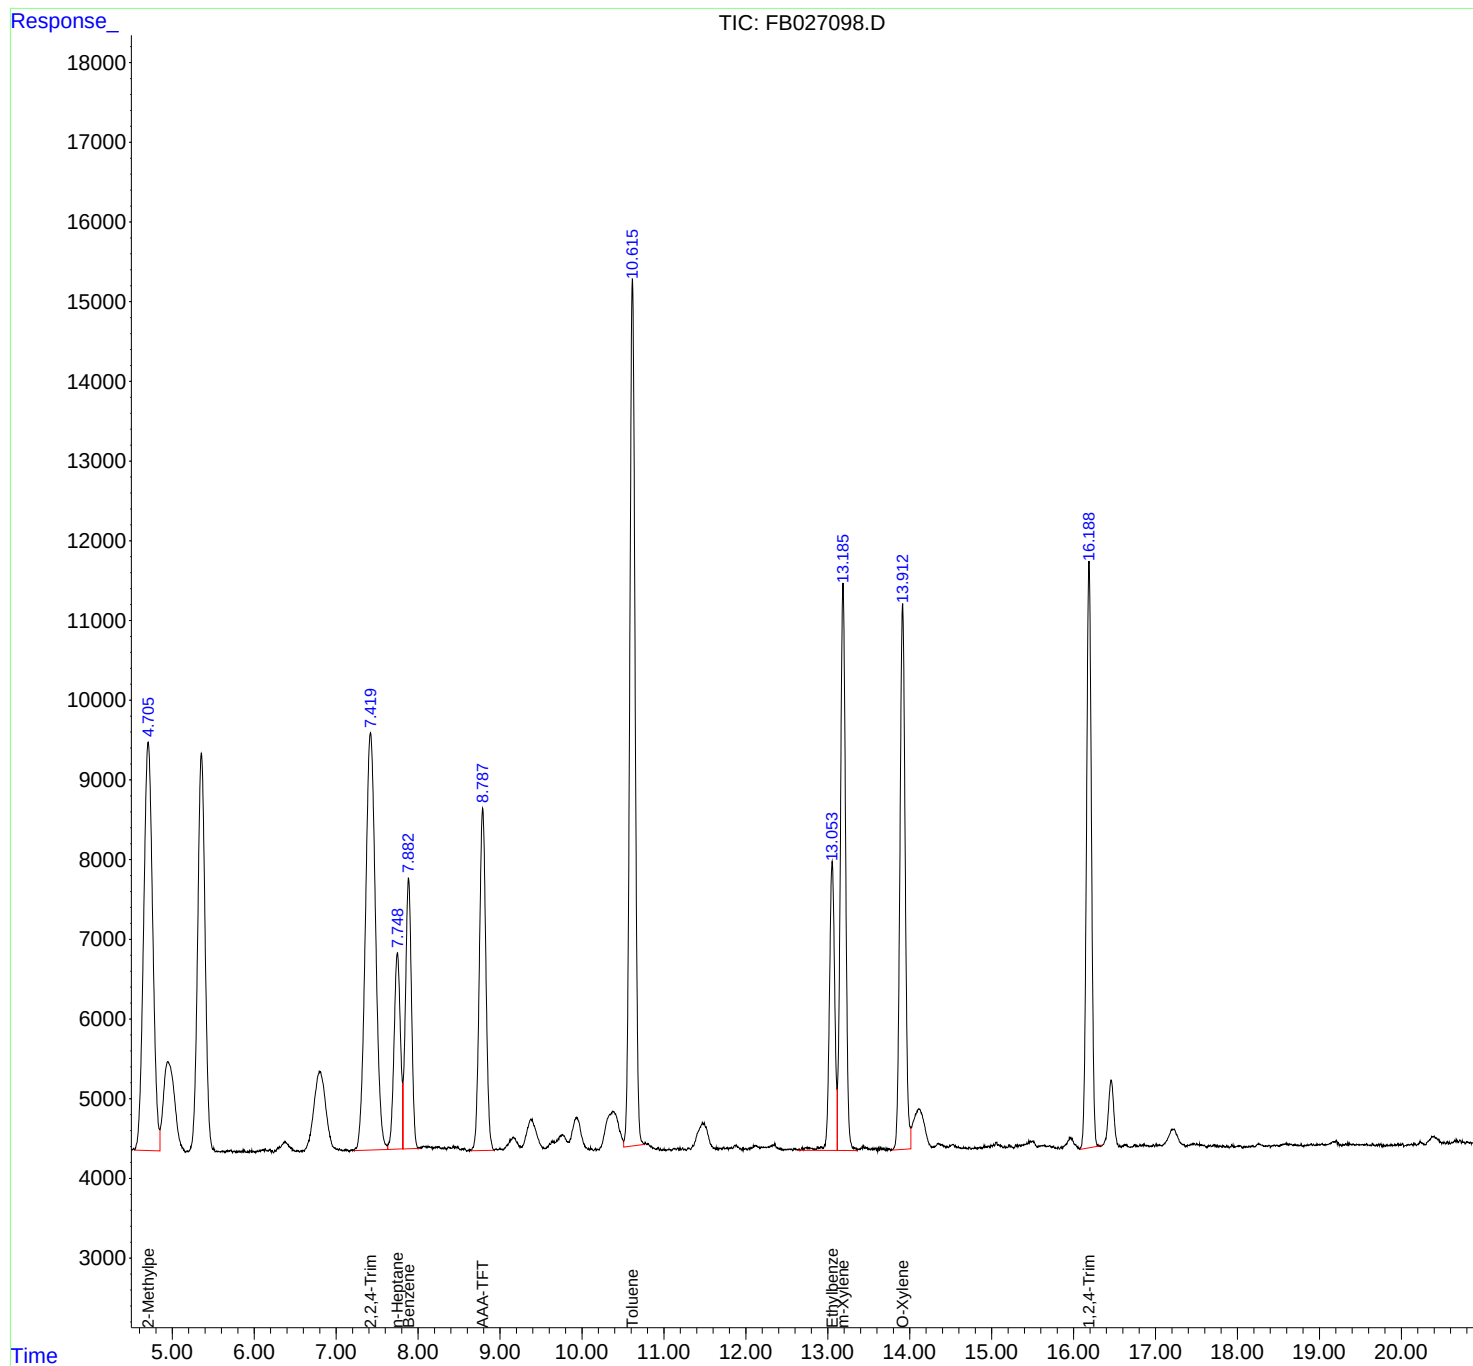


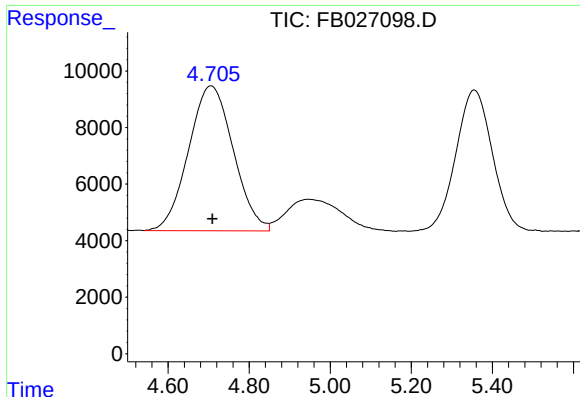

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.002 min
Response: 393316
Conc: 20.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0428S1

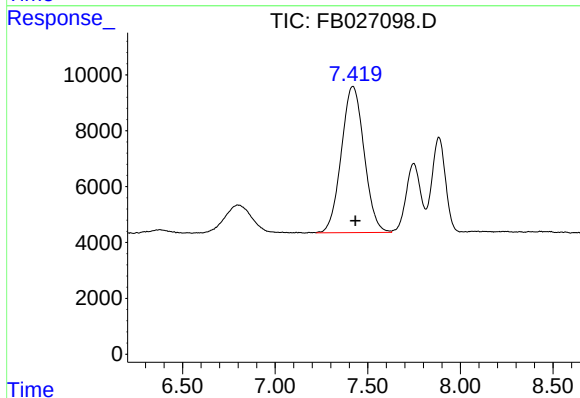


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.013 min
Response: 446643
Conc: 22.33 ng/ml

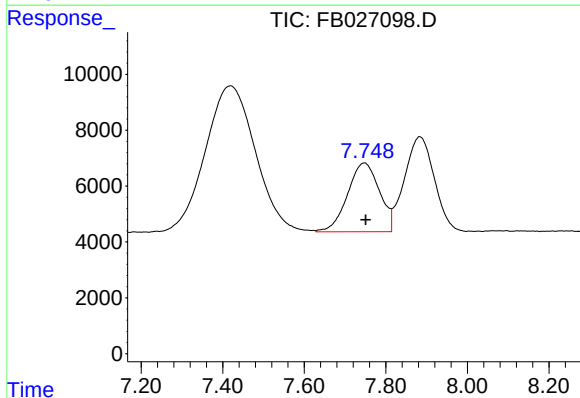


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 133536
Conc: 6.83 ng/ml

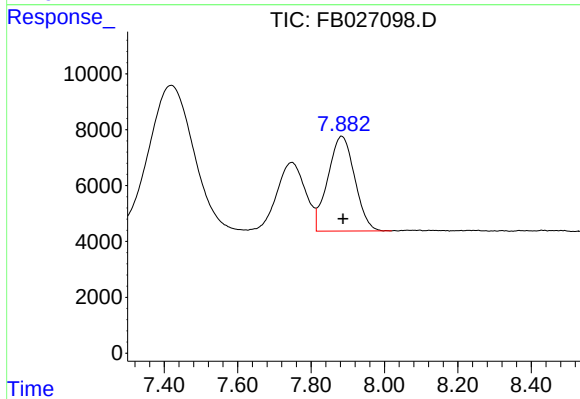

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.003 min
Response: 172742
Conc: 7.83 ng/ml

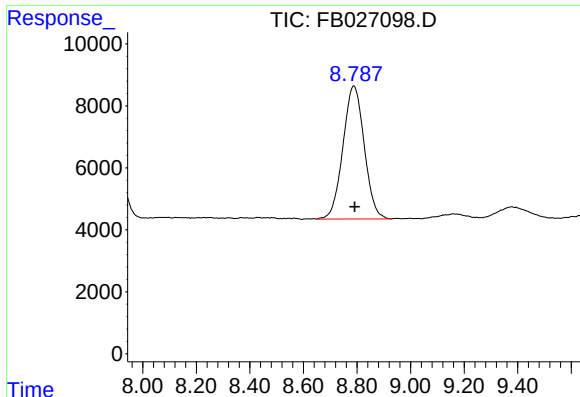

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 237046
Conc: 20.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0428S1

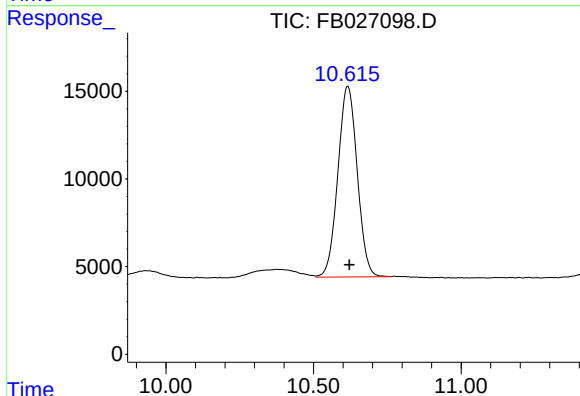


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 495790
Conc: 24.04 ng/ml

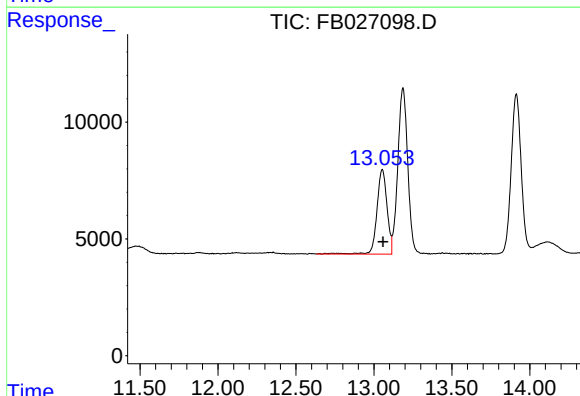


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.004 min
Response: 162712
Conc: 8.52 ng/ml

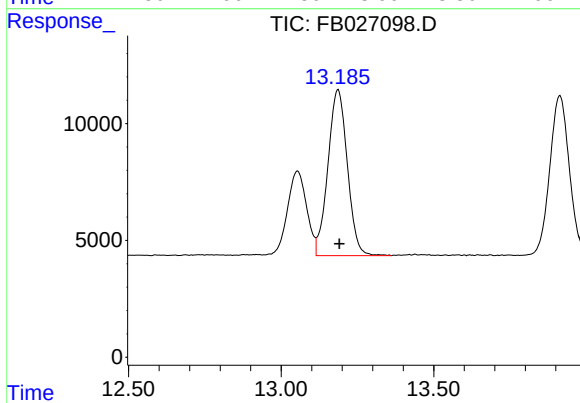

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 314345
Conc: 16.64 ng/ml

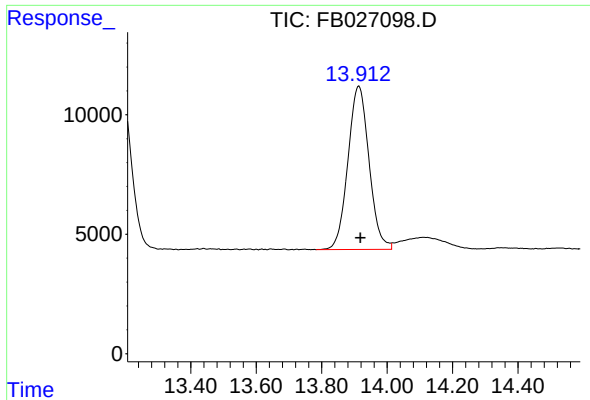

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.005 min
Response: 306415
Conc: 16.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0428S1

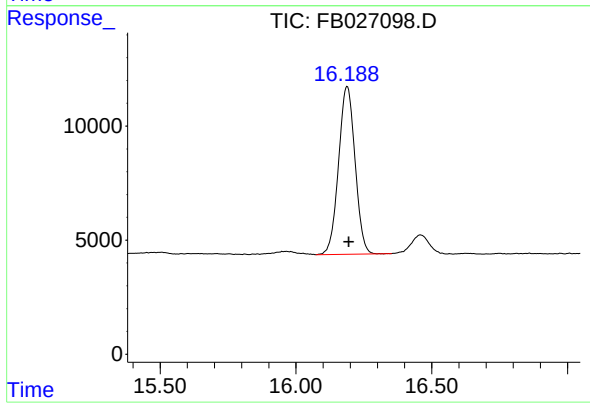

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 309750
Conc: 16.81 ng/ml