

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042919\
 Data File : FB020864.D
 Signal(s) : FID2B.CH
 Acq On : 29 Apr 2019 15:08
 Operator : MJ/SJ
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 50 GRO STD

Integration File: Calibration.e
 Quant Time: Apr 29 15:23:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 14:59:27 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.990	889972	50.228 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.852	3629219	83.523 ng/ml
2) t 2,2,4-Trimethylpentane	7.606	3384008	84.902 ng/ml
3) t n-Heptane	7.946	1061755	27.908 ng/ml
4) t Benzene	8.083	1103275	27.326 ng/ml
6) t Toluene	10.835	2113138	76.345 ng/ml
7) t Ethylbenzene	13.285	694474	24.179 ng/ml
8) t m-Xylene	13.418	1476439	48.623 ng/ml
9) t O-Xylene	14.149	1536753	48.418 ng/ml
10) t 1,2,4-Trimethylbenzene	16.433	1549503	48.935 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042919\
Data File : FB020864.D
Signal(s) : FID2B.CH
Acq On : 29 Apr 2019 15:08
Operator : MJ/SJ
Sample : 50 GRO STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
50 GRO STD

Integration File: Calibration.e
Quant Time: Apr 29 15:23:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 14:59:27 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

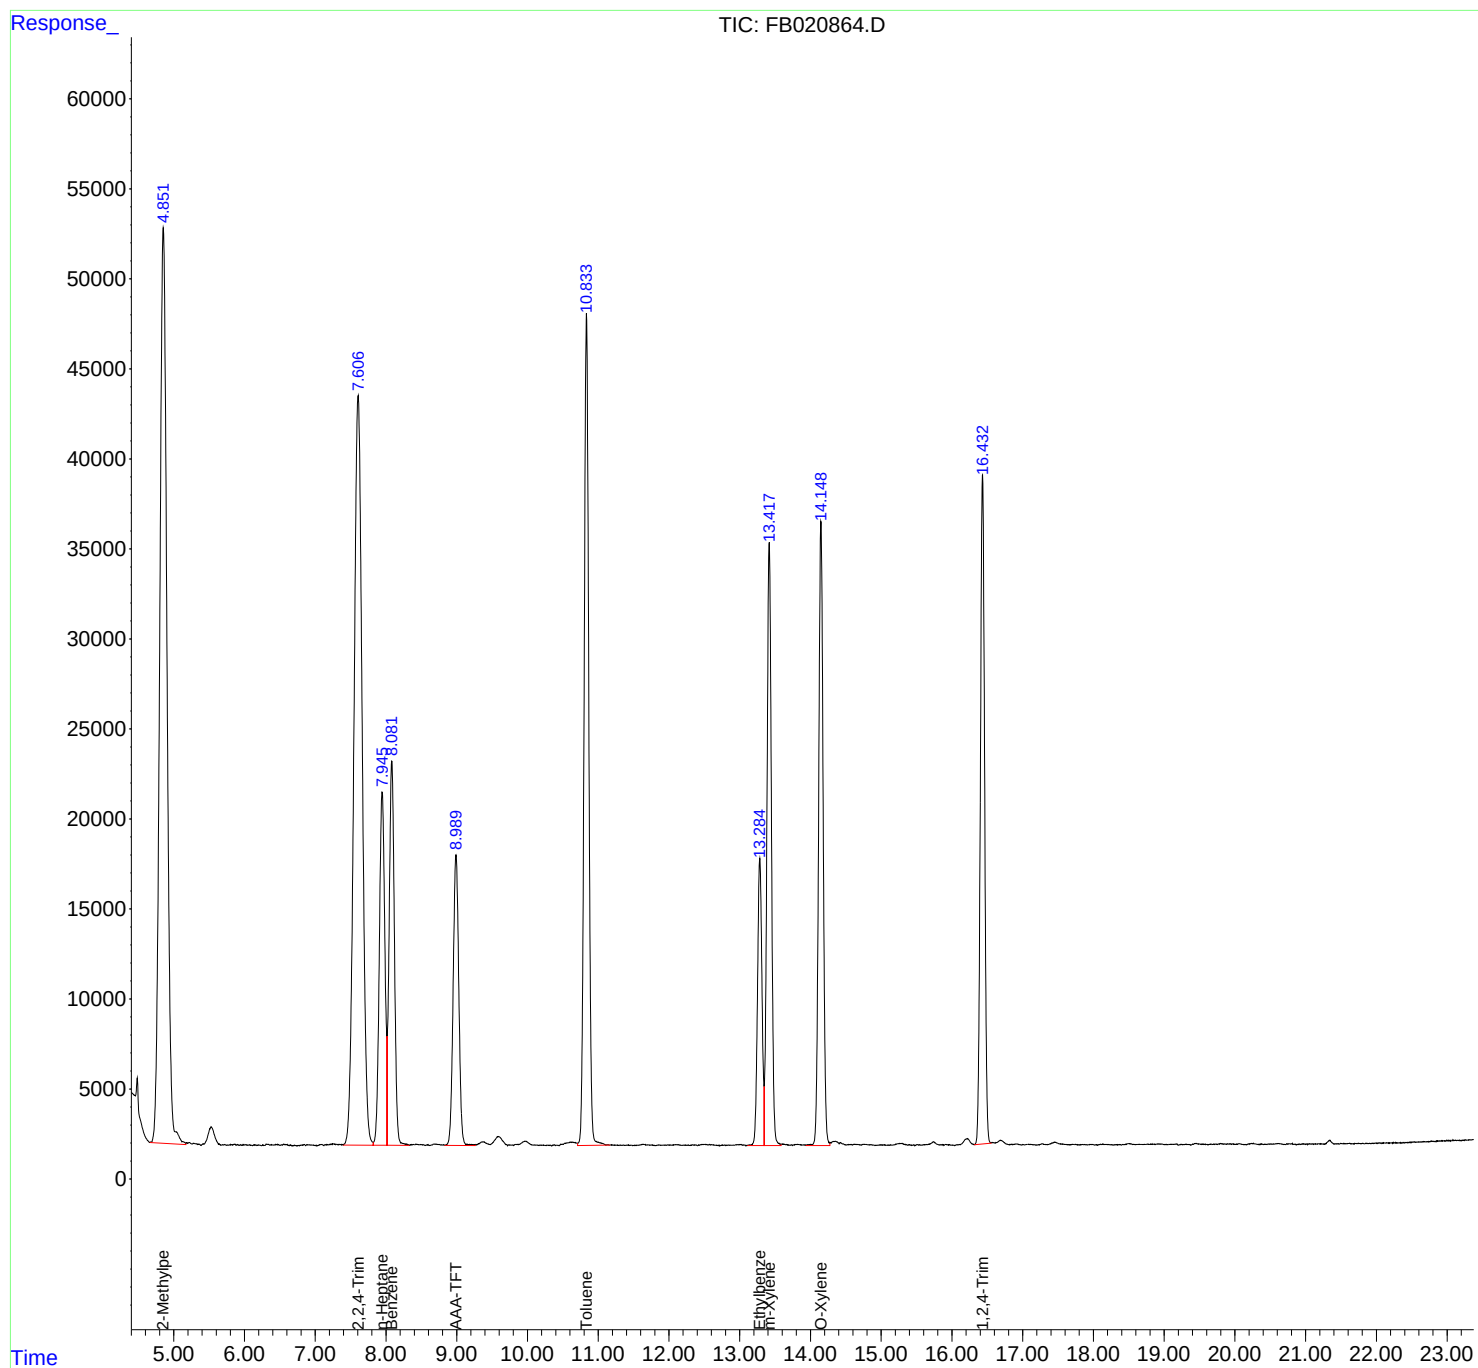


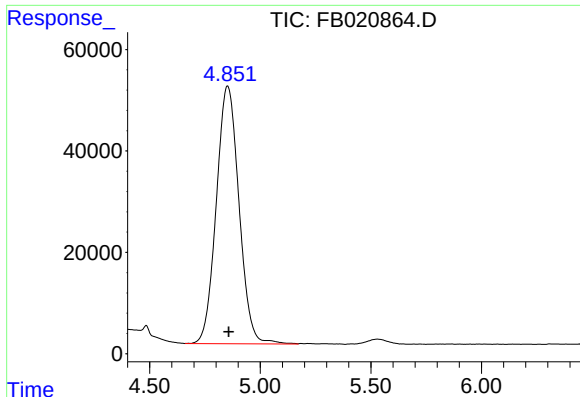

#1 2-Methylpentane


R.T.: 4.852 min
Delta R.T.: -0.005 min
Response: 3629219
Conc: 83.52 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

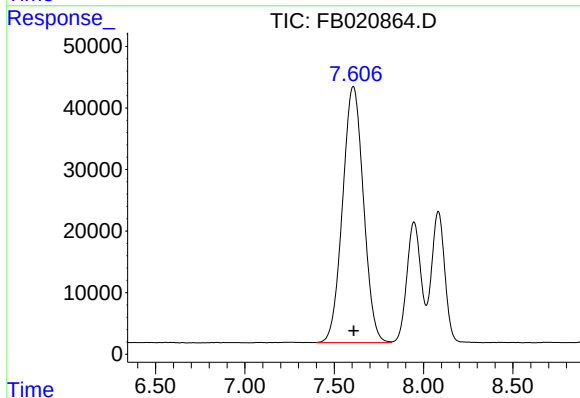


#2 2,2,4-Trimethylpentane

R.T.: 7.606 min
Delta R.T.: -0.002 min
Response: 3384008
Conc: 84.90 ng/ml

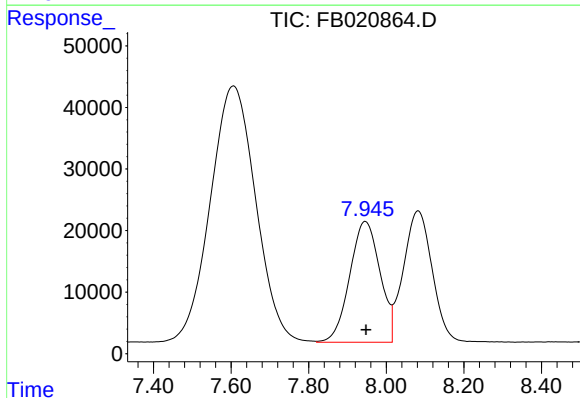


#3 n-Heptane

R.T.: 7.946 min
Delta R.T.: -0.002 min
Response: 1061755
Conc: 27.91 ng/ml

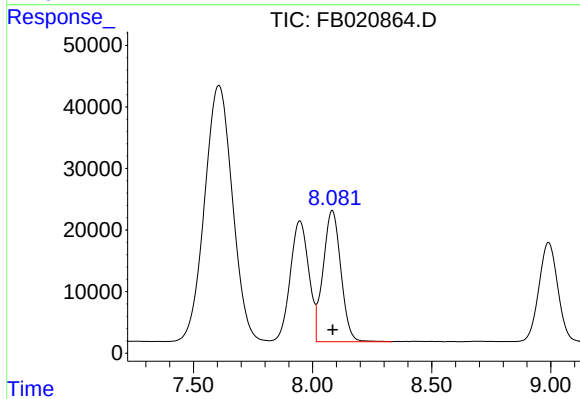

#4 Benzene


R.T.: 8.083 min
Delta R.T.: -0.002 min
Response: 1103275
Conc: 27.33 ng/ml

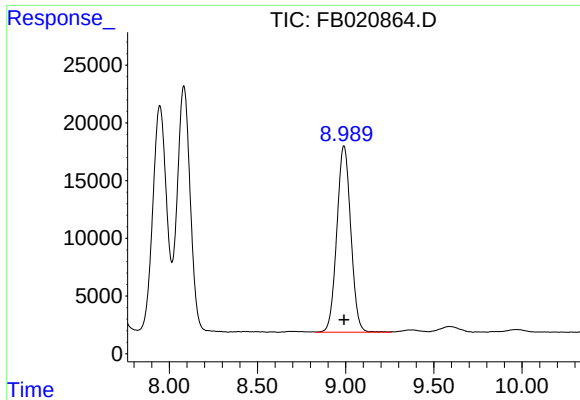

#5 AAA-TFT


R.T.: 8.990 min
Delta R.T.: -0.001 min
Response: 889972
Conc: 50.23 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

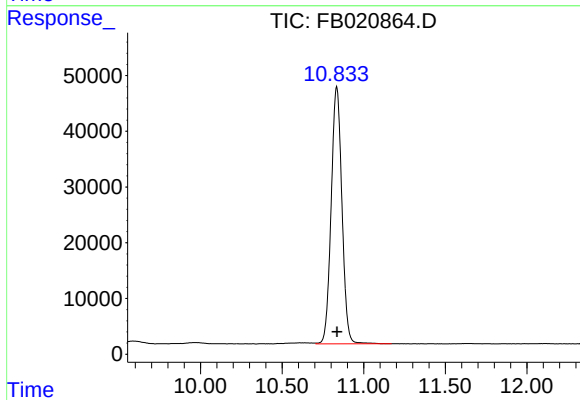


#6 Toluene

R.T.: 10.835 min
Delta R.T.: -0.001 min
Response: 2113138
Conc: 76.35 ng/ml

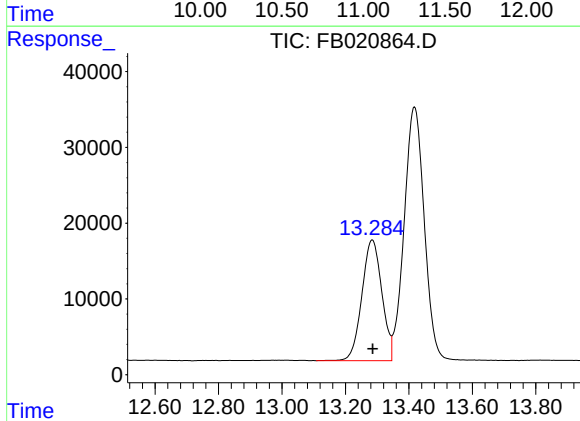


#7 Ethylbenzene

R.T.: 13.285 min
Delta R.T.: 0.000 min
Response: 694474
Conc: 24.18 ng/ml

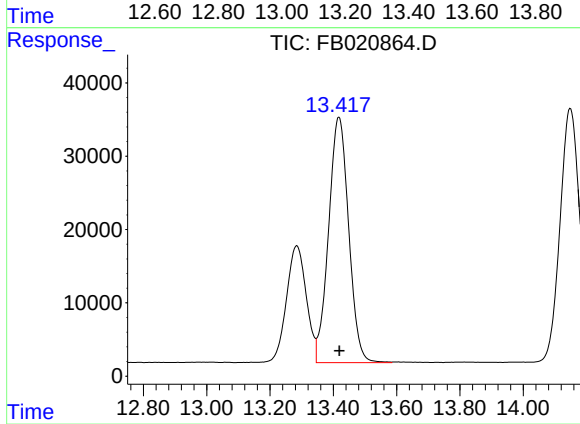

#8 m-Xylene


R.T.: 13.418 min
Delta R.T.: 0.000 min
Response: 1476439
Conc: 48.62 ng/ml

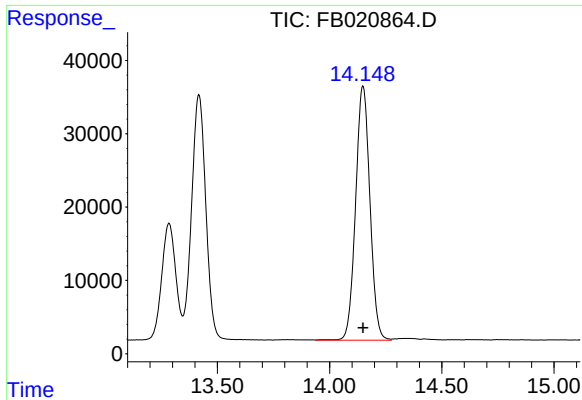

#9 O-Xylene

R.T.: 14.149 min
Delta R.T.: 0.000 min
Response: 1536753
Conc: 48.42 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

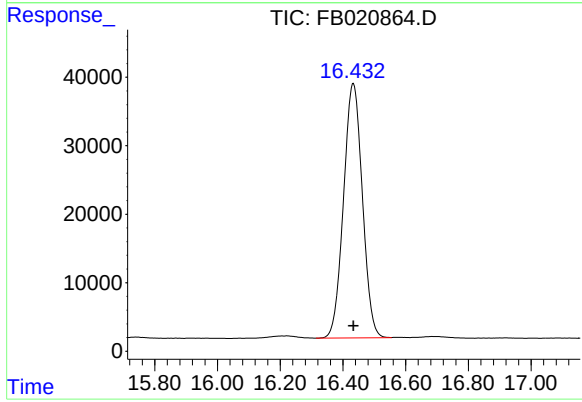

#10 1,2,4-Trimethylbenzene

R.T.: 16.433 min
Delta R.T.: 0.000 min
Response: 1549503
Conc: 48.93 ng/ml