

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042921\
 Data File : FB025685.D
 Signal(s) : FID2B.CH
 Acq On : 29 Apr 2021 10:12
 Operator : DD/AJ
 Sample : BSF0429S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 30 01:22:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.246	395313	20.102 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.218	710199	29.357 ng/ml
2) t 2,2,4-Trimethylpentane	7.905	666071	35.814 ng/ml
3) t n-Heptane	8.223	303037	10.343 ng/ml
4) t Benzene	8.376	376788	9.752 ng/ml
6) t Toluene	11.064	1100375	30.487 ng/ml
7) t Ethylbenzene	13.470	352874	10.293 ng/ml
8) t m-Xylene	13.600	701535	20.638 ng/ml
9) t O-Xylene	14.323	674213	20.695 ng/ml
10) t 1,2,4-Trimethylbenzene	16.576	550169	20.929 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042921\
Data File : FB025685.D
Signal(s) : FID2B.CH
Acq On : 29 Apr 2021 10:12
Operator : DD/AJ
Sample : BSF0429S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 30 01:22:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

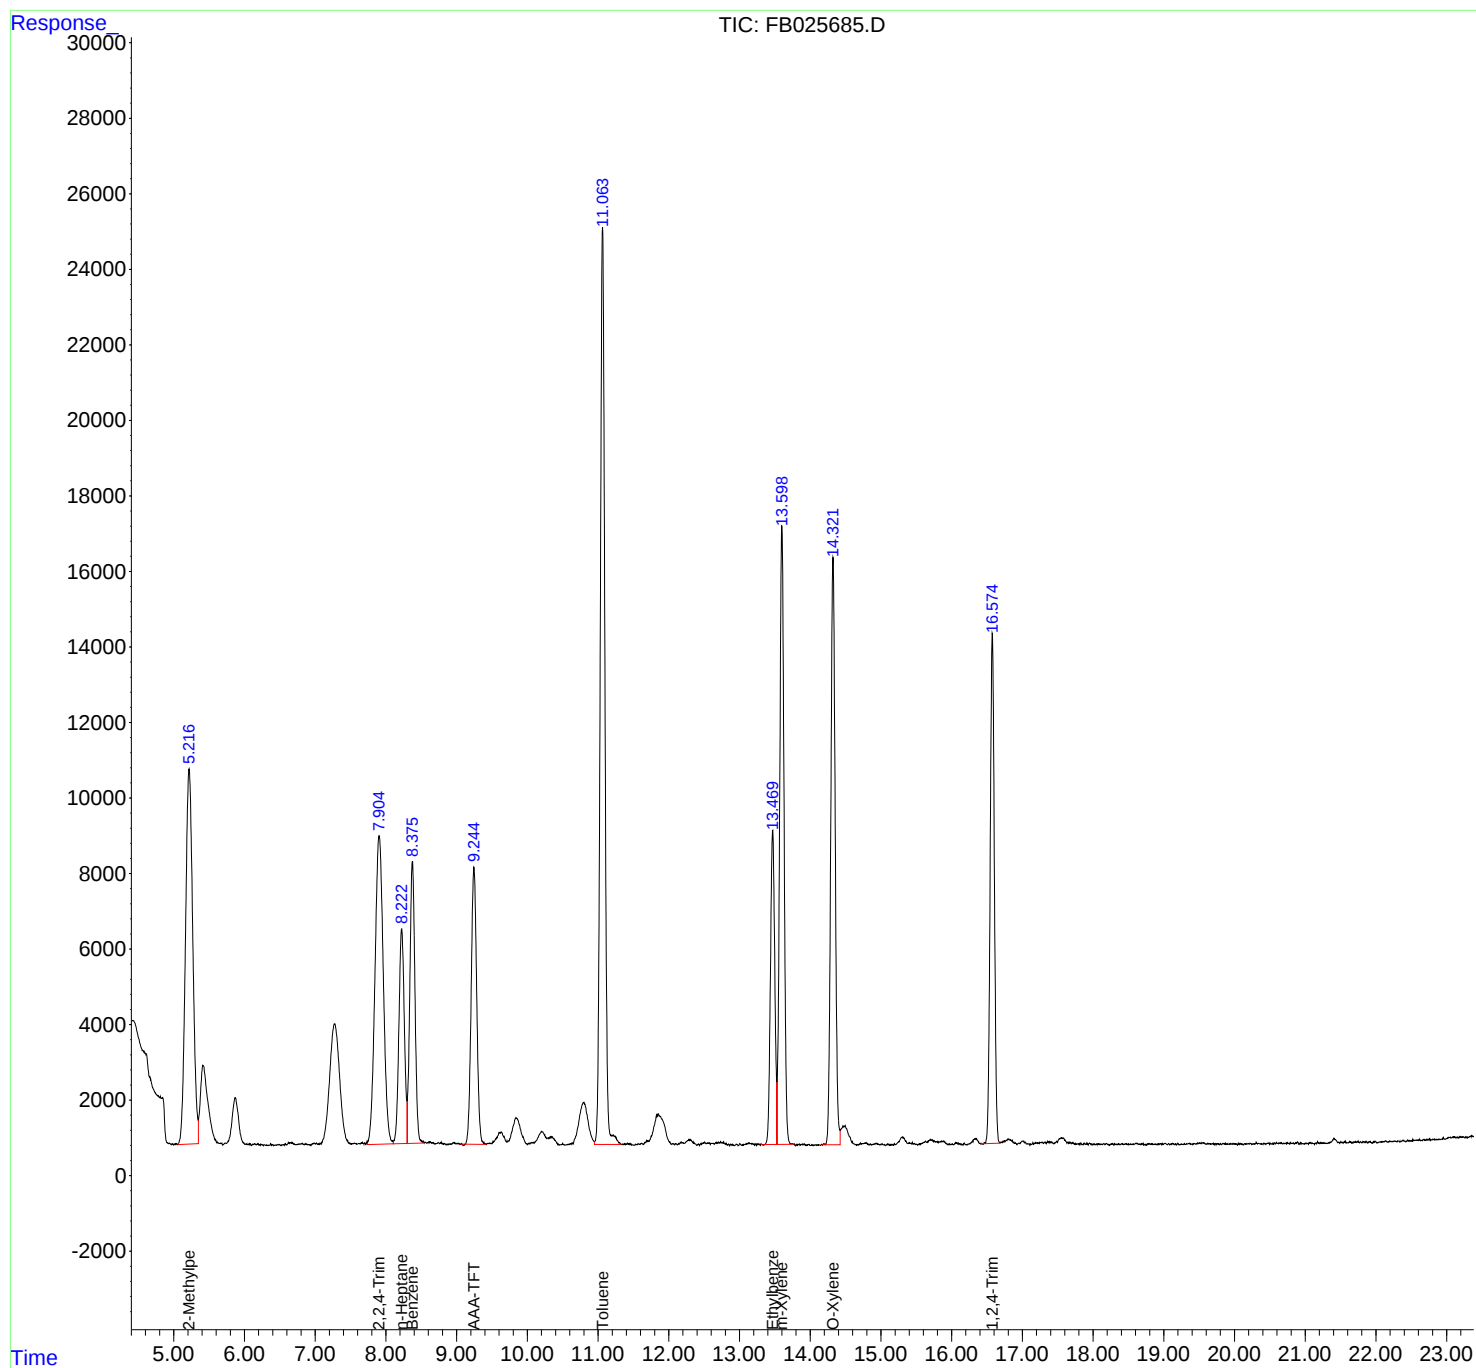


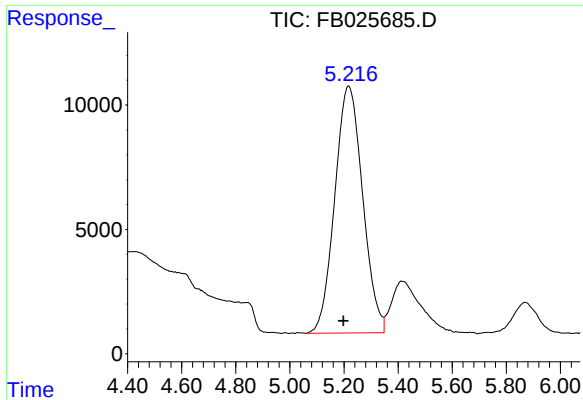

#1 2-Methylpentane


R.T.: 5.218 min
Delta R.T.: 0.020 min
Response: 710199
Conc: 29.36 ng/ml

Instrument :
FID_B
ClientSampleId :

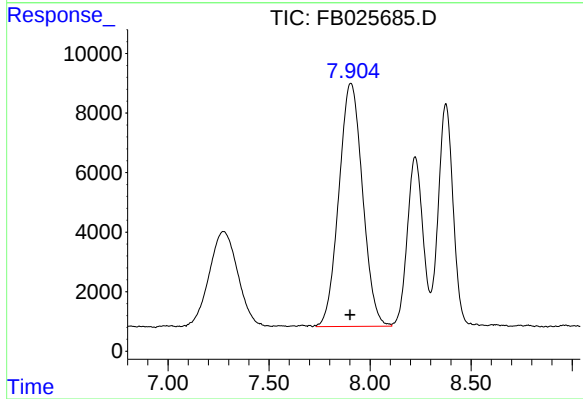


#2 2,2,4-Trimethylpentane

R.T.: 7.905 min
Delta R.T.: 0.003 min
Response: 666071
Conc: 35.81 ng/ml

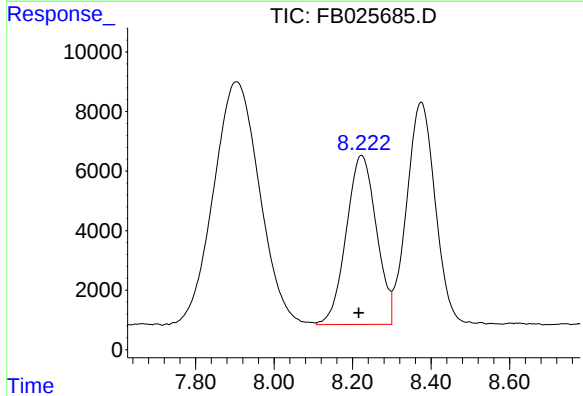


#3 n-Heptane

R.T.: 8.223 min
Delta R.T.: 0.007 min
Response: 303037
Conc: 10.34 ng/ml

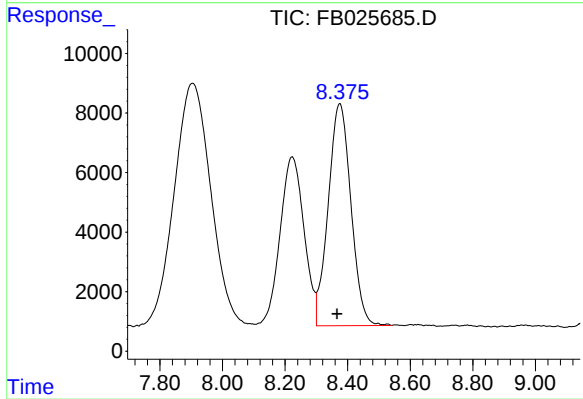

#4 Benzene


R.T.: 8.376 min
Delta R.T.: 0.009 min
Response: 376788
Conc: 9.75 ng/ml

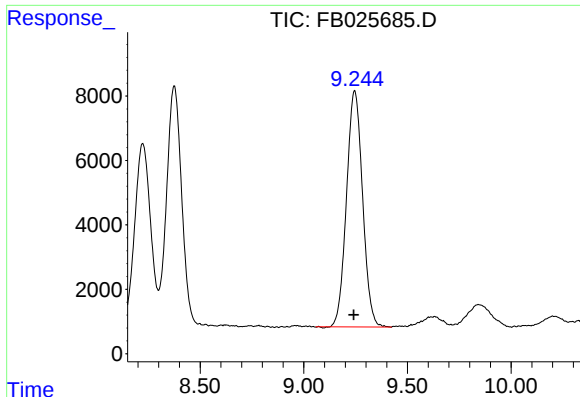

#5 AAA-TFT


R.T.: 9.246 min
Delta R.T.: 0.005 min
Response: 395313
Conc: 20.10 ng/ml

Instrument :
FID_B
ClientSampleId :

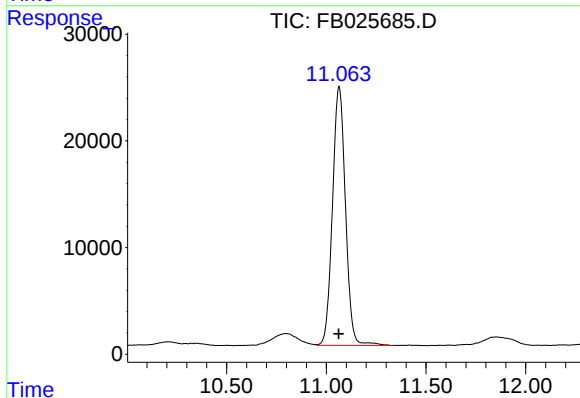


#6 Toluene

R.T.: 11.064 min
Delta R.T.: 0.002 min
Response: 1100375
Conc: 30.49 ng/ml

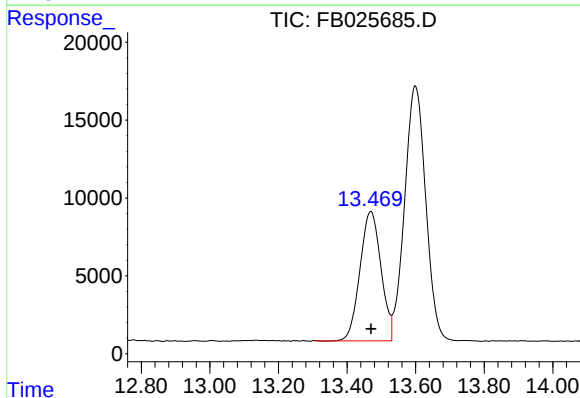


#7 Ethylbenzene

R.T.: 13.470 min
Delta R.T.: 0.000 min
Response: 352874
Conc: 10.29 ng/ml

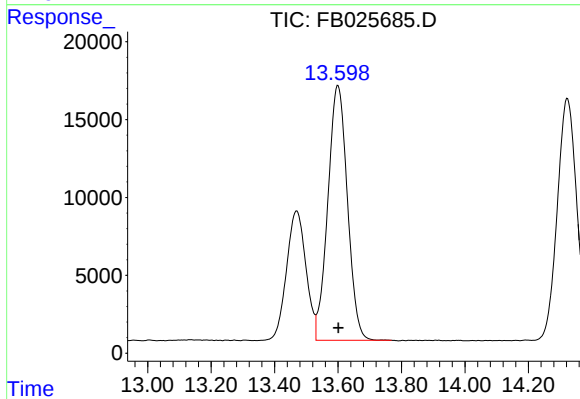

#8 m-Xylene


R.T.: 13.600 min
Delta R.T.: -0.001 min
Response: 701535
Conc: 20.64 ng/ml

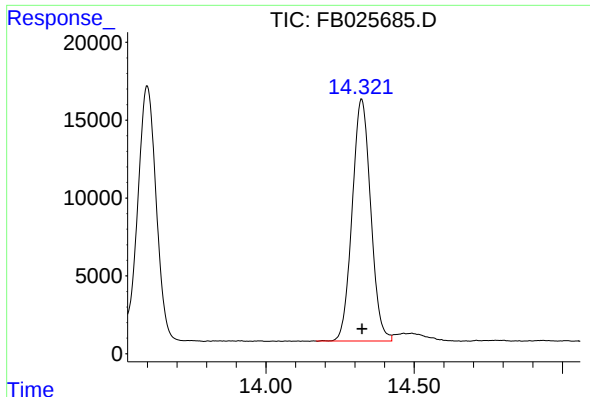

#9 O-Xylene

R.T.: 14.323 min
Delta R.T.: -0.002 min
Response: 674213
Conc: 20.69 ng/ml

Instrument :
FID_B
ClientSampleId :

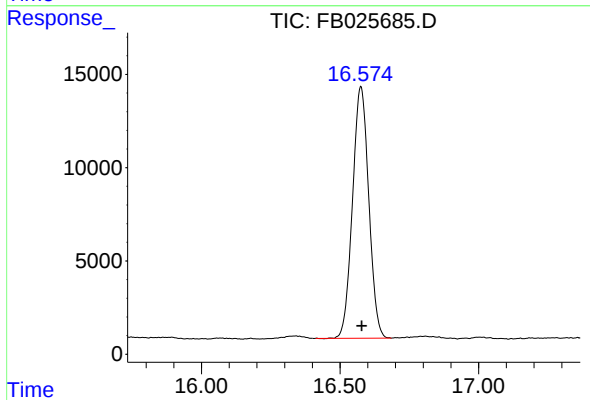

#10 1,2,4-Trimethylbenzene

R.T.: 16.576 min
Delta R.T.: -0.003 min
Response: 550169
Conc: 20.93 ng/ml