

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042921\
 Data File : FB025687.D
 Signal(s) : FID2B.CH
 Acq On : 29 Apr 2021 11:18
 Operator : DD/AJ
 Sample : M2199-03MS
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SAMPLE-3-COMPMS

Integration File: Calibration.e
 Quant Time: Apr 30 01:22:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.238	362099	18.413 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.192	658176	27.206 ng/ml
2) t 2,2,4-Trimethylpentane	7.891	588313	31.633 ng/ml
3) t n-Heptane	8.213	262725	8.967 ng/ml
4) t Benzene	8.364	354225	9.168 ng/ml
6) t Toluene	11.059	1047552	29.024 ng/ml
7) t Ethylbenzene	13.467	334757	9.764 ng/ml
8) t m-Xylene	13.598	667334	19.632 ng/ml
9) t O-Xylene	14.321	612465	18.800 ng/ml
10) t 1,2,4-Trimethylbenzene	16.575	515619	19.614 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042921\
Data File : FB025687.D
Signal(s) : FID2B.CH
Acq On : 29 Apr 2021 11:18
Operator : DD/AJ
Sample : M2199-03MS
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SAMPLE-3-COMPMS

Integration File: Calibration.e
Quant Time: Apr 30 01:22:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

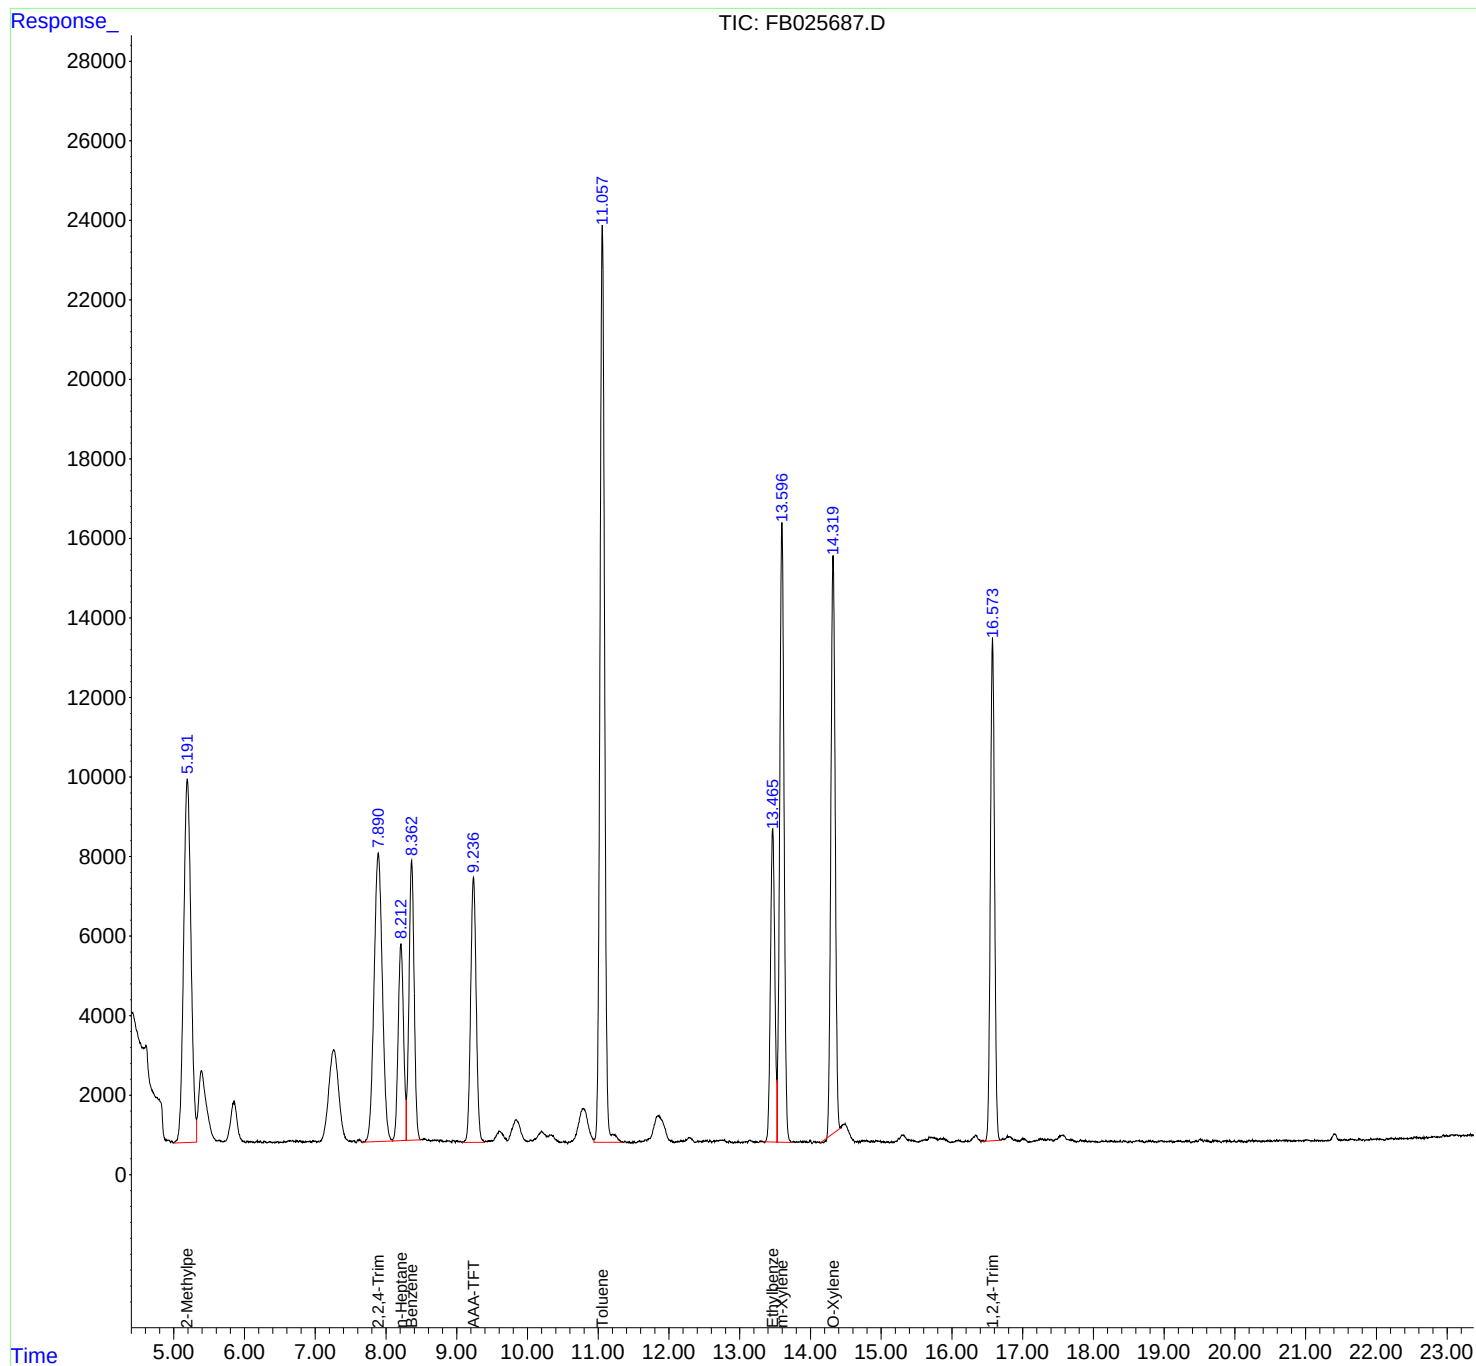


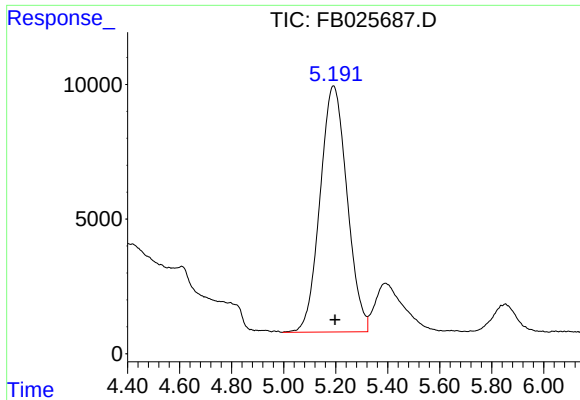

#1 2-Methylpentane


R.T.: 5.192 min
Delta R.T.: -0.006 min
Response: 658176
Conc: 27.21 ng/ml

Instrument :
FID_B
ClientSampleId :
SAMPLE-3-COMPMS

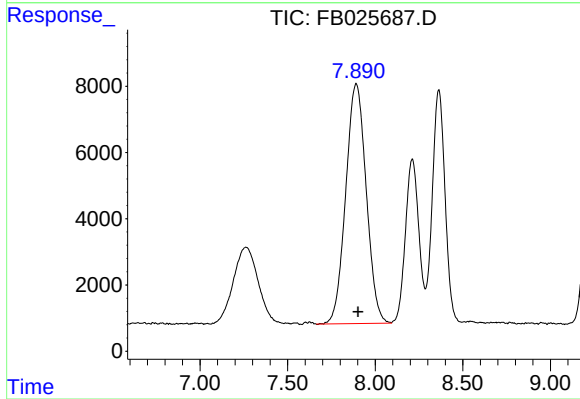


#2 2,2,4-Trimethylpentane

R.T.: 7.891 min
Delta R.T.: -0.011 min
Response: 588313
Conc: 31.63 ng/ml

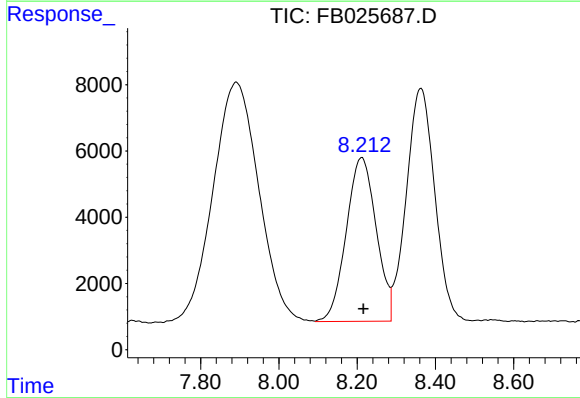


#3 n-Heptane

R.T.: 8.213 min
Delta R.T.: -0.003 min
Response: 262725
Conc: 8.97 ng/ml

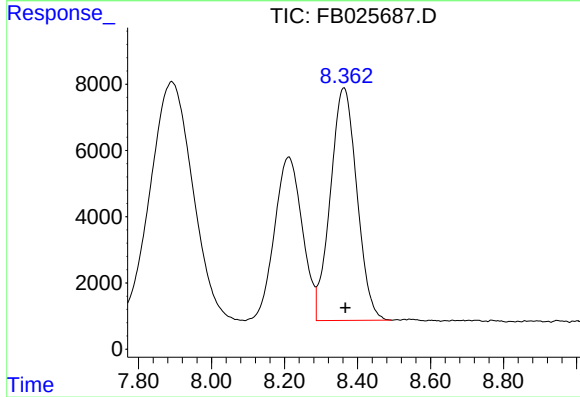

#4 Benzene


R.T.: 8.364 min
Delta R.T.: -0.003 min
Response: 354225
Conc: 9.17 ng/ml

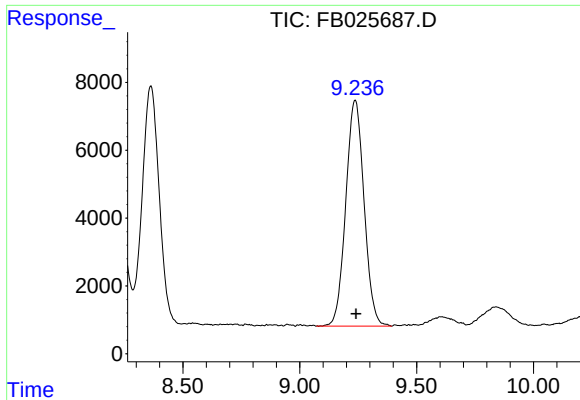

#5 AAA-TFT


R.T.: 9.238 min
Delta R.T.: -0.003 min
Response: 362099
Conc: 18.41 ng/ml

Instrument :
FID_B
ClientSampleId :
SAMPLE-3-COMPMS

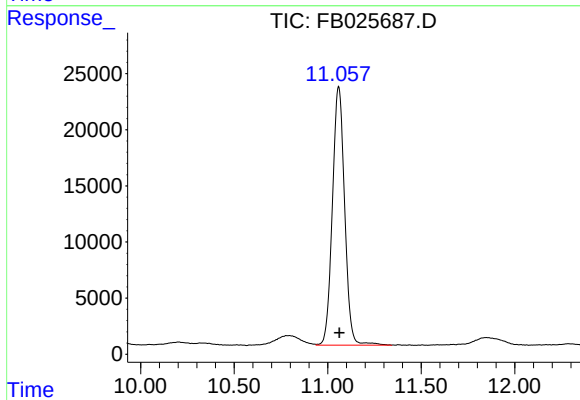


#6 Toluene

R.T.: 11.059 min
Delta R.T.: -0.003 min
Response: 1047552
Conc: 29.02 ng/ml

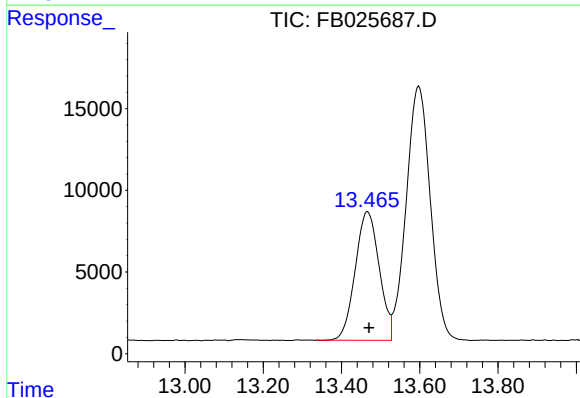


#7 Ethylbenzene

R.T.: 13.467 min
Delta R.T.: -0.004 min
Response: 334757
Conc: 9.76 ng/ml

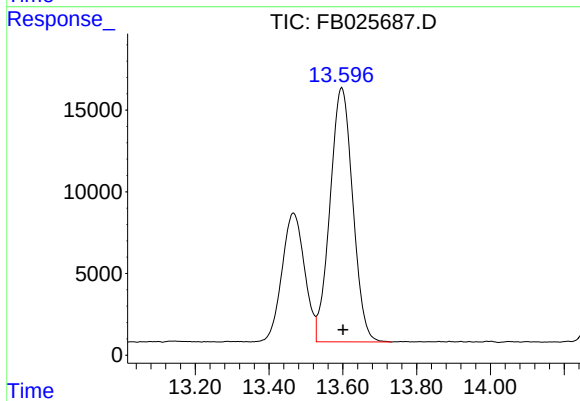

#8 m-Xylene


R.T.: 13.598 min
Delta R.T.: -0.003 min
Response: 667334
Conc: 19.63 ng/ml

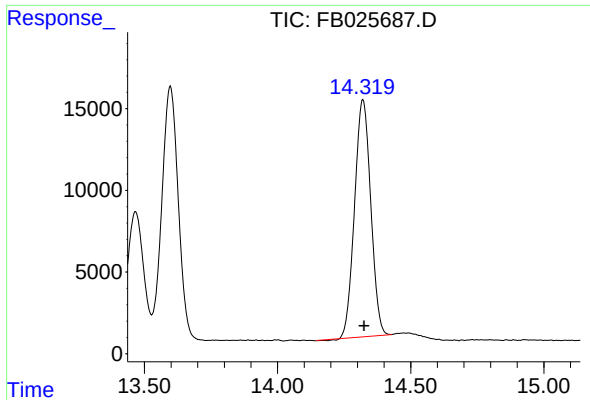

#9 O-Xylene

R.T.: 14.321 min
Delta R.T.: -0.004 min
Response: 612465
Conc: 18.80 ng/ml

Instrument :
FID_B
ClientSampleId :
SAMPLE-3-COMPMS

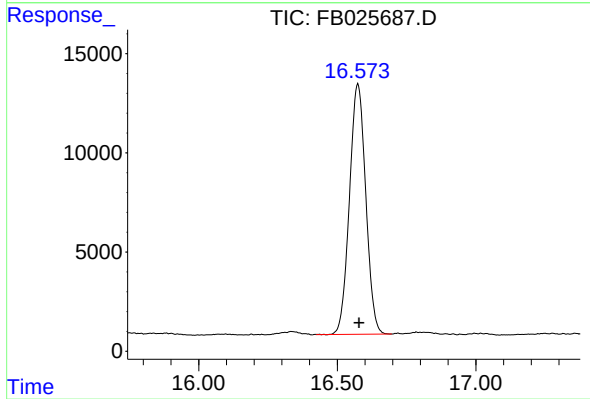

#10 1,2,4-Trimethylbenzene

R.T.: 16.575 min
Delta R.T.: -0.004 min
Response: 515619
Conc: 19.61 ng/ml