

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042921\
 Data File : FB025688.D
 Signal(s) : FID2B.CH
 Acq On : 29 Apr 2021 11:54
 Operator : DD/AJ
 Sample : M2199-03MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SAMPLE-3-COMPMSD

Integration File: Calibration.e
 Quant Time: Apr 30 01:22:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.241	398164	20.247 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.202	685069	28.318 ng/ml
2) t 2,2,4-Trimethylpentane	7.898	650353	34.969 ng/ml
3) t n-Heptane	8.217	297423	10.151 ng/ml
4) t Benzene	8.368	370906	9.600 ng/ml
6) t Toluene	11.062	1086421	30.101 ng/ml
7) t Ethylbenzene	13.469	349125	10.183 ng/ml
8) t m-Xylene	13.599	696959	20.504 ng/ml
9) t O-Xylene	14.323	639171	19.619 ng/ml
10) t 1,2,4-Trimethylbenzene	16.576	543496	20.675 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042921\
Data File : FB025688.D
Signal(s) : FID2B.CH
Acq On : 29 Apr 2021 11:54
Operator : DD/AJ
Sample : M2199-03MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SAMPLE-3-COMPMSD

Integration File: Calibration.e
Quant Time: Apr 30 01:22:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

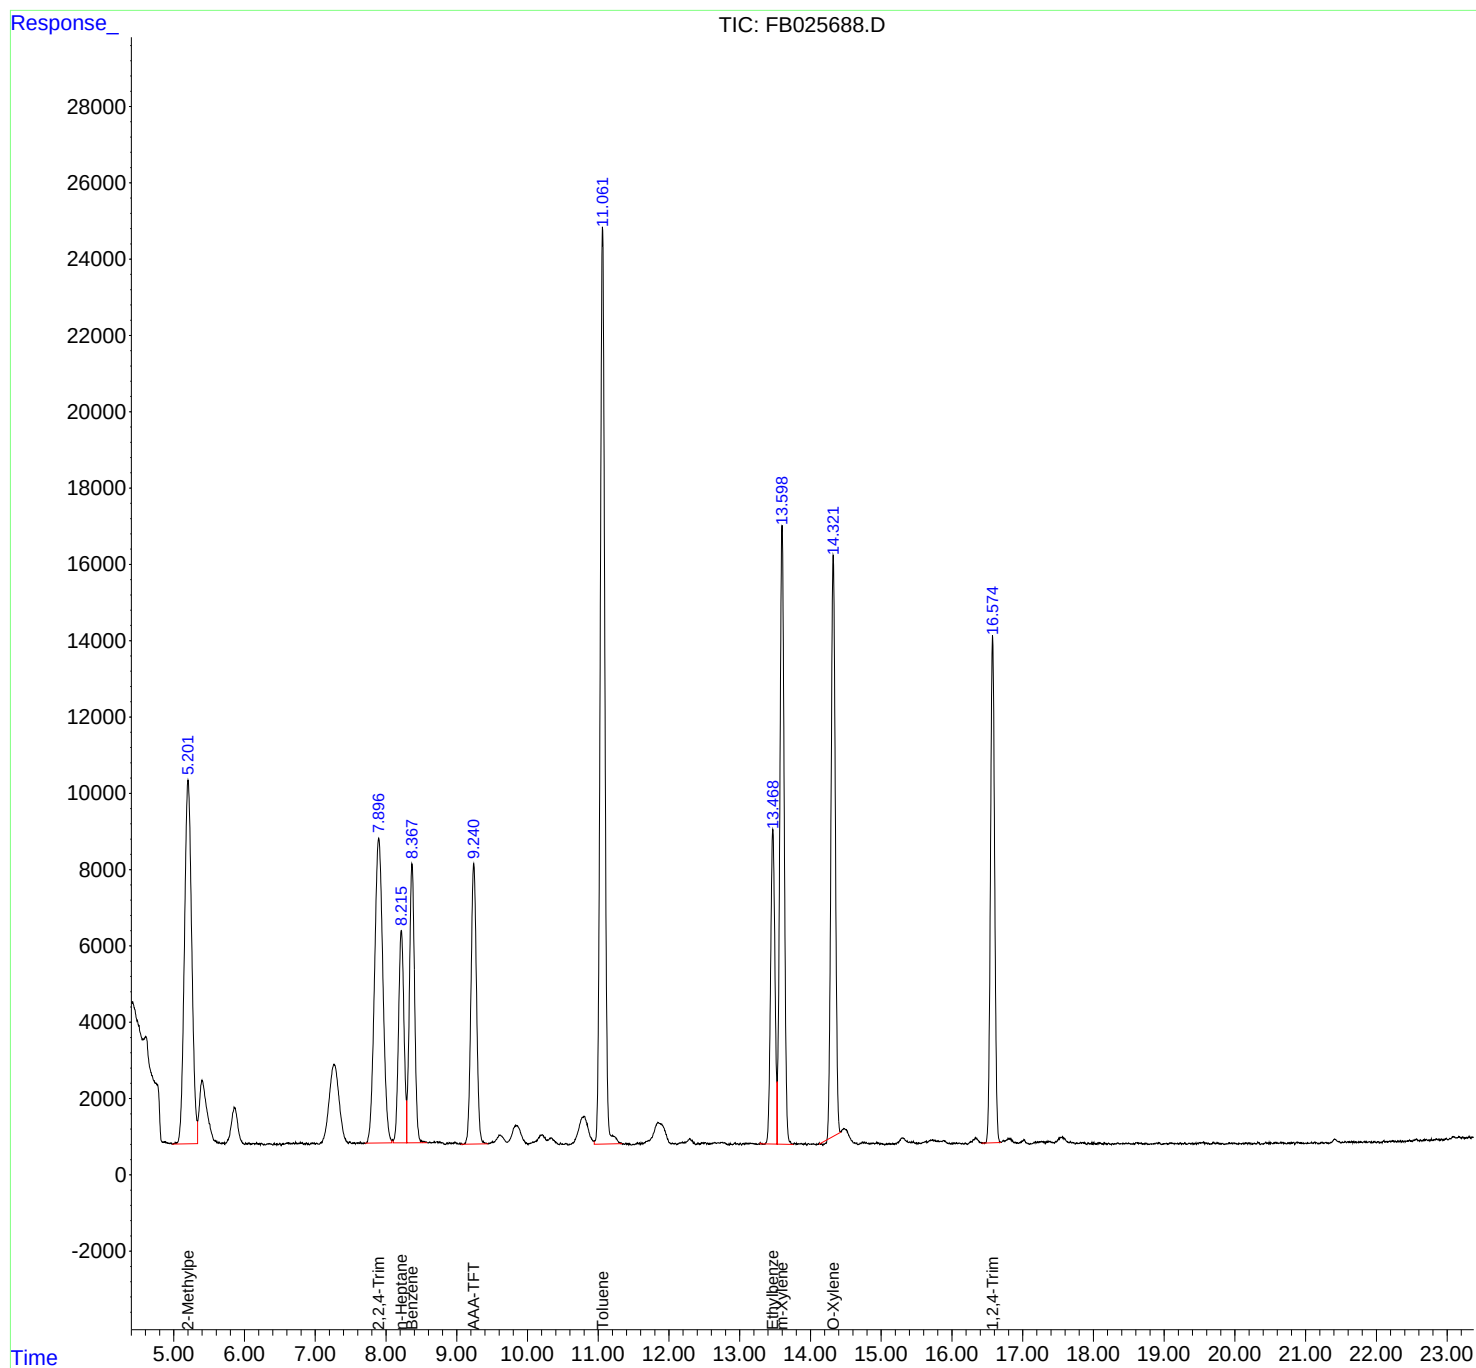


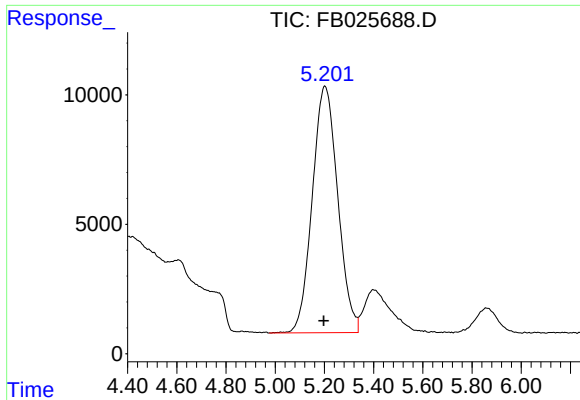

#1 2-Methylpentane


R.T.: 5.202 min
Delta R.T.: 0.004 min
Response: 685069
Conc: 28.32 ng/ml

Instrument :
FID_B
ClientSampleId :
SAMPLE-3-COMPMSD

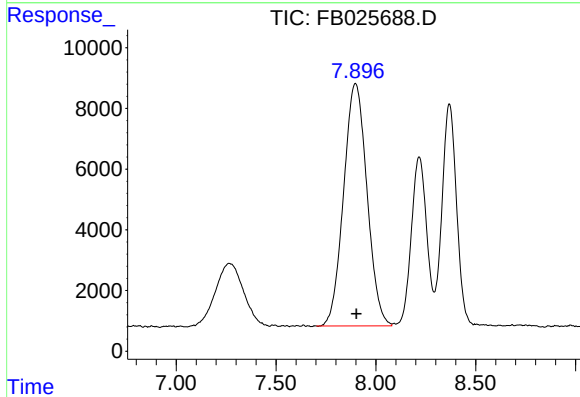


#2 2,2,4-Trimethylpentane

R.T.: 7.898 min
Delta R.T.: -0.004 min
Response: 650353
Conc: 34.97 ng/ml

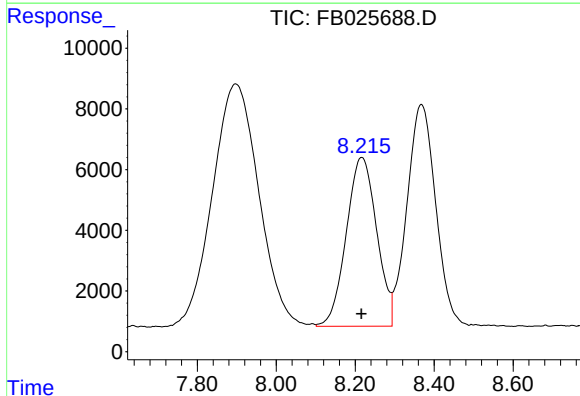


#3 n-Heptane

R.T.: 8.217 min
Delta R.T.: 0.000 min
Response: 297423
Conc: 10.15 ng/ml

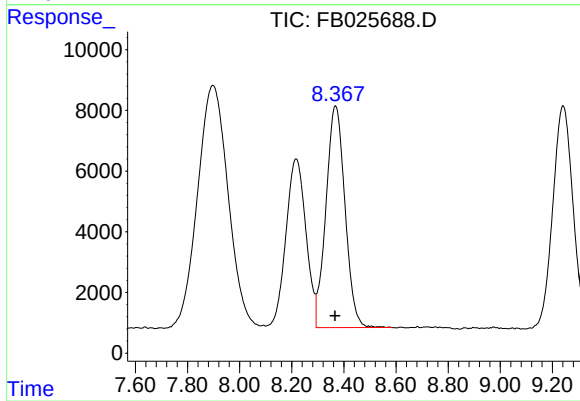

#4 Benzene


R.T.: 8.368 min
Delta R.T.: 0.002 min
Response: 370906
Conc: 9.60 ng/ml

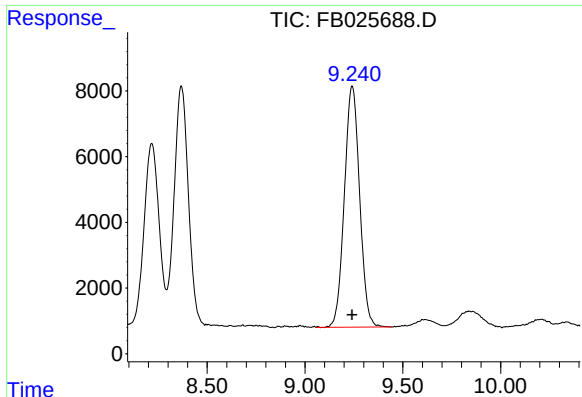

#5 AAA-TFT


R.T.: 9.241 min
Delta R.T.: 0.000 min
Response: 398164
Conc: 20.25 ng/ml

Instrument :
FID_B
ClientSampleId :
SAMPLE-3-COMPMSD

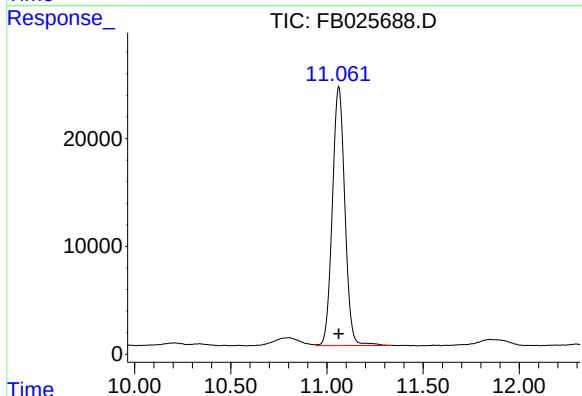


#6 Toluene

R.T.: 11.062 min
Delta R.T.: 0.000 min
Response: 1086421
Conc: 30.10 ng/ml

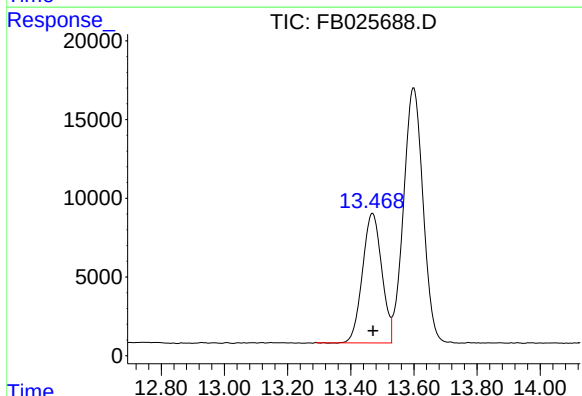


#7 Ethylbenzene

R.T.: 13.469 min
Delta R.T.: -0.001 min
Response: 349125
Conc: 10.18 ng/ml

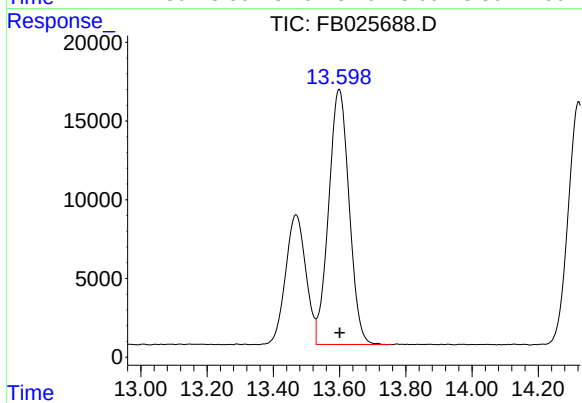

#8 m-Xylene


R.T.: 13.599 min
Delta R.T.: -0.002 min
Response: 696959
Conc: 20.50 ng/ml

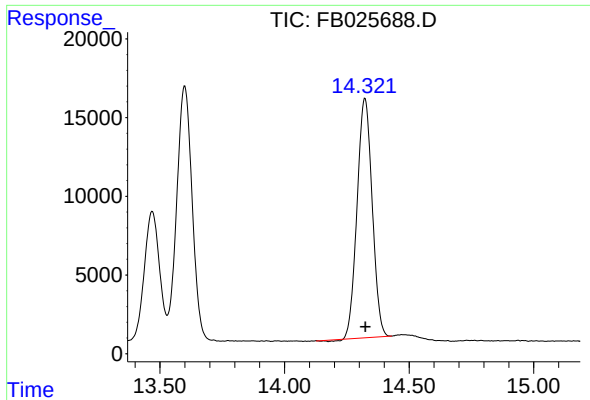

#9 O-Xylene

R.T.: 14.323 min
Delta R.T.: -0.002 min
Response: 639171
Conc: 19.62 ng/ml

Instrument :
FID_B
ClientSampleId :
SAMPLE-3-COMPMSD

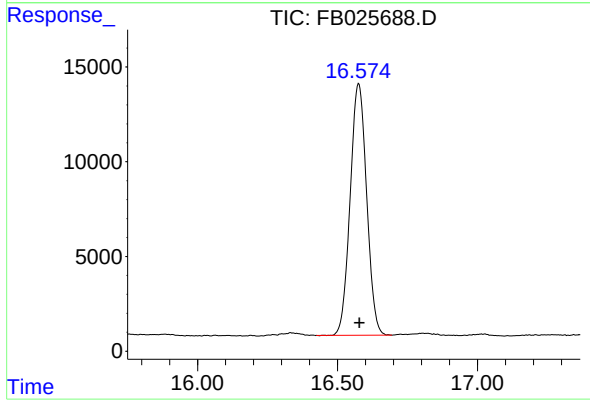

#10 1,2,4-Trimethylbenzene

R.T.: 16.576 min
Delta R.T.: -0.003 min
Response: 543496
Conc: 20.67 ng/ml