

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050119\
 Data File : FB020903.D
 Signal(s) : FID2B.CH
 Acq On : 1 May 2019 14:32
 Operator : MJ/SJ
 Sample : VBF0501S2
 Misc : 5.00g/5.00ml DI WATER (Methanol blank)
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 VBF0501S2

Integration File: Calibration.e
 Quant Time: May 02 01:39:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	362697	20.218 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.845	18812	0.417 ng/ml
2) t 2,2,4-Trimethylpentane	7.580	41730	1.001 ng/ml
3) t n-Heptane	7.949	76204	1.925 ng/ml
4) t Benzene	8.082	37839	0.904 ng/ml
6) t Toluene	10.839	342067	12.348 ng/ml
7) t Ethylbenzene	13.283	2503259	89.255 ng/ml
8) t m-Xylene	13.417	990221	33.318 ng/ml
9) t O-Xylene	14.147	594538	19.181 ng/ml
10) t 1,2,4-Trimethylbenzene	16.428	3521155	113.535 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050119\
Data File : FB020903.D
Signal(s) : FID2B.CH
Acq On : 1 May 2019 14:32
Operator : MJ/SJ
Sample : VBF0501S2
Misc : 5.00g/5.00ml DI WATER (Methanol blank)
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0501S2

Integration File: Calibration.e
Quant Time: May 02 01:39:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

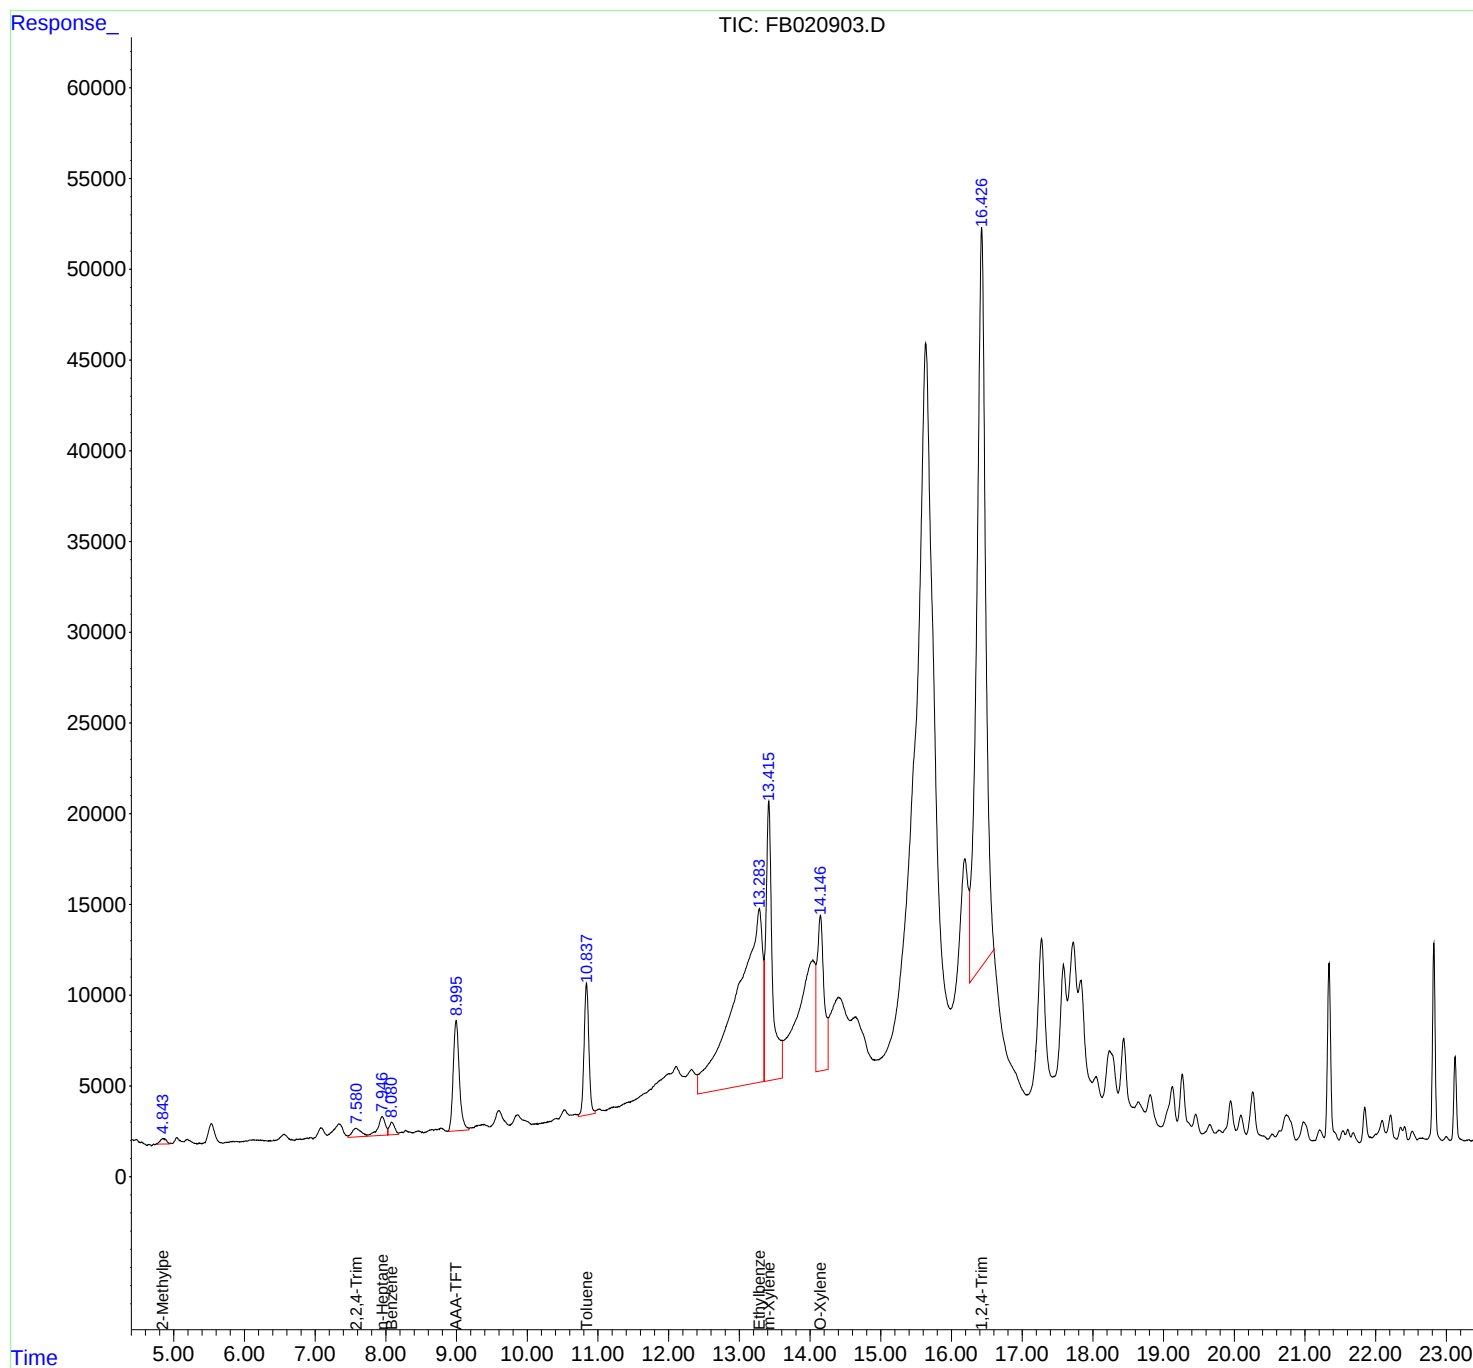


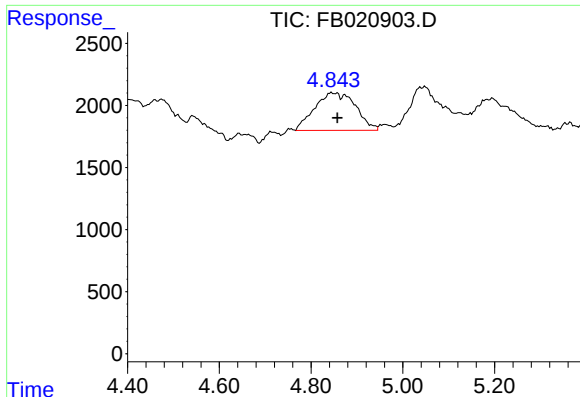

#1 2-Methylpentane


R.T.: 4.845 min
Delta R.T.: -0.012 min
Response: 18812
Conc: 0.42 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0501S2

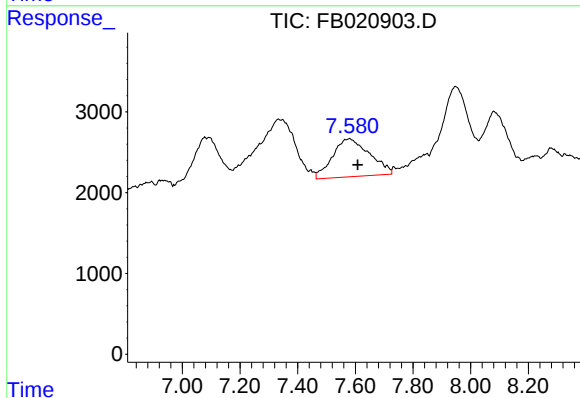


#2 2,2,4-Trimethylpentane

R.T.: 7.580 min
Delta R.T.: -0.029 min
Response: 41730
Conc: 1.00 ng/ml

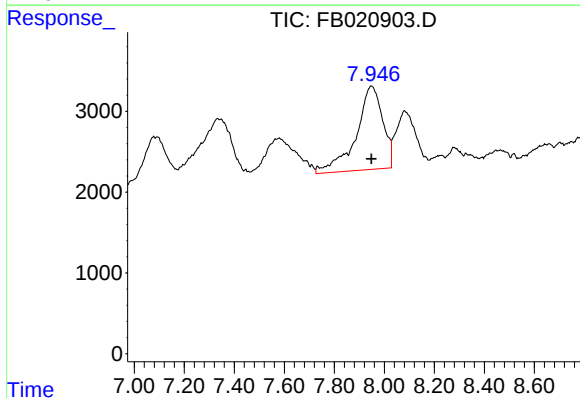


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 76204
Conc: 1.92 ng/ml

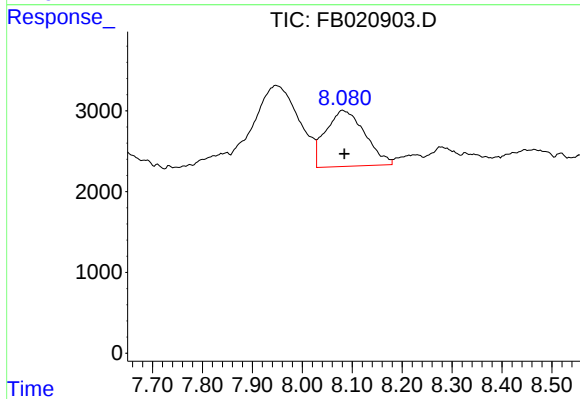

#4 Benzene


R.T.: 8.082 min
Delta R.T.: -0.002 min
Response: 37839
Conc: 0.90 ng/ml

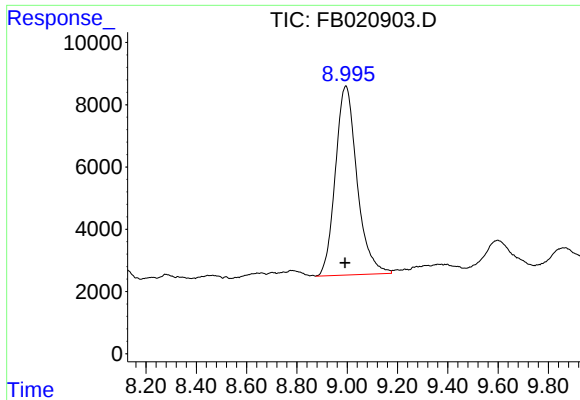

#5 AAA-TFT


R.T.: 8.995 min
Delta R.T.: 0.003 min
Response: 362697
Conc: 20.22 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0501S2

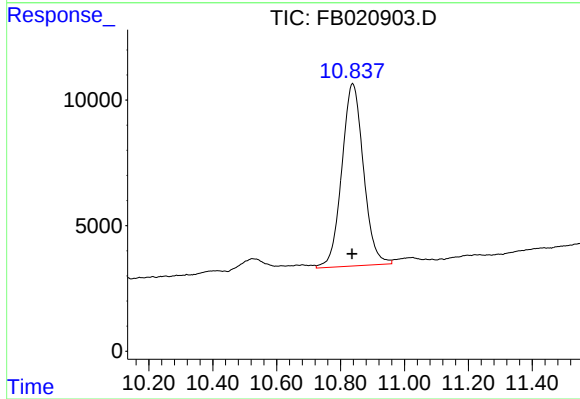


#6 Toluene

R.T.: 10.839 min
Delta R.T.: 0.003 min
Response: 342067
Conc: 12.35 ng/ml

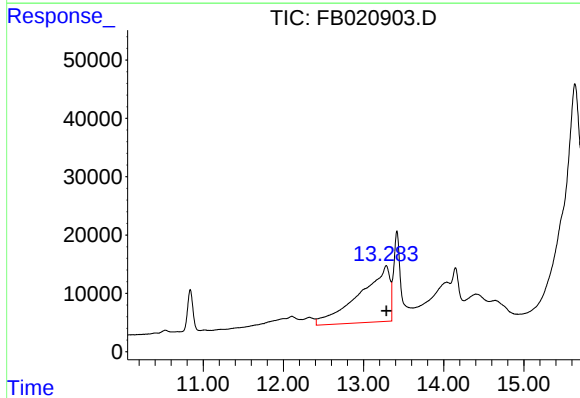


#7 Ethylbenzene

R.T.: 13.283 min
Delta R.T.: -0.002 min
Response: 2503259
Conc: 89.26 ng/ml

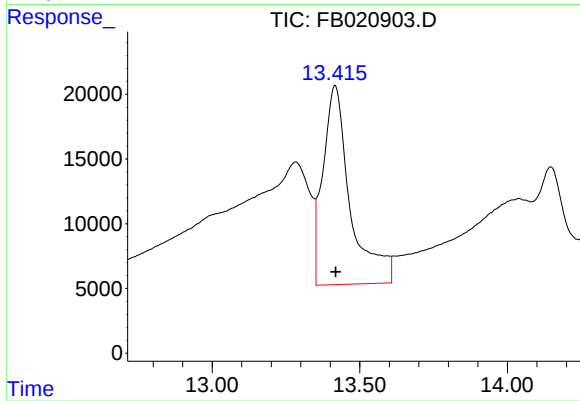

#8 m-Xylene


R.T.: 13.417 min
Delta R.T.: -0.002 min
Response: 990221
Conc: 33.32 ng/ml

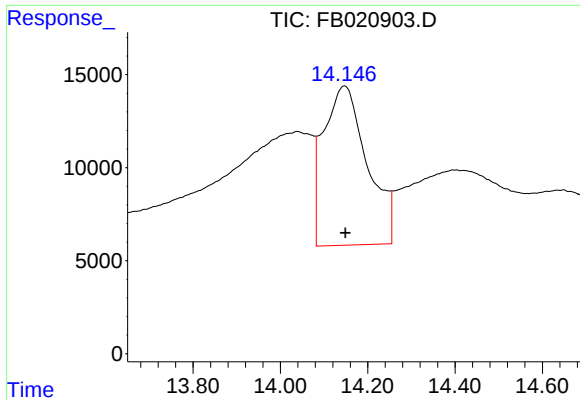

#9 O-Xylene

R.T.: 14.147 min
Delta R.T.: -0.002 min
Response: 594538
Conc: 19.18 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0501S2

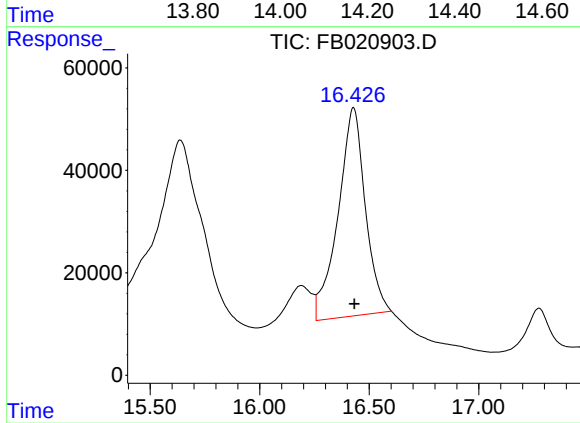

#10 1,2,4-Trimethylbenzene

R.T.: 16.428 min
Delta R.T.: -0.005 min
Response: 3521155
Conc: 113.54 ng/ml