

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050119\
 Data File : FB020917.D
 Signal(s) : FID2B.CH
 Acq On : 1 May 2019 22:40
 Operator : MJ/SJ
 Sample : K2191-02 50X
 Misc : 5.00g/5.00ml DI WATER (Methanol)
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 P-66-TP-A

Integration File: Calibration.e
 Quant Time: May 02 01:41:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	395188	22.029 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.836	7878	0.175 ng/ml
4) t Benzene	8.097	3077	0.074 ng/ml
6) t Toluene	10.840	19670	0.710 ng/ml
7) t Ethylbenzene	13.276	8137	0.290 ng/ml
8) t m-Xylene	13.419	26964	0.907 ng/ml
9) t O-Xylene	14.157	15956	0.515 ng/ml
10) t 1,2,4-Trimethylbenzene	16.433	18257	0.589 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050119\
Data File : FB020917.D
Signal(s) : FID2B.CH
Acq On : 1 May 2019 22:40
Operator : MJ/SJ
Sample : K2191-02 50X
Misc : 5.00g/5.00ml DI WATER (Methanol)
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
P-66-TP-A

Integration File: Calibration.e
Quant Time: May 02 01:41:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

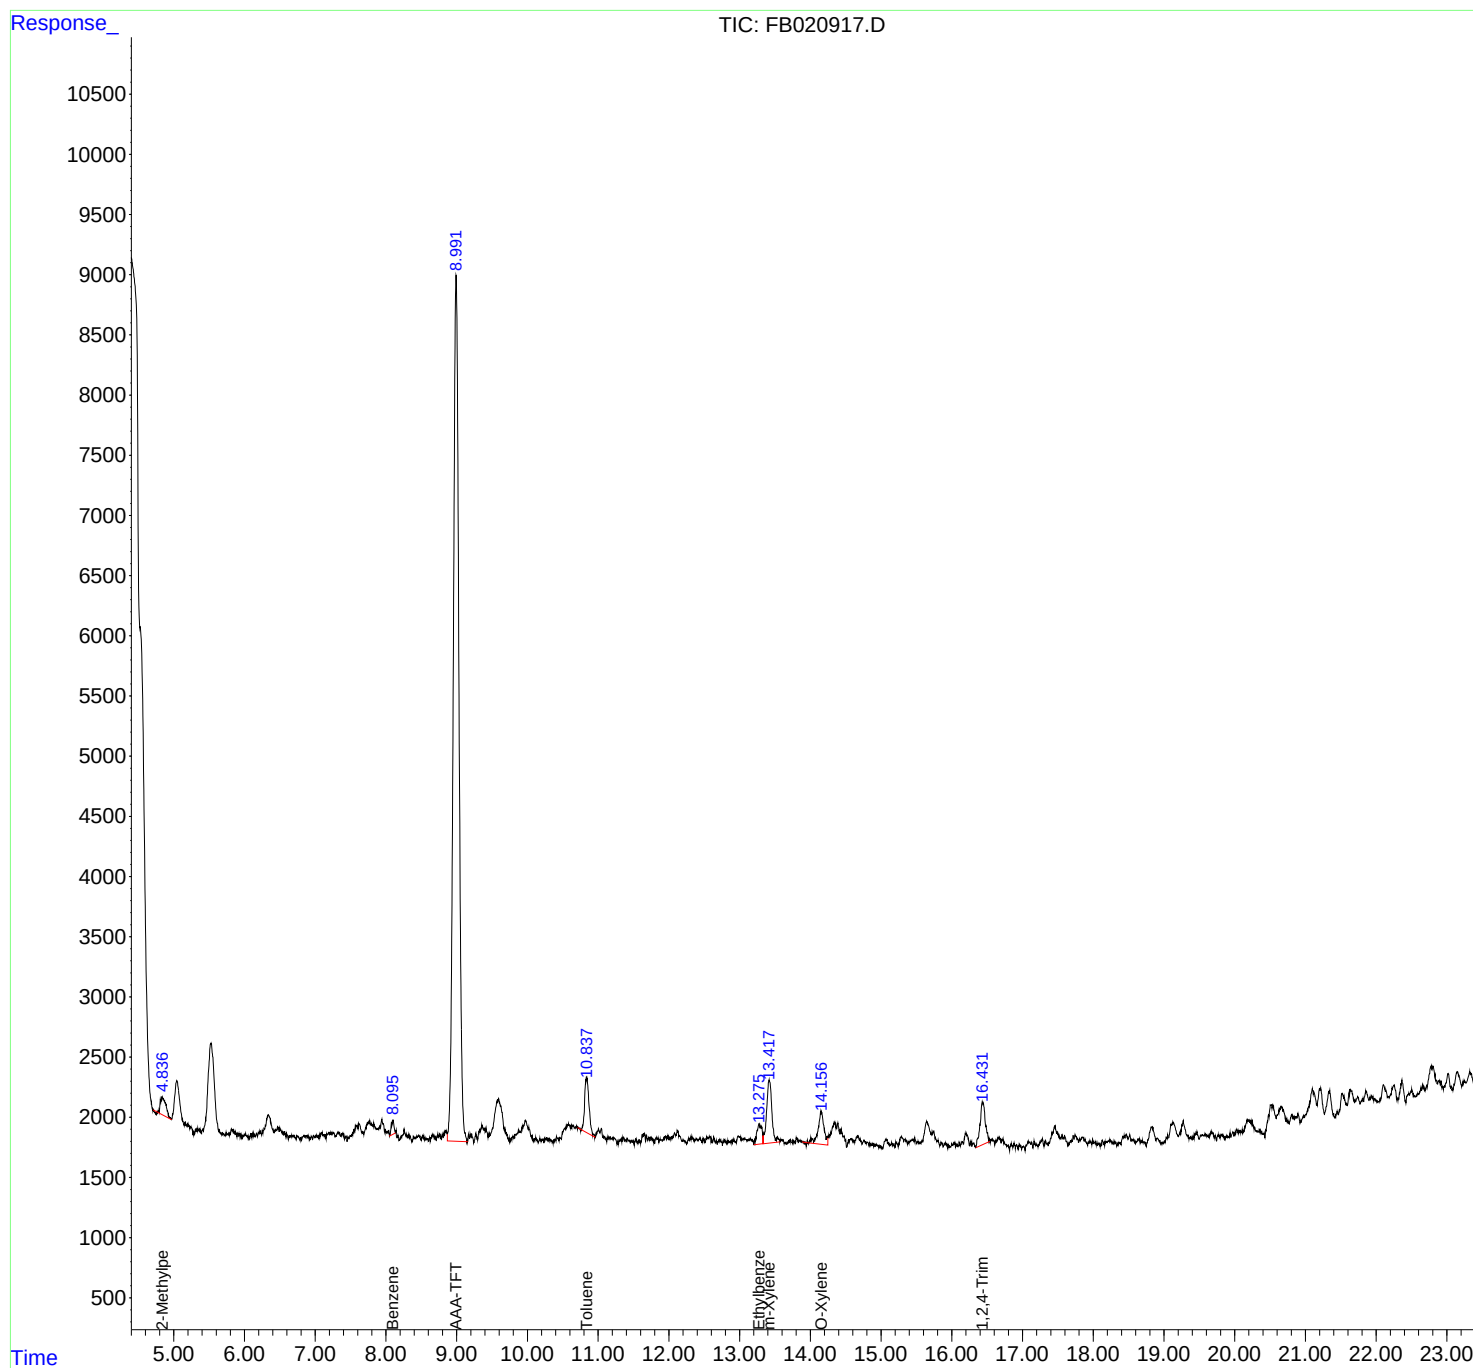


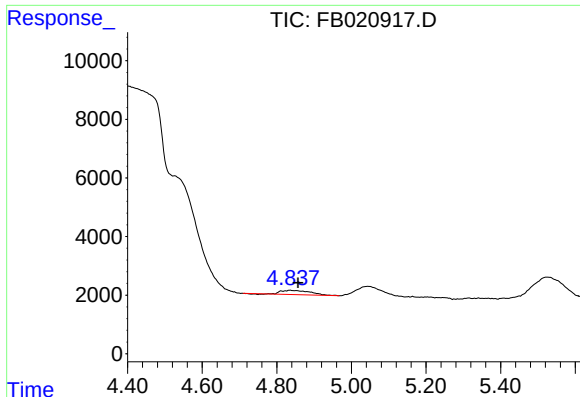

#1 2-Methylpentane


R.T.: 4.836 min
Delta R.T.: -0.021 min
Response: 7878
Conc: 0.17 ng/ml

Instrument :
FID_B
ClientSampleId :
P-66-TP-A

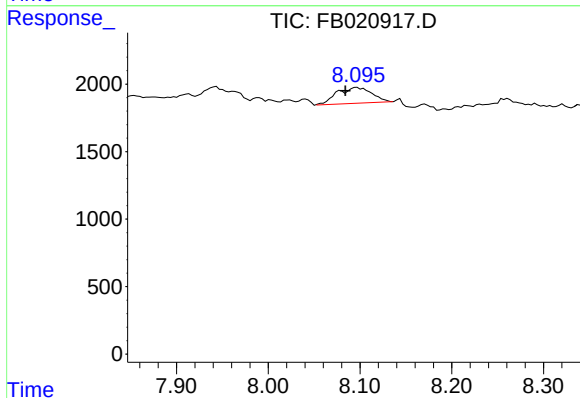


#4 Benzene

R.T.: 8.097 min
Delta R.T.: 0.012 min
Response: 3077
Conc: 0.07 ng/ml

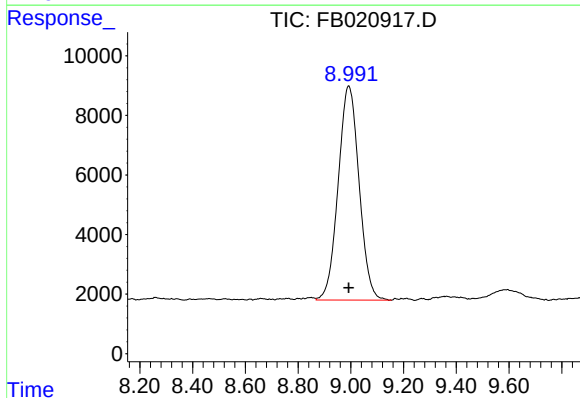


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 395188
Conc: 22.03 ng/ml

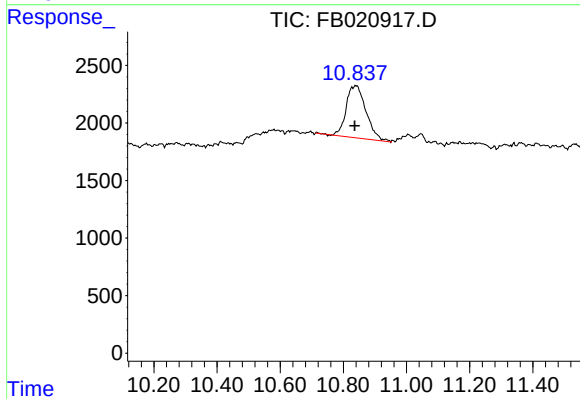

#6 Toluene


R.T.: 10.840 min
Delta R.T.: 0.004 min
Response: 19670
Conc: 0.71 ng/ml

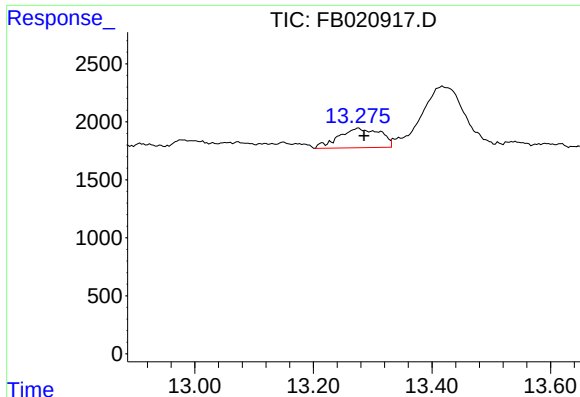

#7 Ethylbenzene


R.T.: 13.276 min
Delta R.T.: -0.010 min
Response: 8137
Conc: 0.29 ng/ml

Instrument :
FID_B
ClientSampleId :
P-66-TP-A

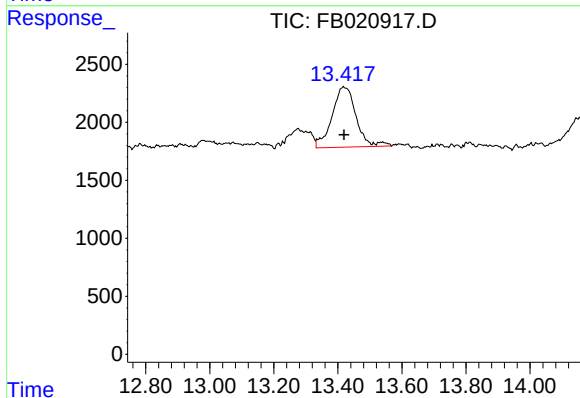


#8 m-Xylene

R.T.: 13.419 min
Delta R.T.: 0.000 min
Response: 26964
Conc: 0.91 ng/ml

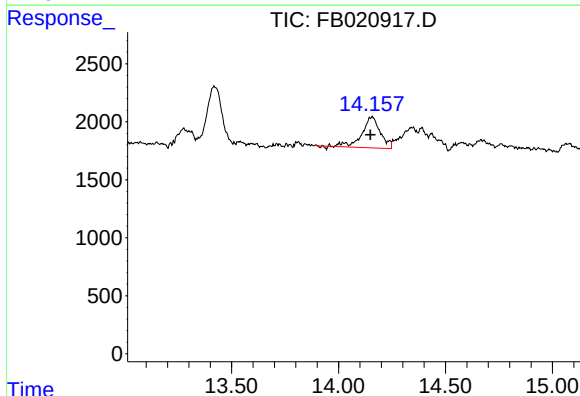

#9 o-Xylene

R.T.: 14.157 min
Delta R.T.: 0.008 min
Response: 15956
Conc: 0.51 ng/ml

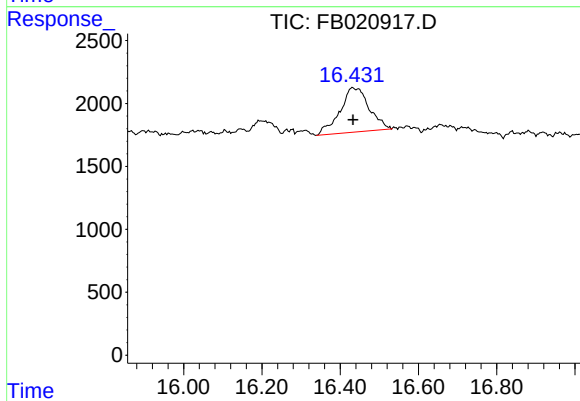

#10 1,2,4-Trimethylbenzene

R.T.: 16.433 min
Delta R.T.: 0.000 min
Response: 18257
Conc: 0.59 ng/ml