

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050119\
 Data File : FB020901.D
 Signal(s) : FID2B.CH
 Acq On : 1 May 2019 12:59
 Operator : MJ/SJ
 Sample : K2241-09
 Misc : 1 PPB MDL WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File: Calibration.e
 Quant Time: May 02 01:38:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.994	290984	16.220 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.859	55175	1.223 ng/ml
2) t 2,2,4-Trimethylpentane	7.606	55072	1.321 ng/ml
3) t n-Heptane	7.959	17300	0.437 ng/ml
4) t Benzene	8.084	17047	0.407 ng/ml
6) t Toluene	10.839	33738	1.218 ng/ml
7) t Ethylbenzene	13.289	14881	0.531 ng/ml
8) t m-Xylene	13.417	25343	0.853 ng/ml
9) t O-Xylene	14.149	23603	0.761 ng/ml
10) t 1,2,4-Trimethylbenzene	16.436	28951	0.933 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050119\
Data File : FB020901.D
Signal(s) : FID2B.CH
Acq On : 1 May 2019 12:59
Operator : MJ/SJ
Sample : K2241-09
Misc : 1 PPB MDL WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Integration File: Calibration.e
Quant Time: May 02 01:38:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

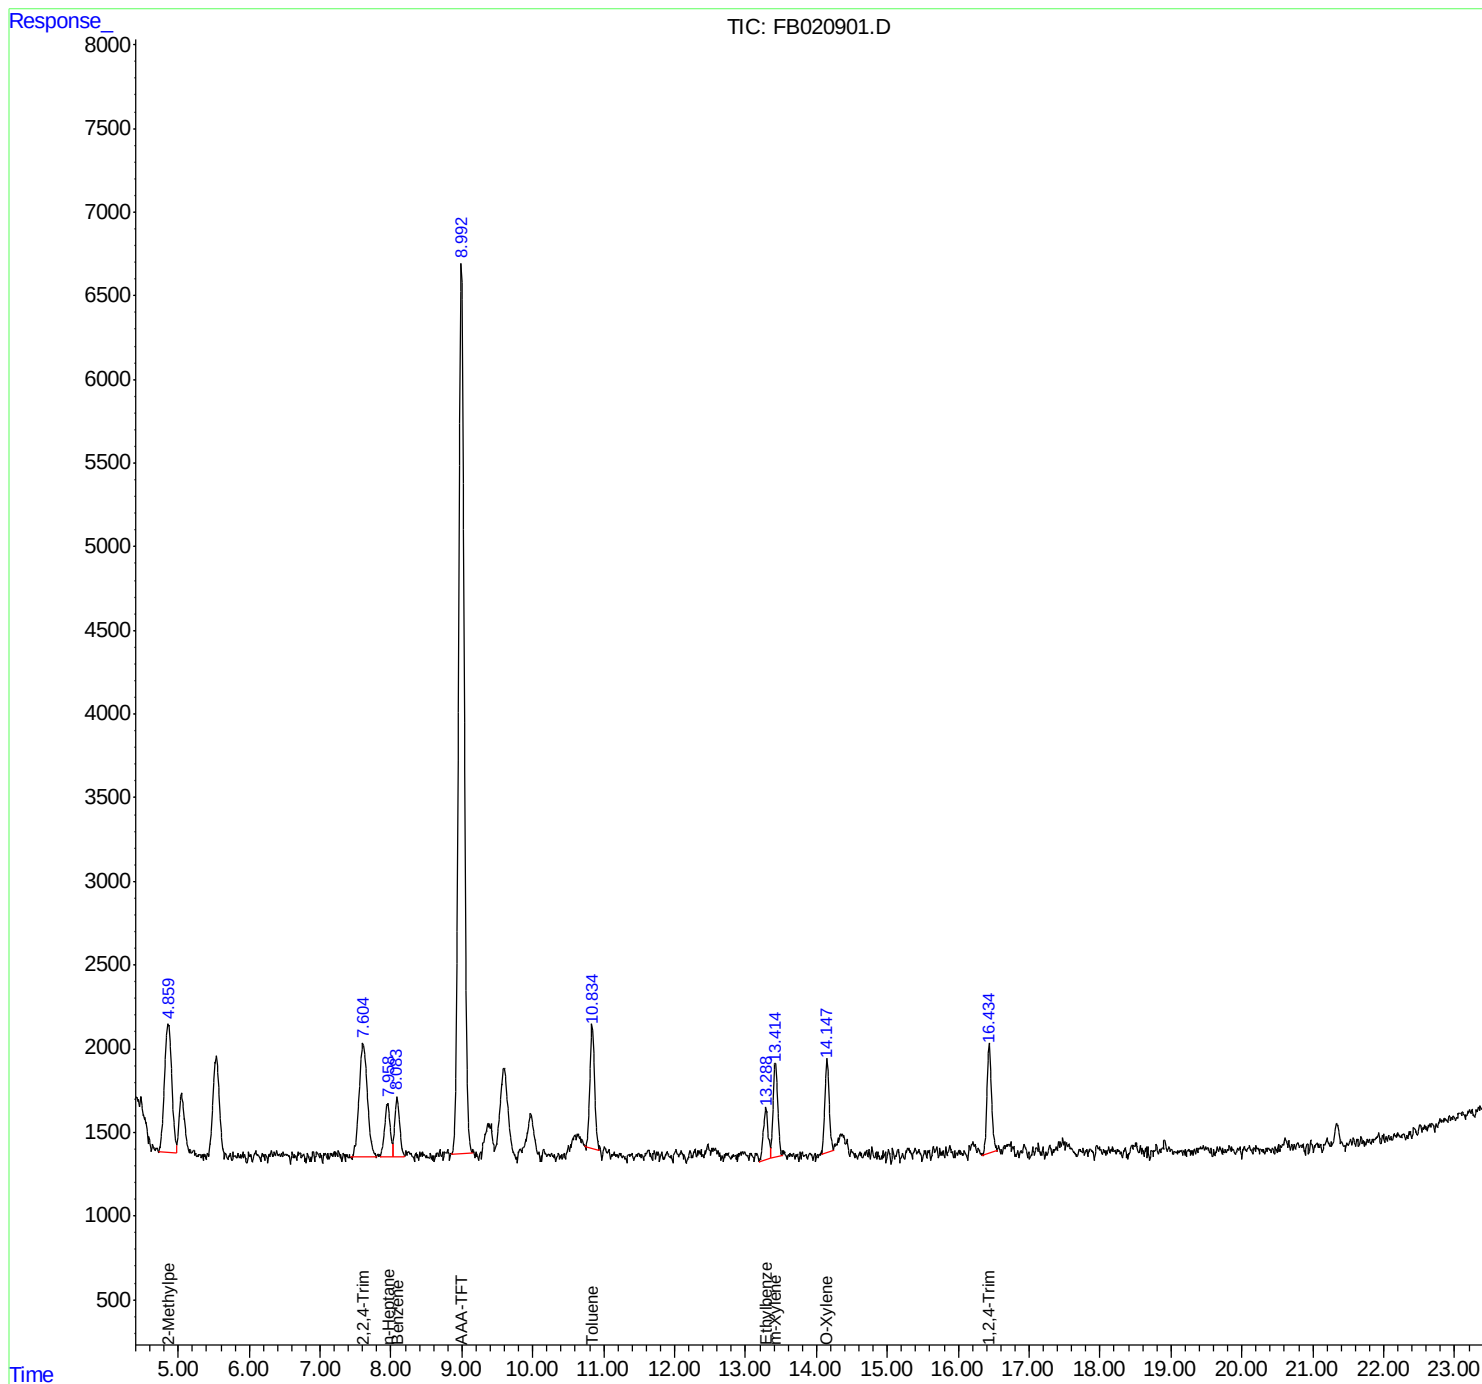


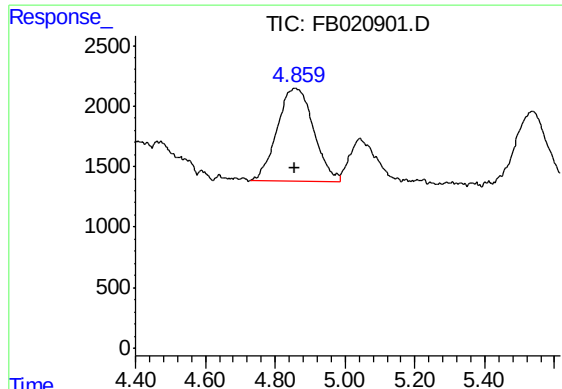

#1 2-Methylpentane


R.T.: 4.859 min
Delta R.T.: 0.002 min
Response: 55175
Conc: 1.22 ng/ml

Instrument :
FID_B
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

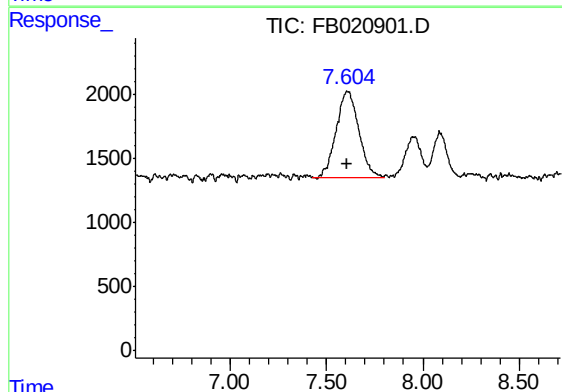


#2 2,2,4-Trimethylpentane

R.T.: 7.606 min
Delta R.T.: -0.003 min
Response: 55072
Conc: 1.32 ng/ml

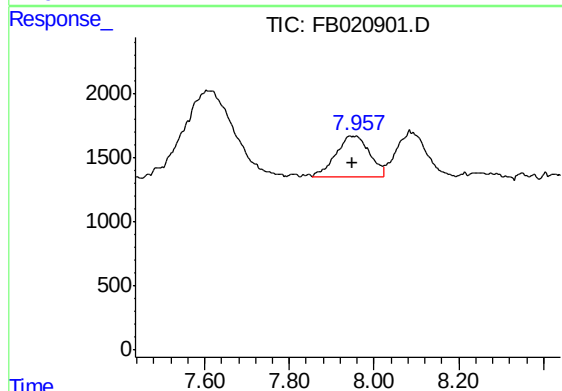


#3 n-Heptane

R.T.: 7.959 min
Delta R.T.: 0.010 min
Response: 17300
Conc: 0.44 ng/ml

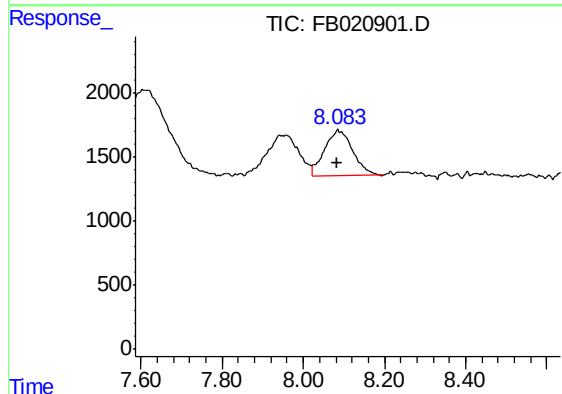

#4 Benzene


R.T.: 8.084 min
Delta R.T.: 0.000 min
Response: 17047
Conc: 0.41 ng/ml

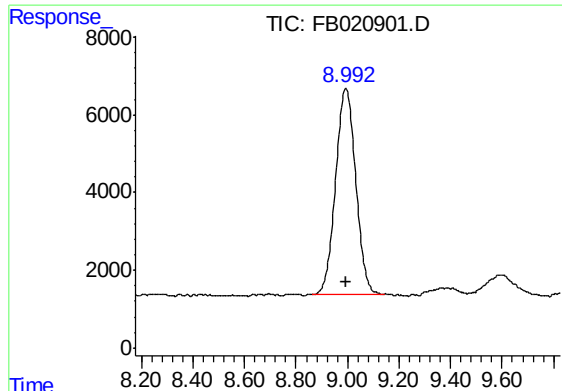

#5 AAA-TFT


R.T.: 8.994 min
Delta R.T.: 0.002 min
Response: 290984
Conc: 16.22 ng/ml

Instrument :
FID_B
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

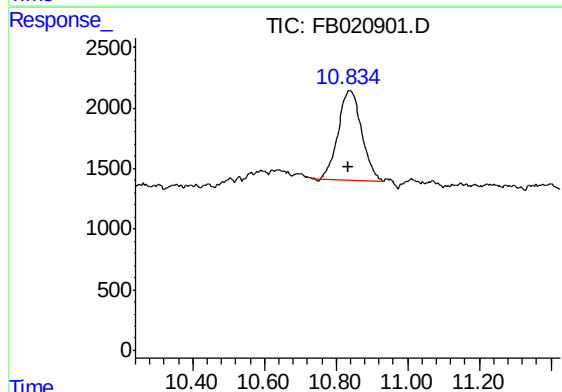


#6 Toluene

R.T.: 10.839 min
Delta R.T.: 0.003 min
Response: 33738
Conc: 1.22 ng/ml

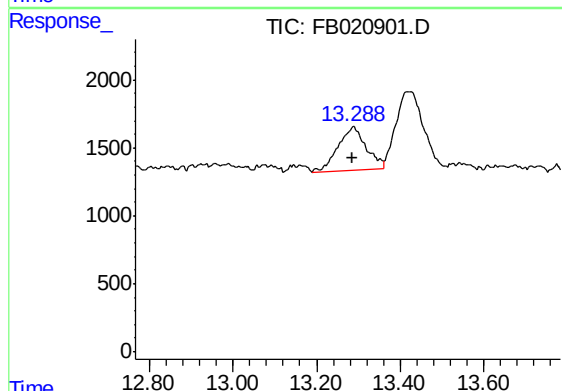


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: 0.003 min
Response: 14881
Conc: 0.53 ng/ml

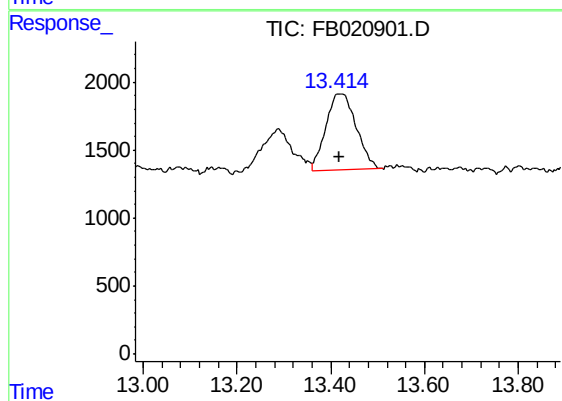

#8 m-Xylene


R.T.: 13.417 min
Delta R.T.: -0.002 min
Response: 25343
Conc: 0.85 ng/ml

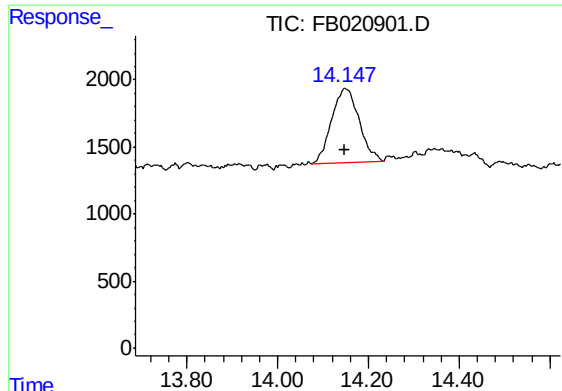

#9 O-Xylene

R.T.: 14.149 min
Delta R.T.: 0.000 min
Response: 23603
Conc: 0.76 ng/ml

Instrument :
FID_B
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

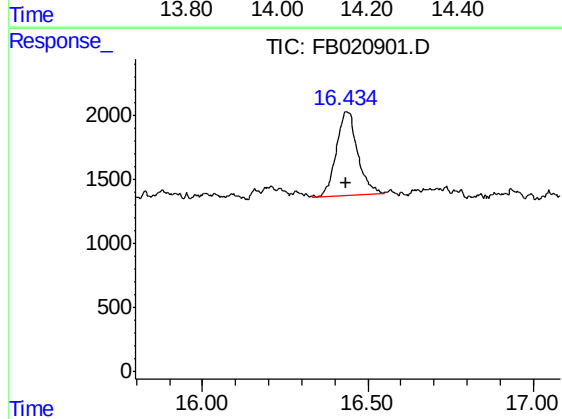

#10 1,2,4-Trimethylbenzene

R.T.: 16.436 min
Delta R.T.: 0.003 min
Response: 28951
Conc: 0.93 ng/ml