

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050123\
 Data File : FB029757.D
 Signal(s) : FID2B.CH
 Acq On : 1 May 2023 13:00
 Operator : YP/AJ
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 02 01:42:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
 Quant Title :
 QLast Update : Mon Apr 17 12:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	245334	18.410 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.419	261	0.017 ng/ml
3) t n-Heptane	7.756	33811	2.101 ng/ml
4) t Benzene	7.893	8223	0.414 ng/ml
6) t Toluene	10.619	201835	10.450 ng/ml
7) t Ethylbenzene	13.055	72611	4.012 ng/ml
8) t m-Xylene	13.187	276114	15.267 ng/ml
9) t O-Xylene	13.918	118847	6.778 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	276057	15.447 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050123\
Data File : FB029757.D
Signal(s) : FID2B.CH
Acq On : 1 May 2023 13:00
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 02 01:42:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

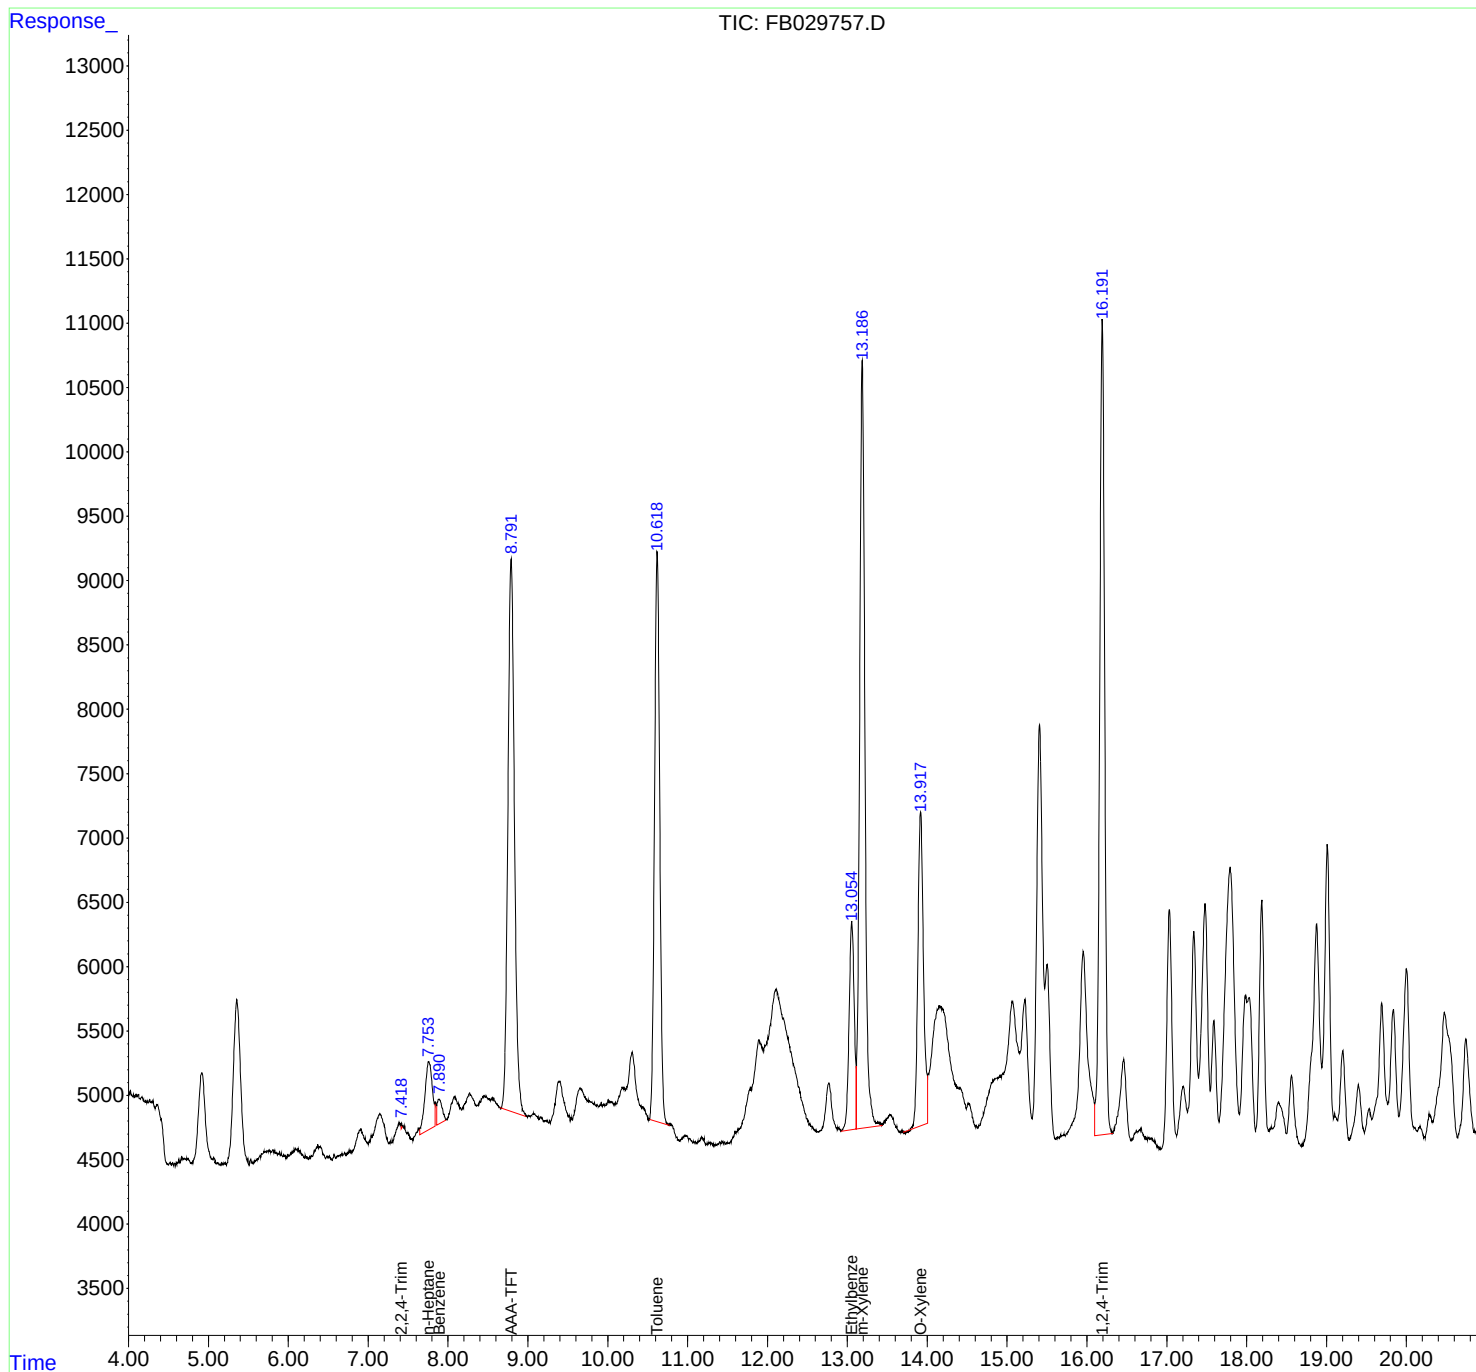


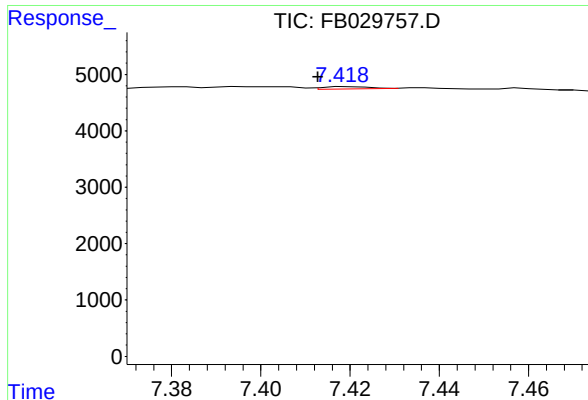

#2 2,2,4-Trimethylpentane


R.T.: 7.419 min
Delta R.T.: 0.006 min
Response: 261
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :

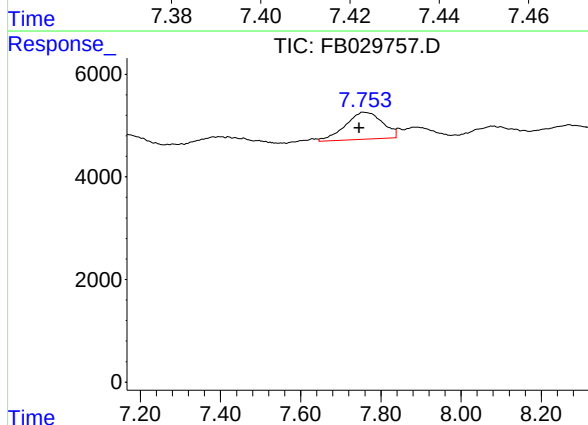


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.009 min
Response: 33811
Conc: 2.10 ng/ml

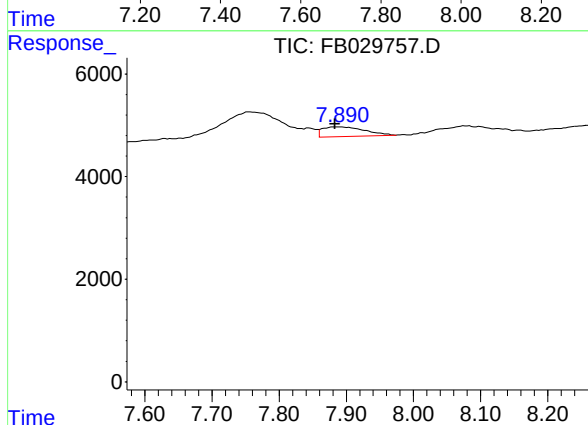


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.009 min
Response: 8223
Conc: 0.41 ng/ml

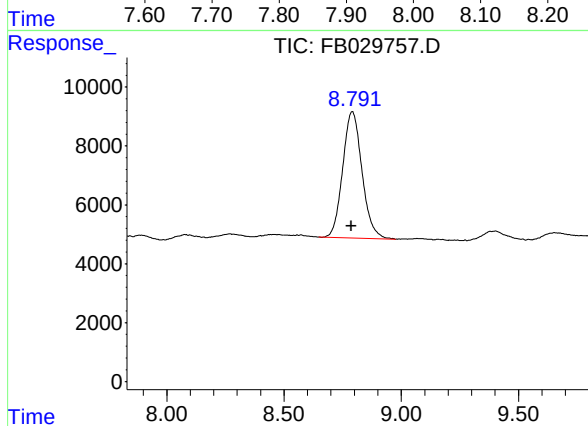

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.004 min
Response: 245334
Conc: 18.41 ng/ml

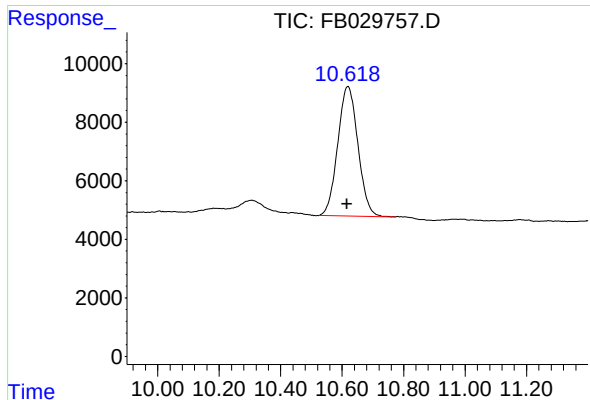

#6 Toluene


R.T.: 10.619 min
Delta R.T.: 0.004 min
Response: 201835
Conc: 10.45 ng/ml

Instrument :
FID_B
ClientSampleId :

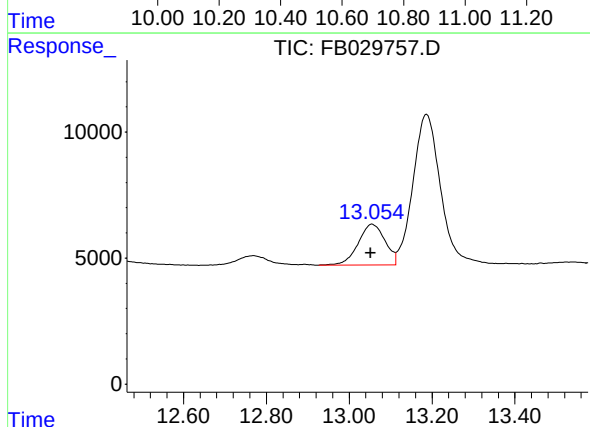


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.003 min
Response: 72611
Conc: 4.01 ng/ml

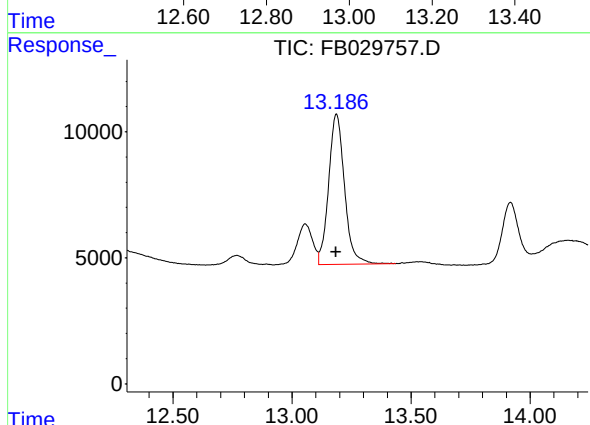


#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: 0.002 min
Response: 276114
Conc: 15.27 ng/ml

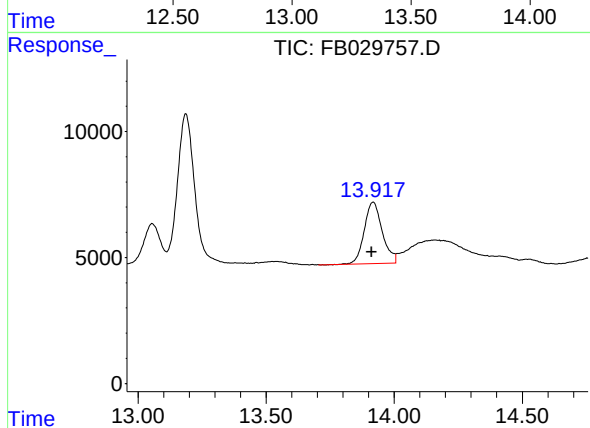

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.007 min
Response: 118847
Conc: 6.78 ng/ml

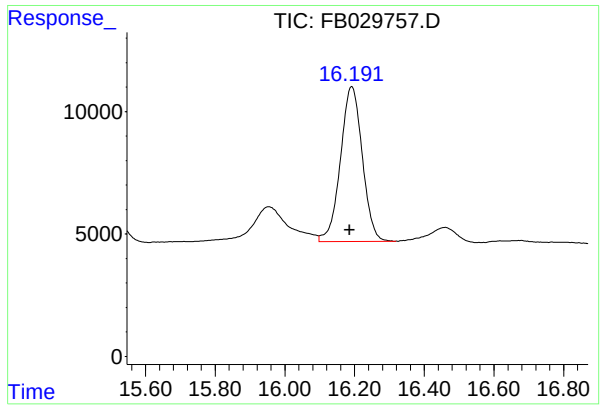

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.006 min
Response: 276057
Conc: 15.45 ng/ml

Instrument :

FID_B

ClientSampleId :