

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050123\
 Data File : FB029761.D
 Signal(s) : FID2B.CH
 Acq On : 1 May 2023 15:29
 Operator : YP/AJ
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 02 01:42:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
 Quant Title :
 QLast Update : Mon Apr 17 12:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.791	269925	20.255 ng/ml
Target Compounds				
6) t	Toluene	10.620	18222	0.943 ng/ml
7) t	Ethylbenzene	13.056	4936	0.273 ng/ml
8) t	m-Xylene	13.188	18101	1.001 ng/ml
9) t	O-Xylene	13.918	5935	0.338 ng/ml
10) t	1,2,4-Trimethylbenzene	16.187	12054	0.674 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050123\
Data File : FB029761.D
Signal(s) : FID2B.CH
Acq On : 1 May 2023 15:29
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 02 01:42:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

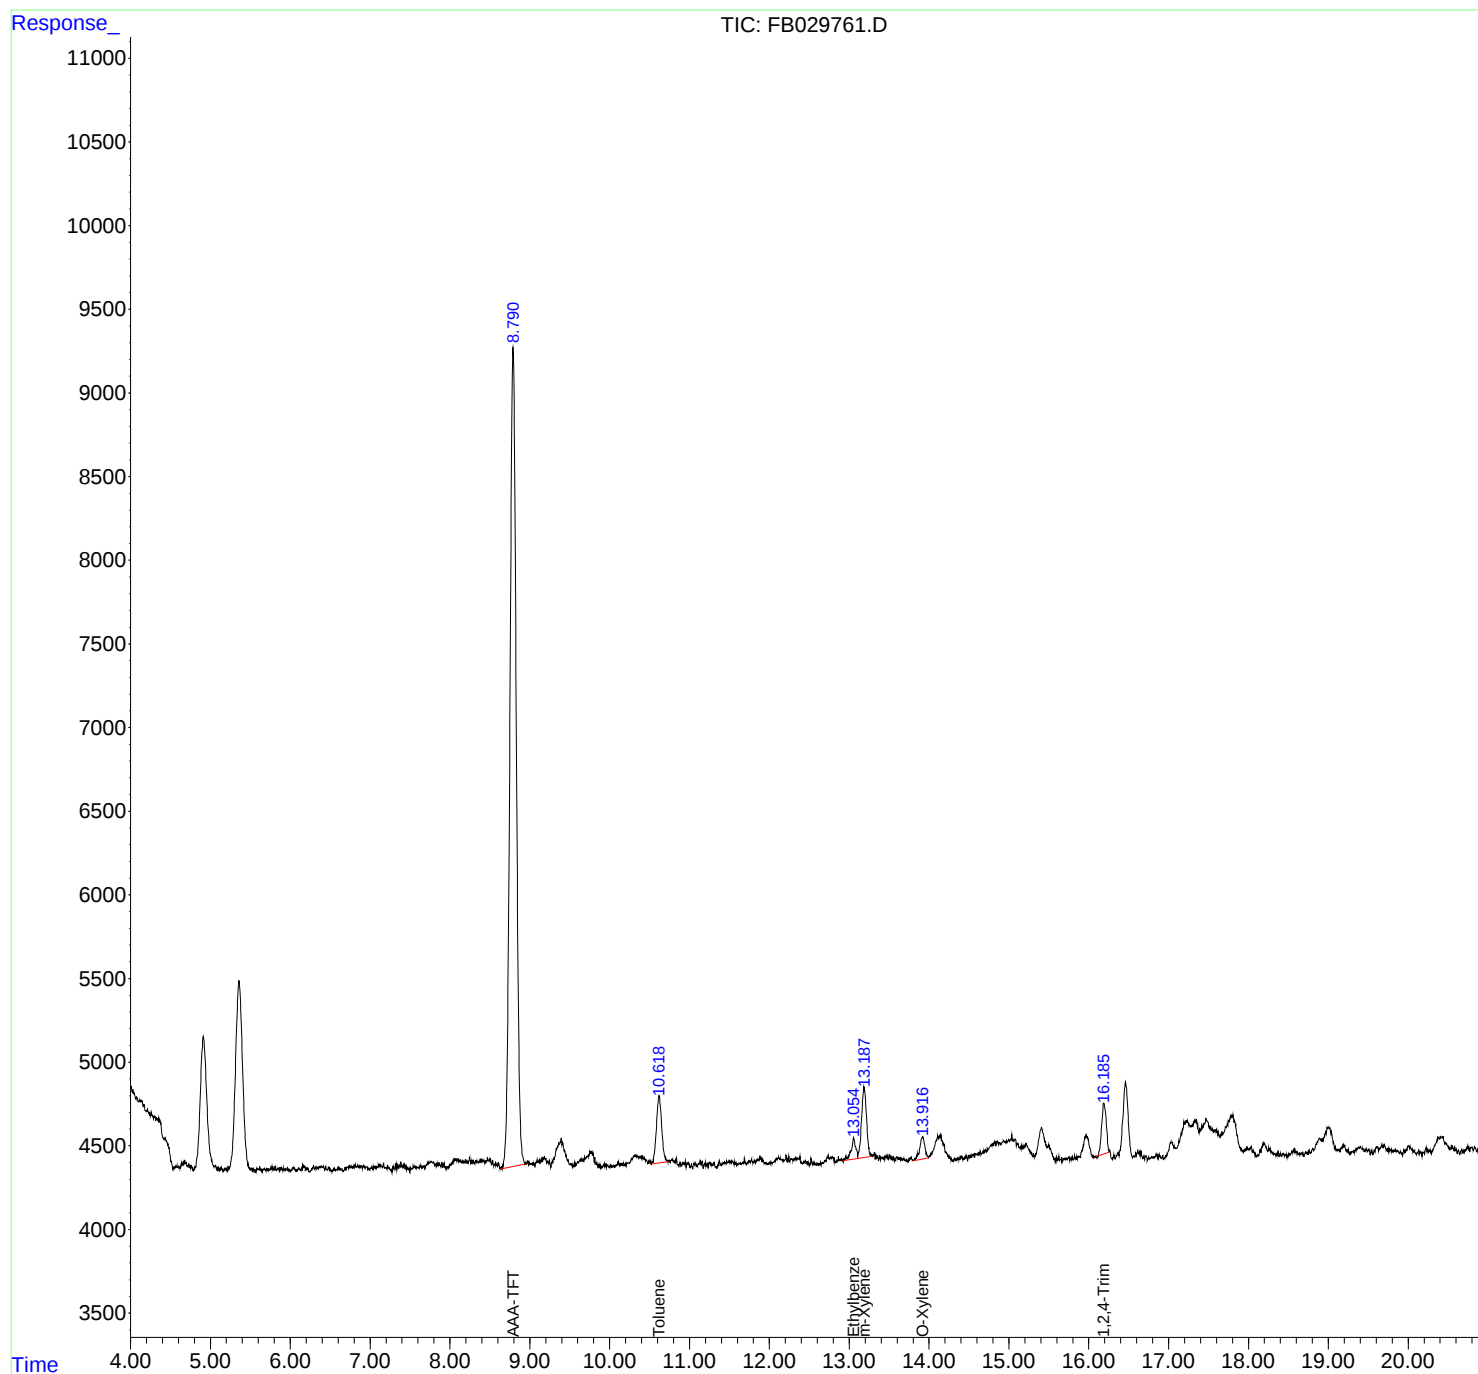


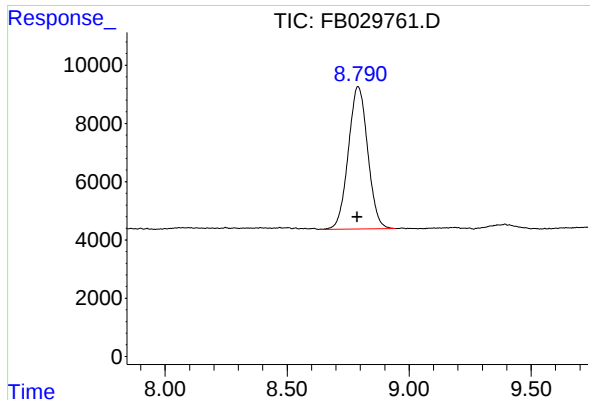

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.004 min
Response: 269925
Conc: 20.26 ng/ml

Instrument :
FID_B
ClientSampleId :

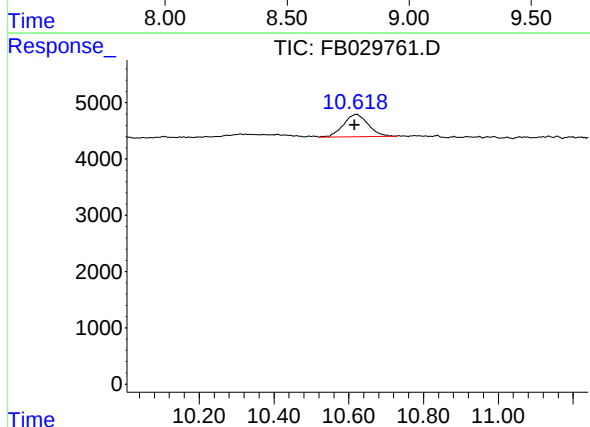


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.004 min
Response: 18222
Conc: 0.94 ng/ml

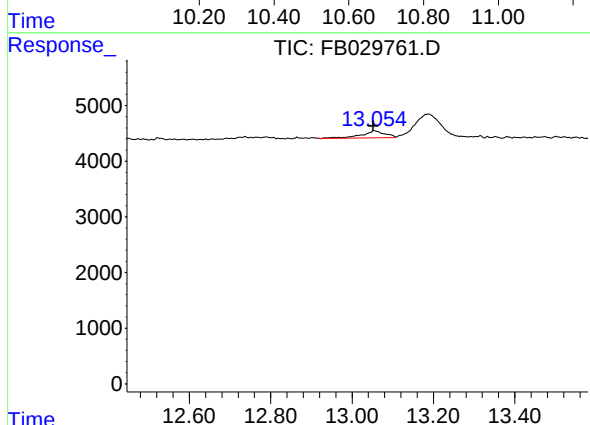


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.004 min
Response: 4936
Conc: 0.27 ng/ml

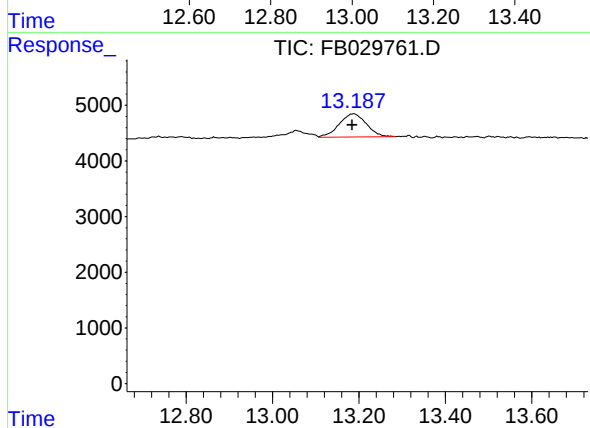

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.004 min
Response: 18101
Conc: 1.00 ng/ml

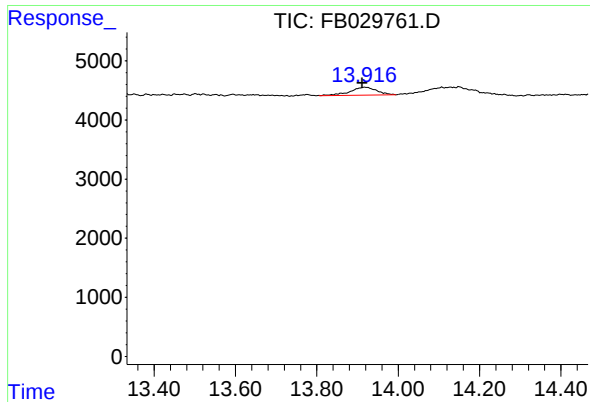

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.007 min
Response: 5935
Conc: 0.34 ng/ml

Instrument :
FID_B
ClientSampleId :

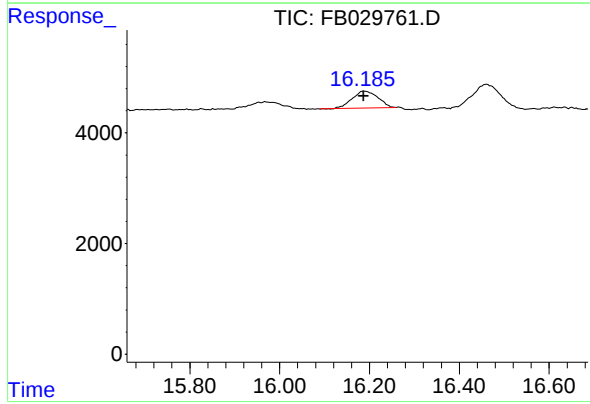

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.000 min
Response: 12054
Conc: 0.67 ng/ml