

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050123\
Data File : FB029765.D
Signal(s) : FID2B.CH
Acq On : 1 May 2023 17:59
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 02 01:43:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	269905	20.254 ng/ml
Target Compounds			
6) t Toluene	10.620	9707	0.503 ng/ml
8) t m-Xylene	13.186	9553	0.528 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	9106	0.510 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050123\
Data File : FB029765.D
Signal(s) : FID2B.CH
Acq On : 1 May 2023 17:59
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 02 01:43:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

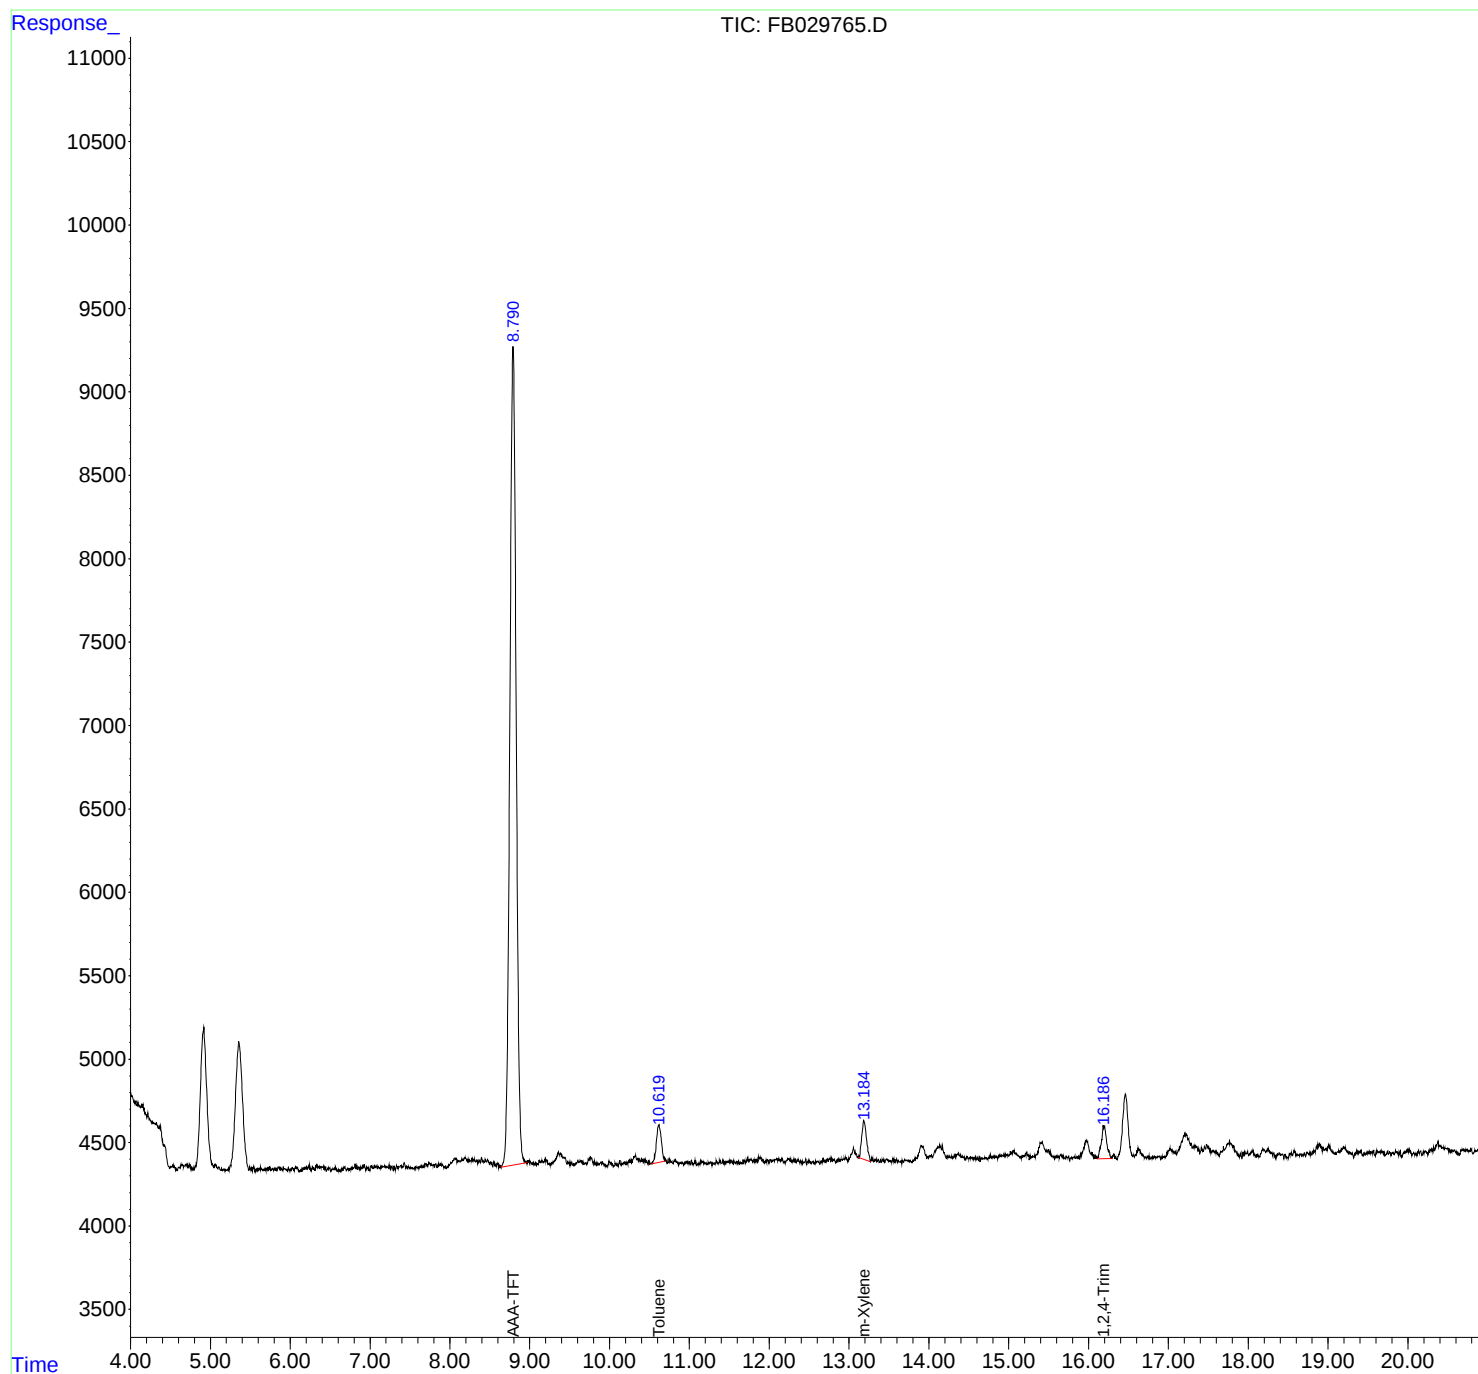


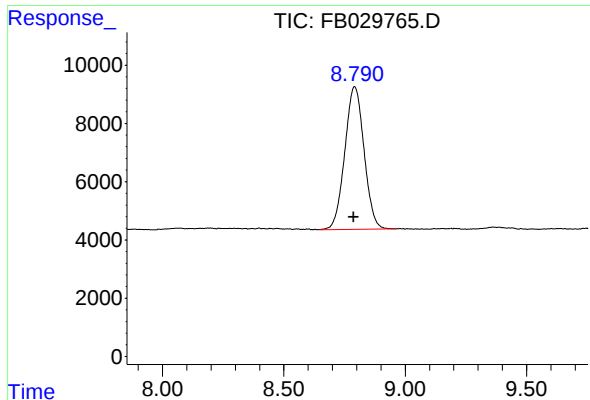

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.004 min
Response: 269905
Conc: 20.25 ng/ml

Instrument :
FID_B
ClientSampleId :

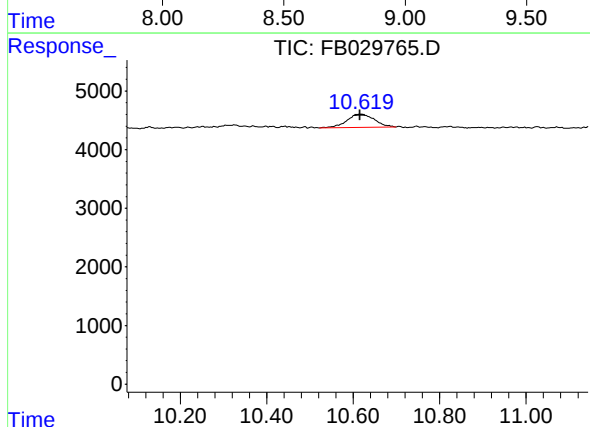


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.005 min
Response: 9707
Conc: 0.50 ng/ml

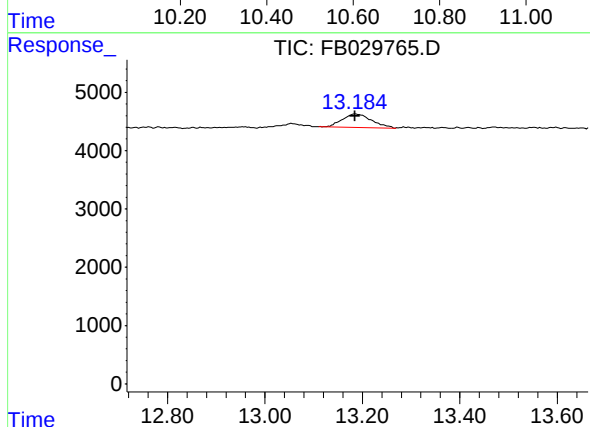

#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: 0.001 min
Response: 9553
Conc: 0.53 ng/ml

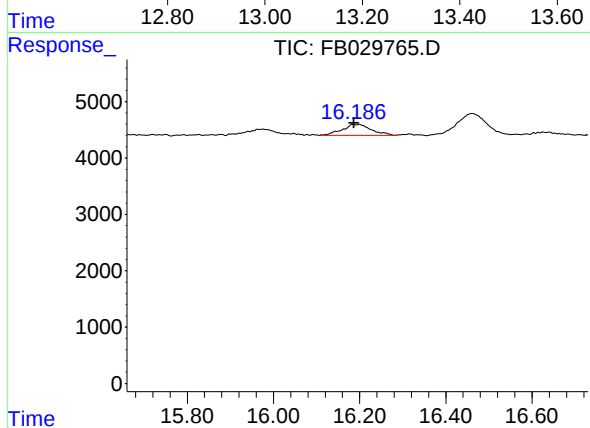

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.000 min
Response: 9106
Conc: 0.51 ng/ml