

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050422\
 Data File : FB027113.D
 Signal(s) : FID2B.CH
 Acq On : 4 May 2022 18:23
 Operator : AJ/MA
 Sample : BSF0504S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 05 02:22:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	292034	25.831 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	584364	31.044 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	605574	30.270 ng/ml
3) t n-Heptane	7.750	200252	10.237 ng/ml
4) t Benzene	7.886	230549	10.447 ng/ml
6) t Toluene	10.619	652217	31.630 ng/ml
7) t Ethylbenzene	13.055	202691	10.608 ng/ml
8) t m-Xylene	13.188	403707	21.372 ng/ml
9) t O-Xylene	13.914	386718	21.350 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	406723	22.067 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050422\
Data File : FB027113.D
Signal(s) : FID2B.CH
Acq On : 4 May 2022 18:23
Operator : AJ/MA
Sample : BSF0504S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 05 02:22:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

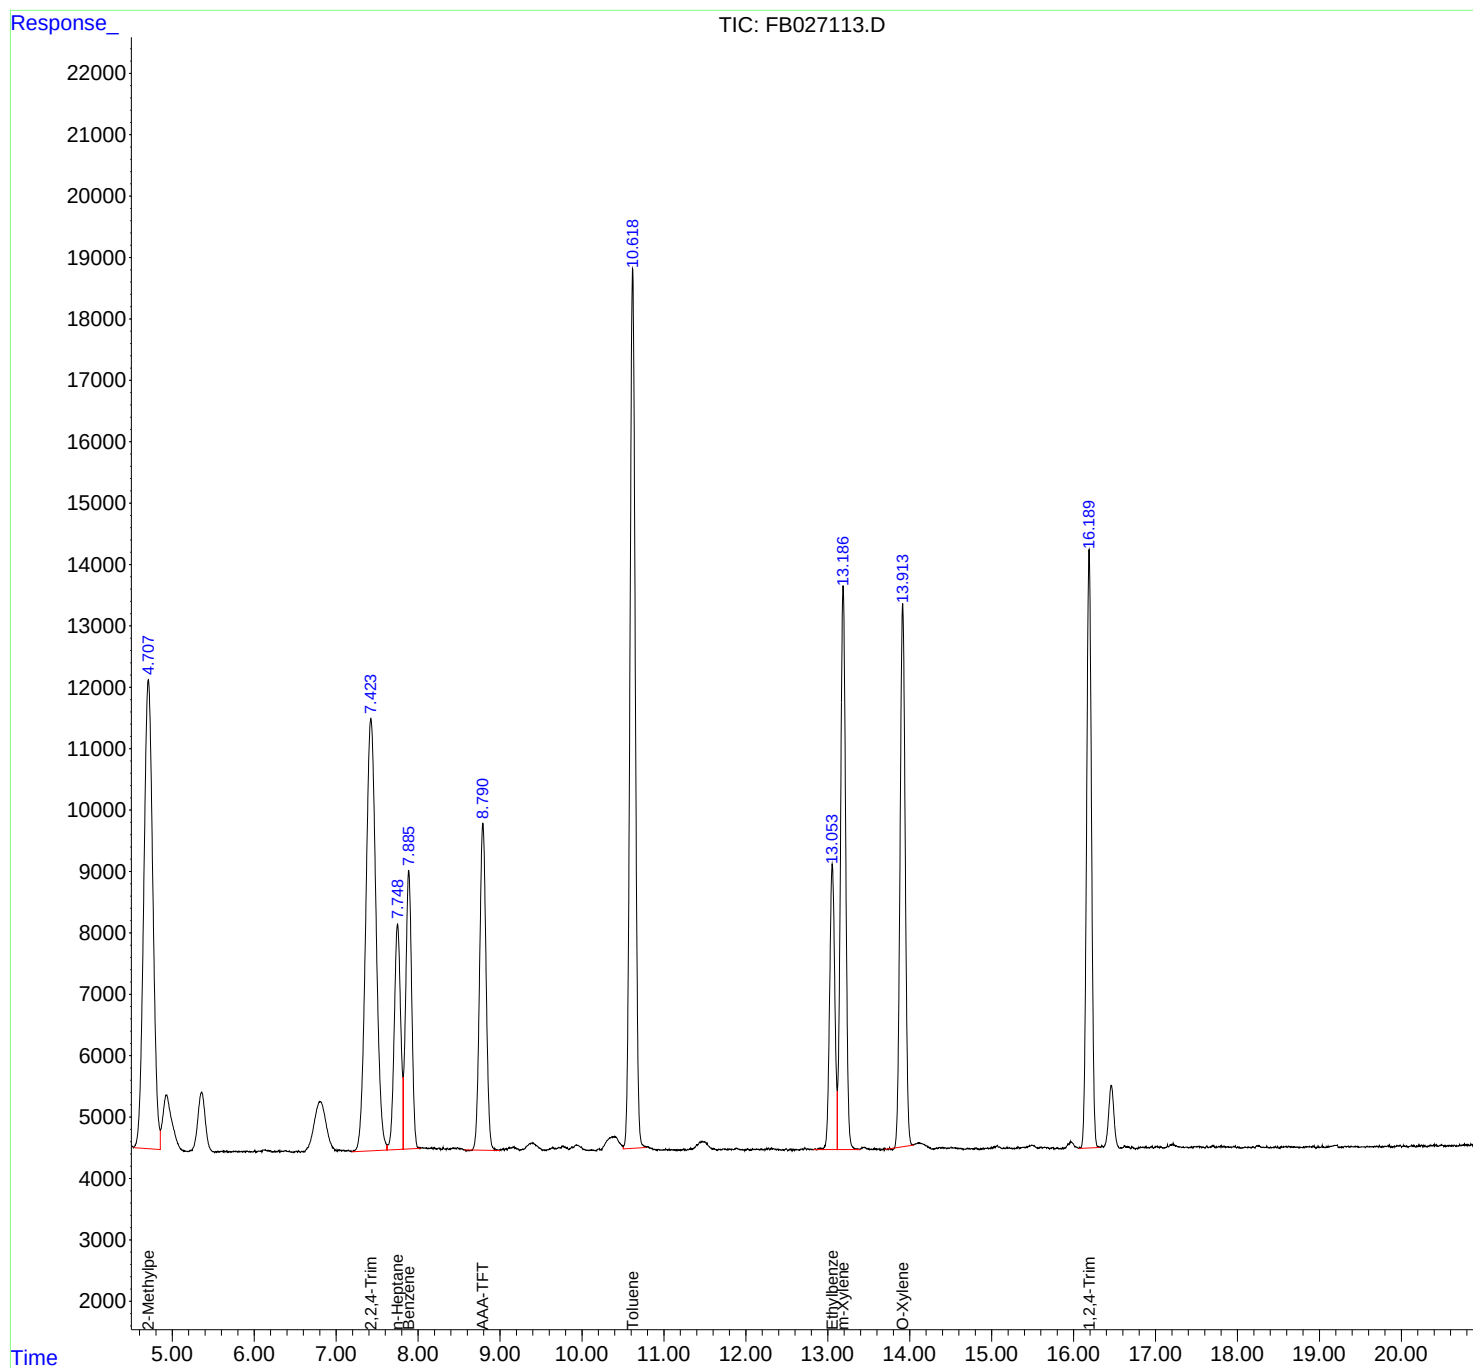

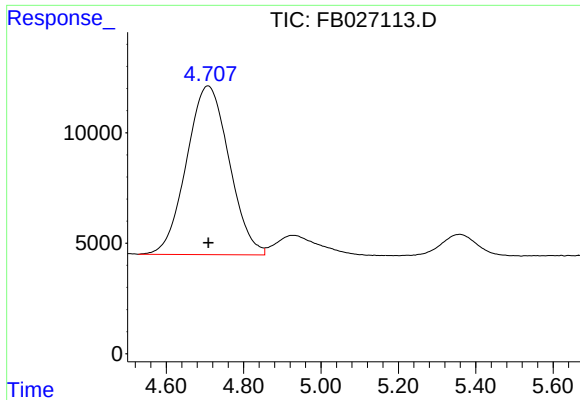


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 584364
Conc: 31.04 ng/ml

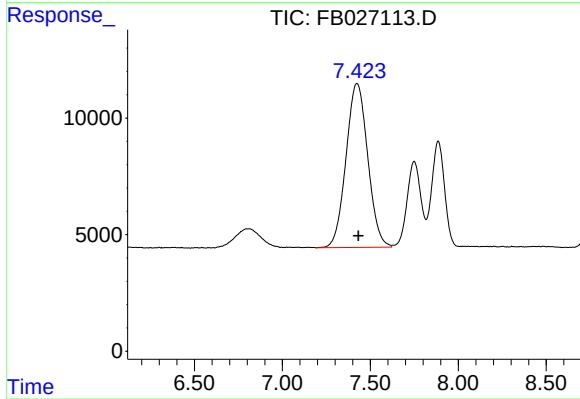


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.009 min
Response: 605574
Conc: 30.27 ng/ml

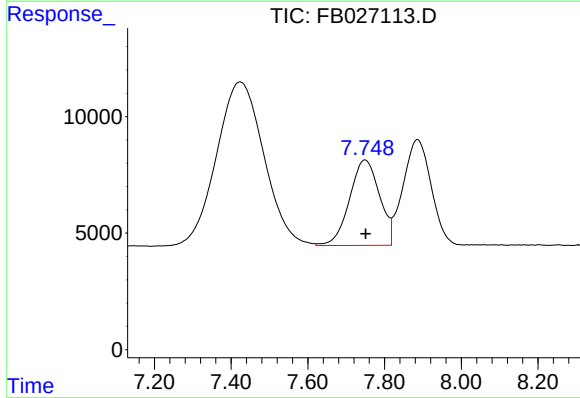


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 200252
Conc: 10.24 ng/ml

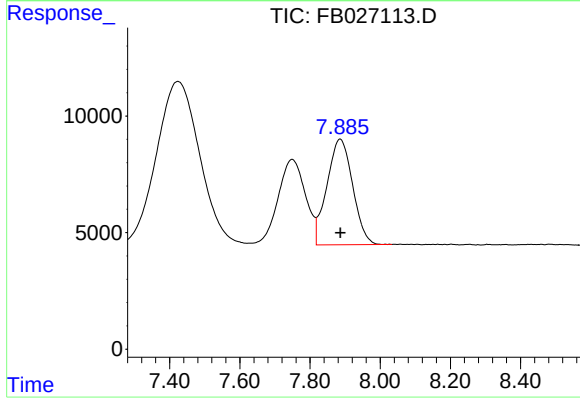


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 230549
Conc: 10.45 ng/ml

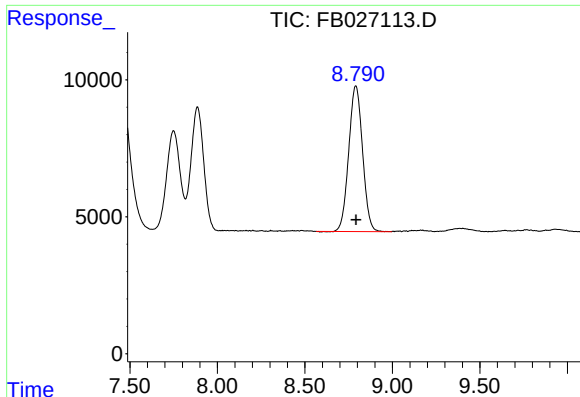


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 292034
Conc: 25.83 ng/ml

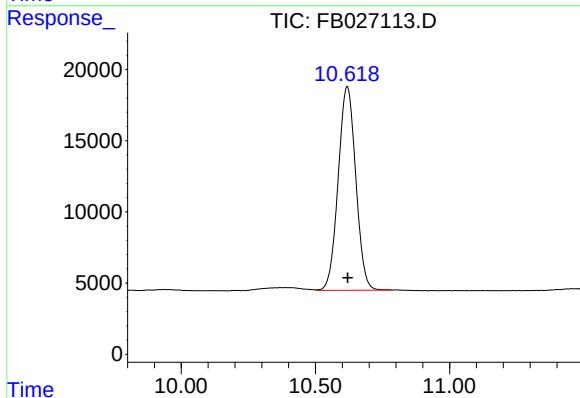


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 652217
Conc: 31.63 ng/ml

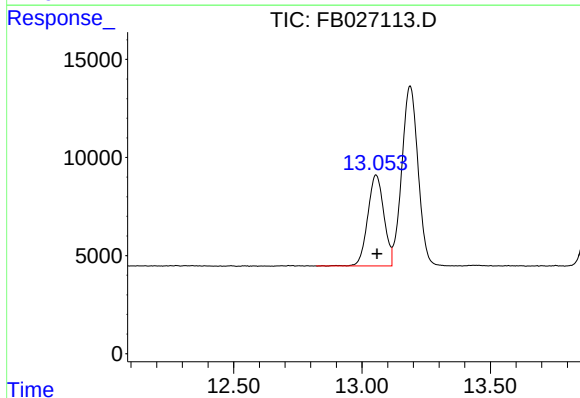


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.003 min
Response: 202691
Conc: 10.61 ng/ml

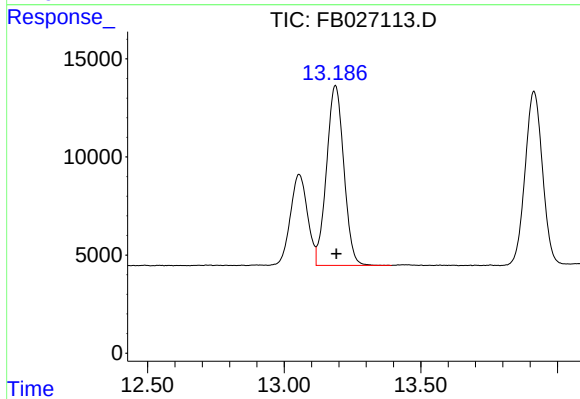


#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: -0.004 min
Response: 403707
Conc: 21.37 ng/ml

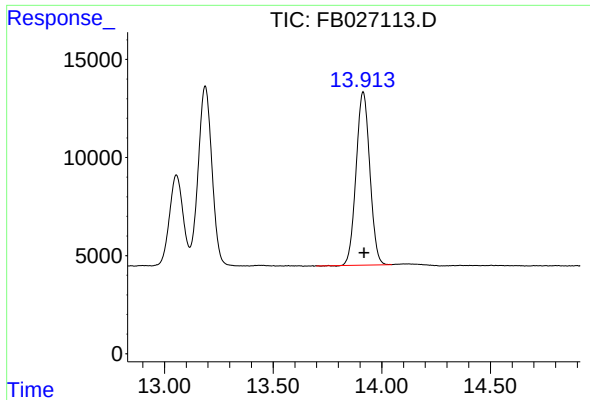

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.004 min
Response: 386718
Conc: 21.35 ng/ml

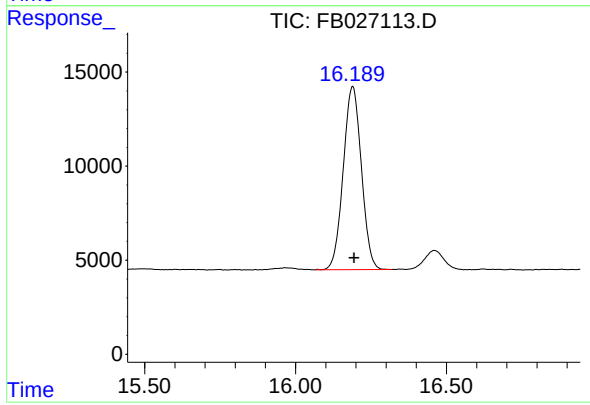

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 406723
Conc: 22.07 ng/ml