

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050619\
 Data File : FB020978.D
 Signal(s) : FID2B.CH
 Acq On : 6 May 2019 14:56
 Operator : MJ/SJ
 Sample : 20 PPB GRO STD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 07 03:14:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	363730	20.275 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.858	1257600	27.879 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	1175548	28.202 ng/ml
3) t n-Heptane	7.952	365357	9.229 ng/ml
4) t Benzene	8.088	398246	9.519 ng/ml
6) t Toluene	10.840	781727	28.220 ng/ml
7) t Ethylbenzene	13.291	254013	9.057 ng/ml
8) t m-Xylene	13.424	547916	18.436 ng/ml
9) t O-Xylene	14.155	562308	18.141 ng/ml
10) t 1,2,4-Trimethylbenzene	16.439	573420	18.489 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050619\
Data File : FB020978.D
Signal(s) : FID2B.CH
Acq On : 6 May 2019 14:56
Operator : MJ/SJ
Sample : 20 PPB GRO STD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 07 03:14:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

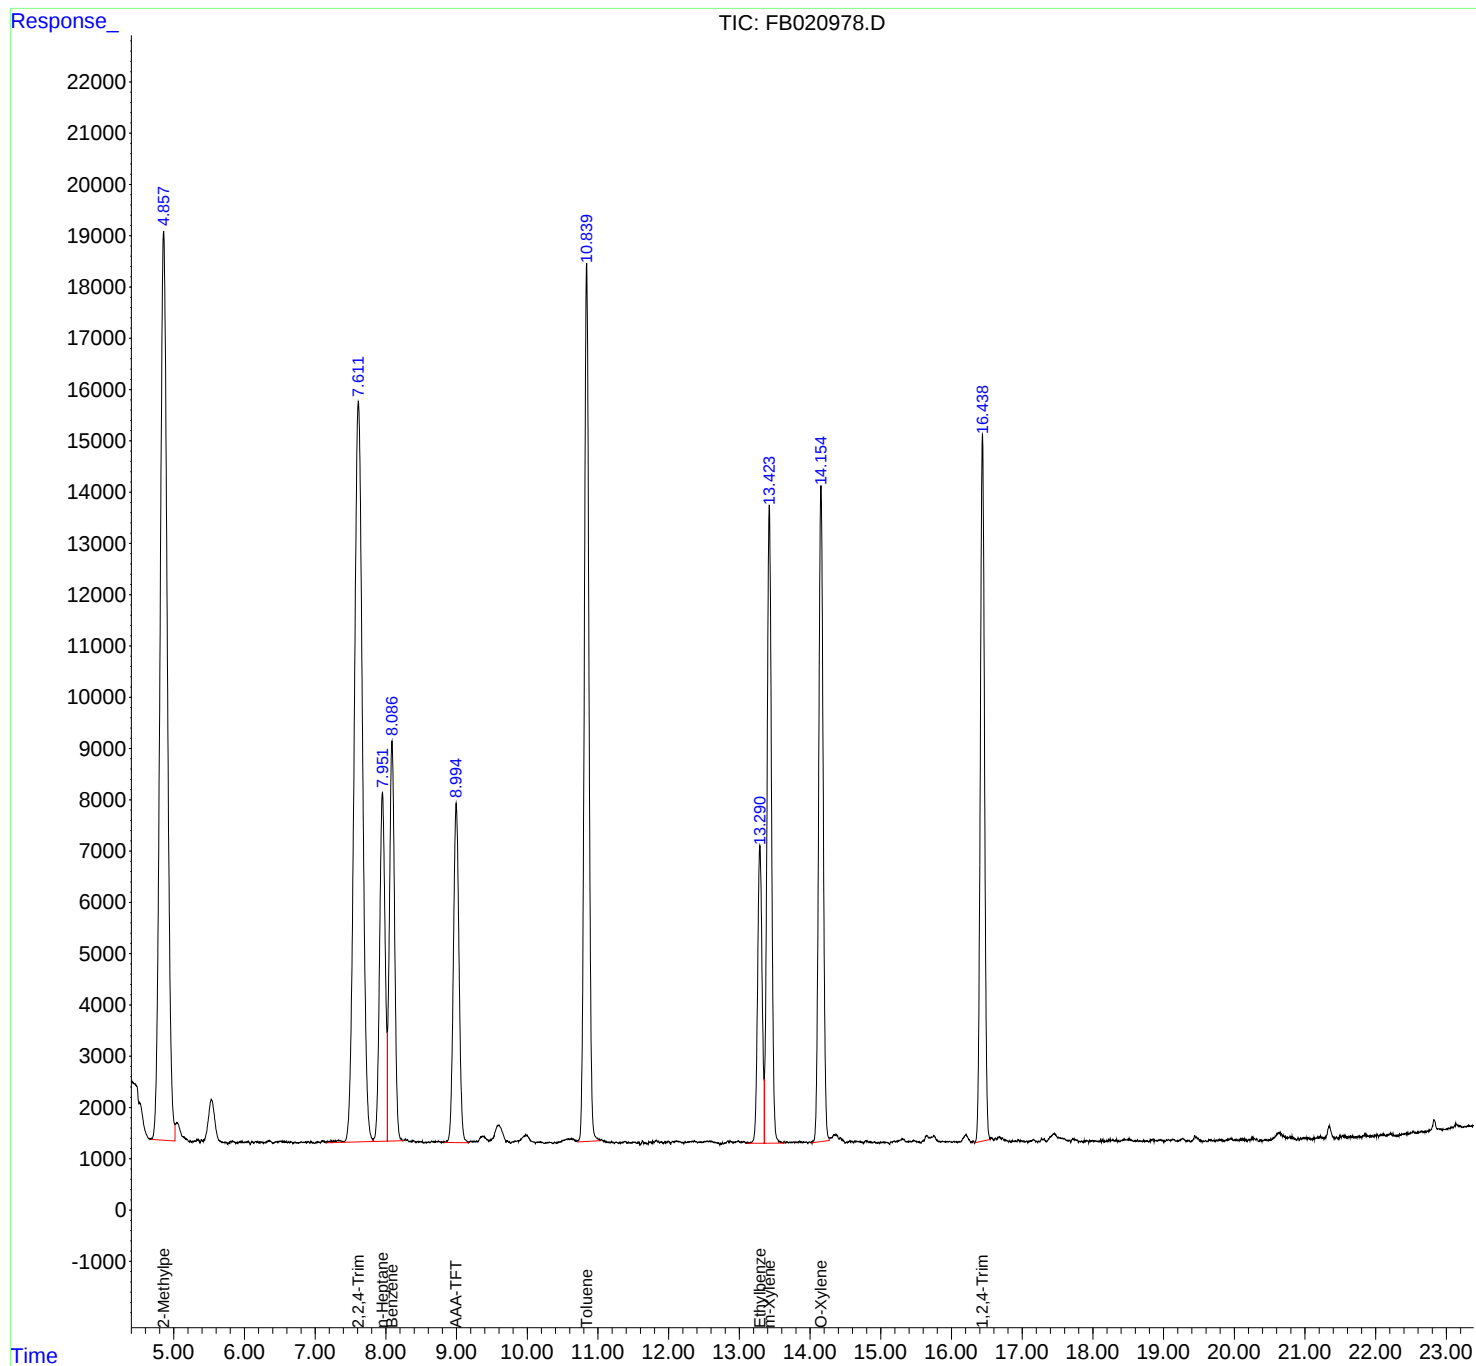

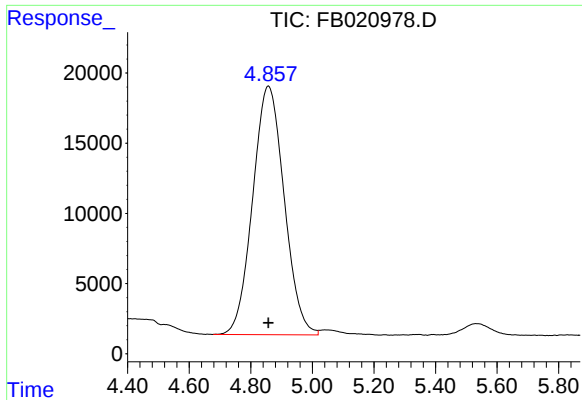


#1 2-Methylpentane

R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 1257600
Conc: 27.88 ng/ml

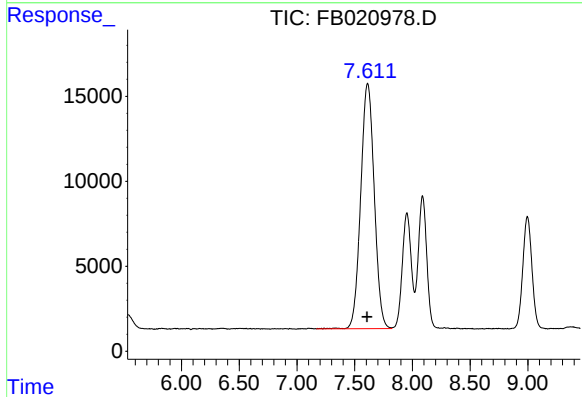


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.003 min
Response: 1175548
Conc: 28.20 ng/ml

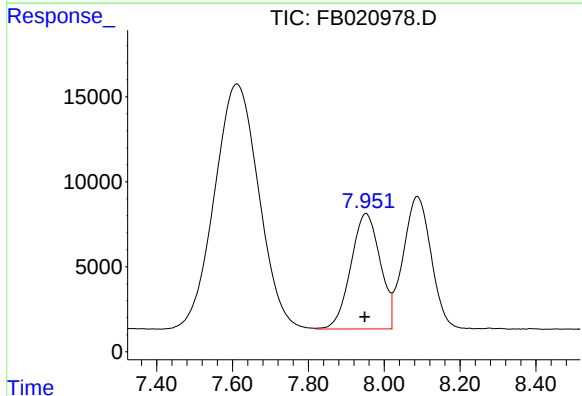


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.004 min
Response: 365357
Conc: 9.23 ng/ml

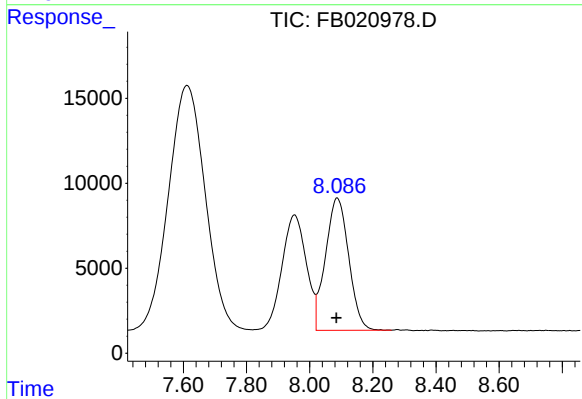


#4 Benzene

R.T.: 8.088 min
Delta R.T.: 0.003 min
Response: 398246
Conc: 9.52 ng/ml

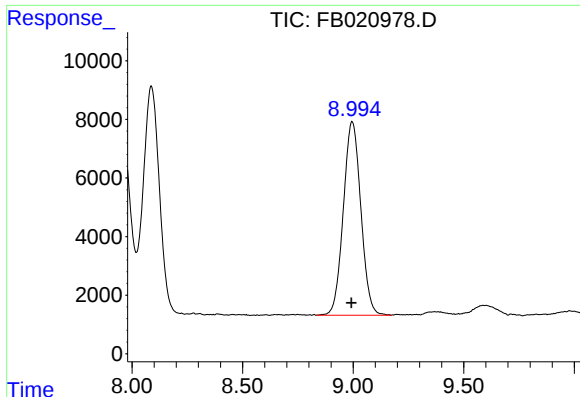


#5 AAA-TFT

R.T.: 8.996 min
Delta R.T.: 0.004 min
Response: 363730
Conc: 20.28 ng/ml

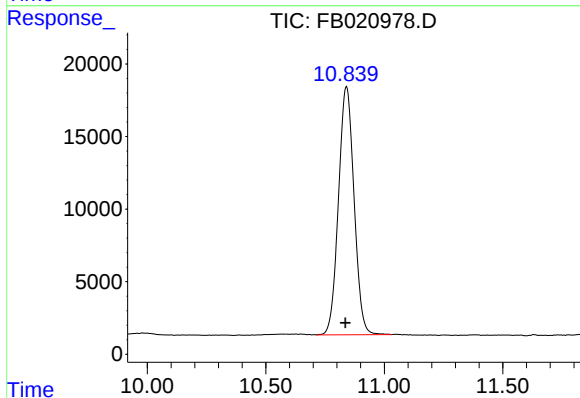


#6 Toluene

R.T.: 10.840 min
Delta R.T.: 0.005 min
Response: 781727
Conc: 28.22 ng/ml

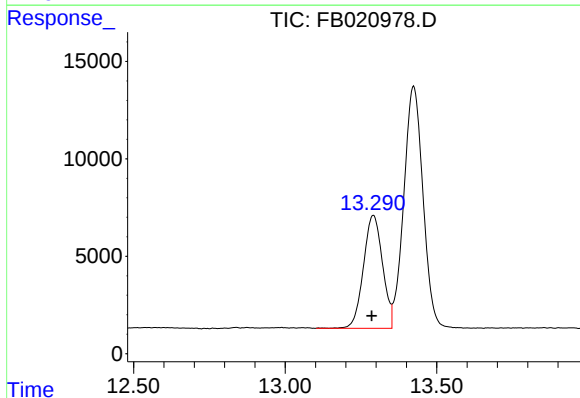


#7 Ethylbenzene

R.T.: 13.291 min
Delta R.T.: 0.005 min
Response: 254013
Conc: 9.06 ng/ml

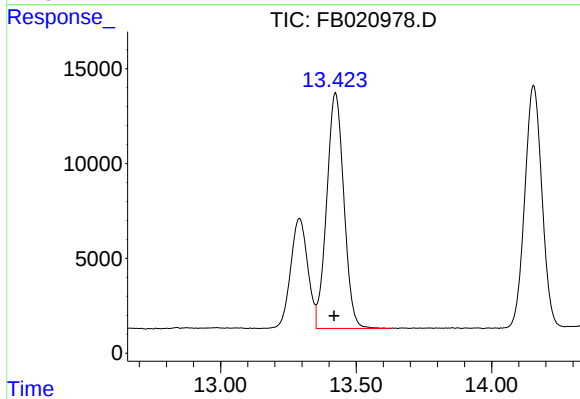

#8 m-Xylene

R.T.: 13.424 min
Delta R.T.: 0.005 min
Response: 547916
Conc: 18.44 ng/ml

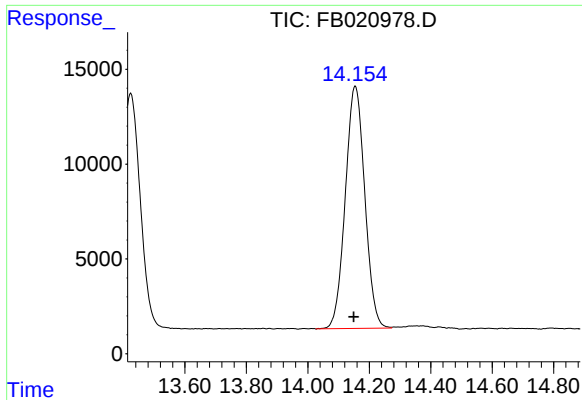


#9 O-Xylene

R.T.: 14.155 min

Delta R.T.: 0.006 min

Response: 562308

Conc: 18.14 ng/ml

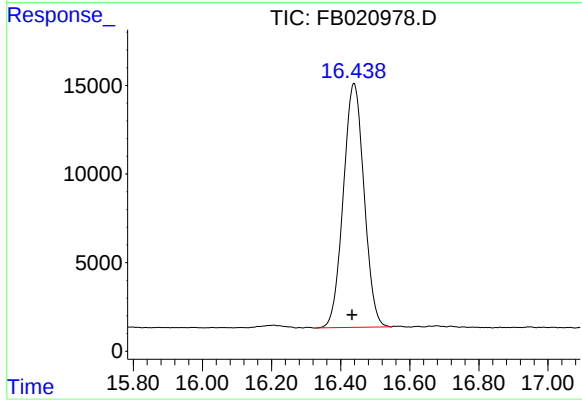

#10 1,2,4-Trimethylbenzene

R.T.: 16.439 min

Delta R.T.: 0.006 min

Response: 573420

Conc: 18.49 ng/ml