

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050622\
 Data File : FB027119.D
 Signal(s) : FID2B.CH
 Acq On : 6 May 2022 12:07
 Operator : AJ/MA
 Sample : BSF0506S1
 Misc : 5.01G/5.00 ML WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 08 22:36:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	239165	21.155 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	568452	30.199 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	582093	29.097 ng/ml
3) t n-Heptane	7.750	204330	10.445 ng/ml
4) t Benzene	7.886	229791	10.412 ng/ml
6) t Toluene	10.619	661257	32.069 ng/ml
7) t Ethylbenzene	13.055	198617	10.395 ng/ml
8) t m-Xylene	13.188	396619	20.997 ng/ml
9) t O-Xylene	13.915	383499	21.172 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	387071	21.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050622\
Data File : FB027119.D
Signal(s) : FID2B.CH
Acq On : 6 May 2022 12:07
Operator : AJ/MA
Sample : BSF0506S1
Misc : 5.01G/5.00 ML WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 08 22:36:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

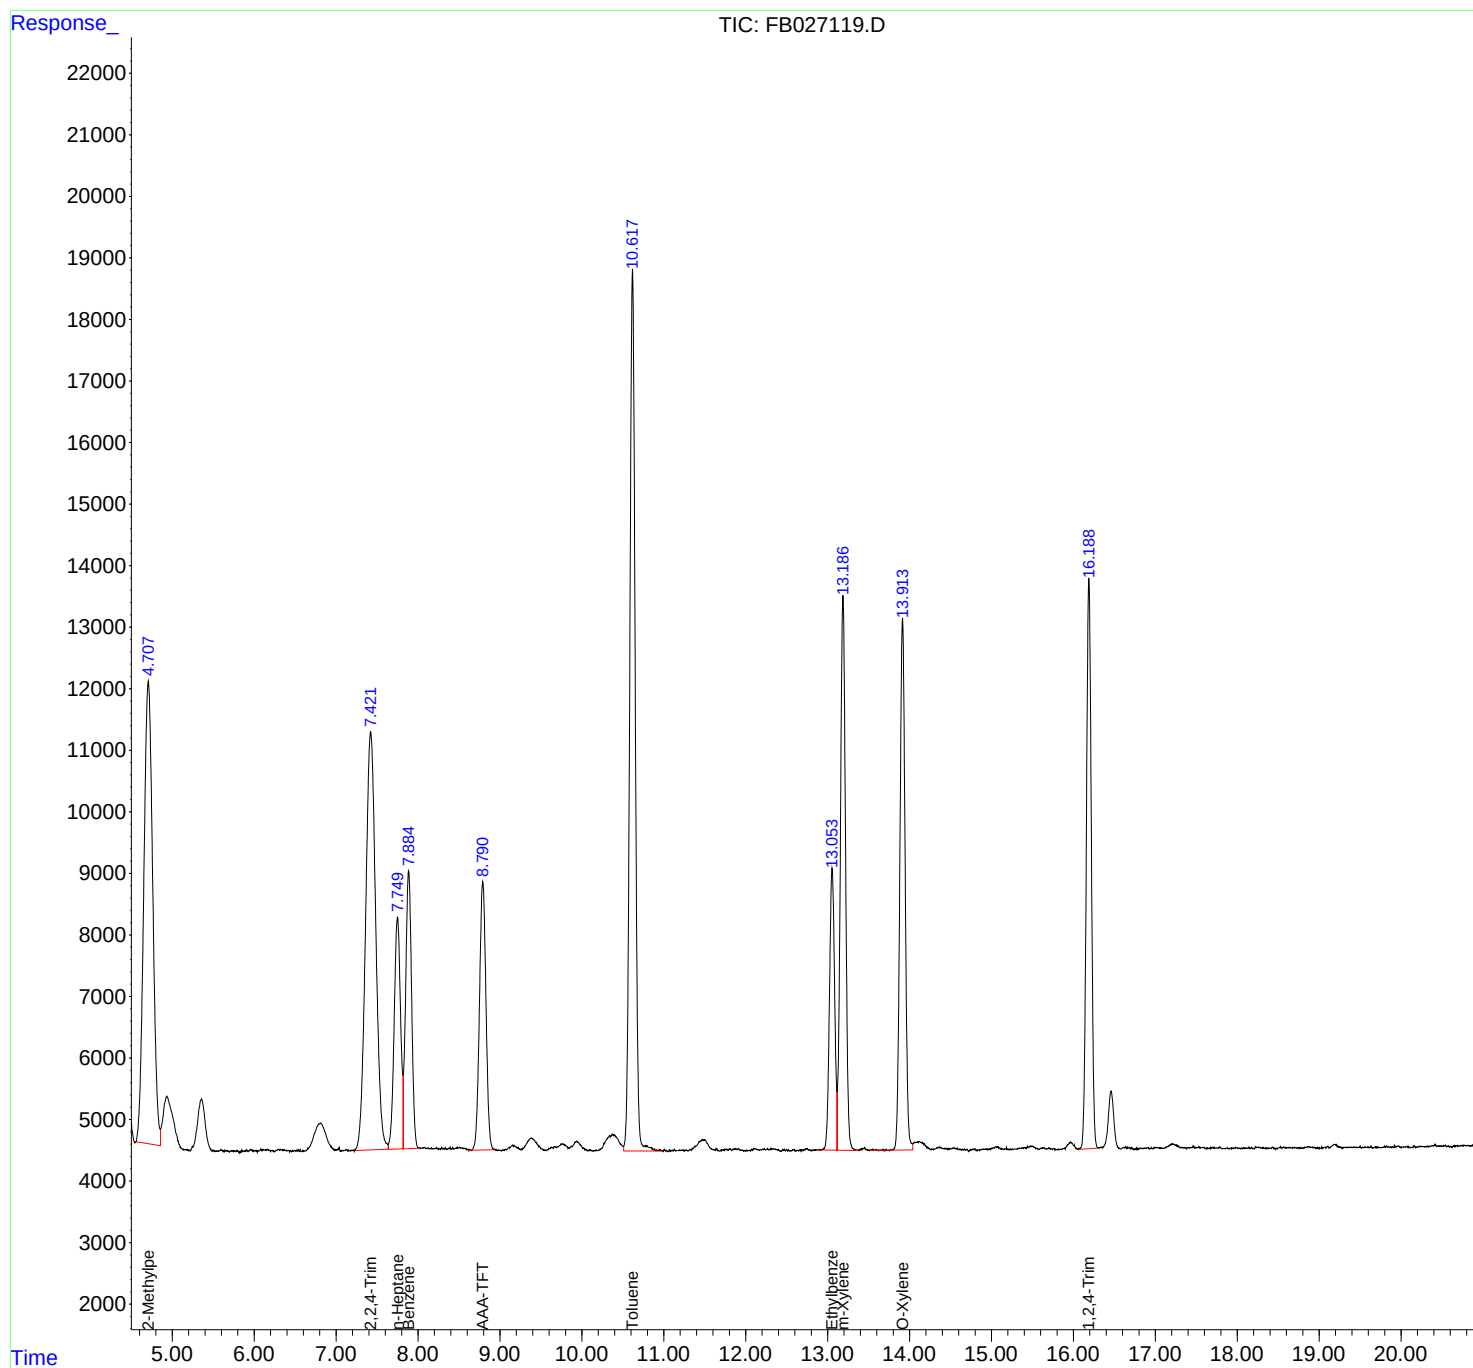


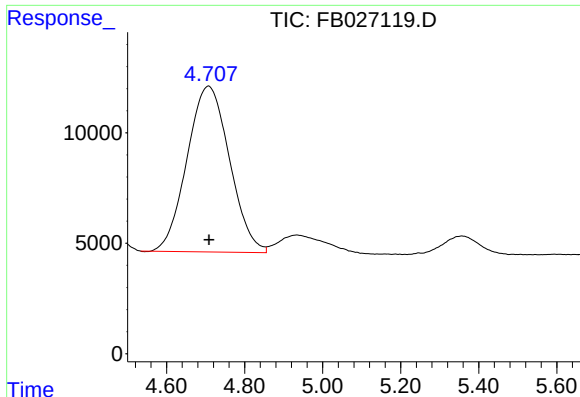

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 568452
Conc: 30.20 ng/ml

Instrument :
FID_B
ClientSampleId :

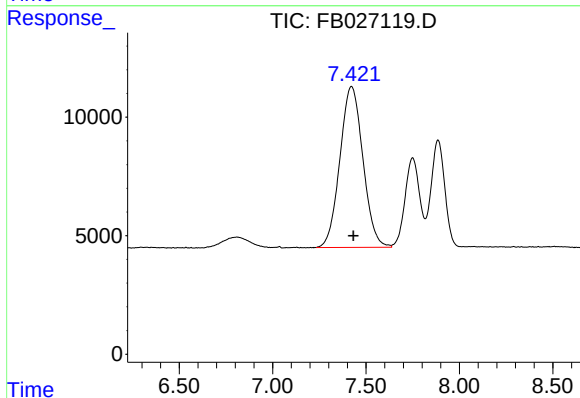


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: -0.011 min
Response: 582093
Conc: 29.10 ng/ml

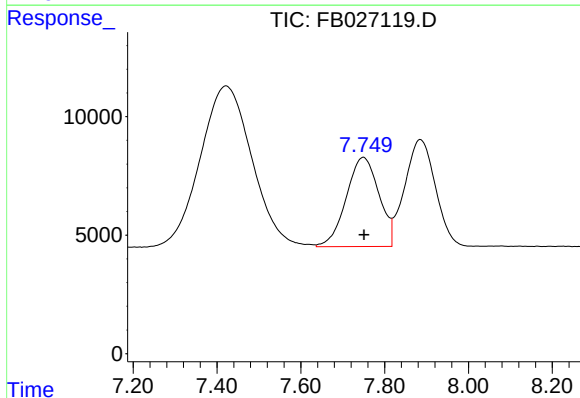


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 204330
Conc: 10.45 ng/ml

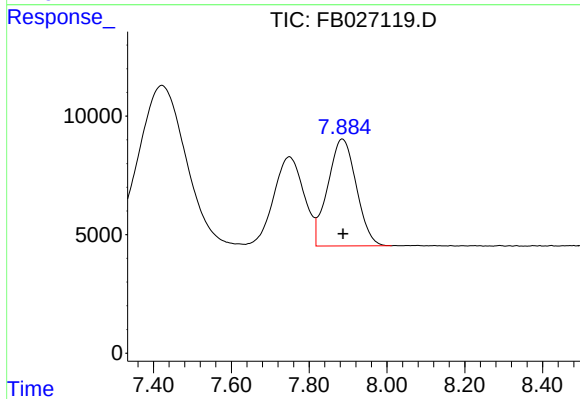

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.001 min
Response: 229791
Conc: 10.41 ng/ml

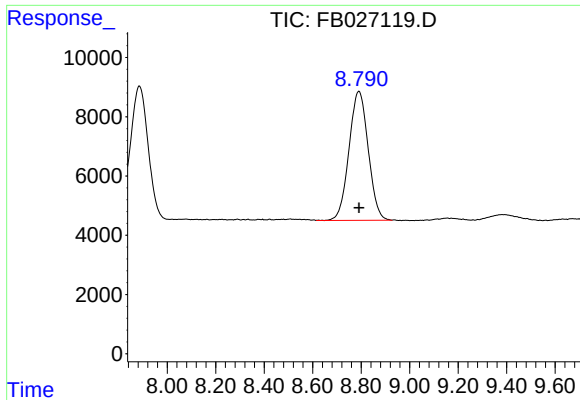

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 239165
Conc: 21.15 ng/ml

Instrument :
FID_B
ClientSampleId :

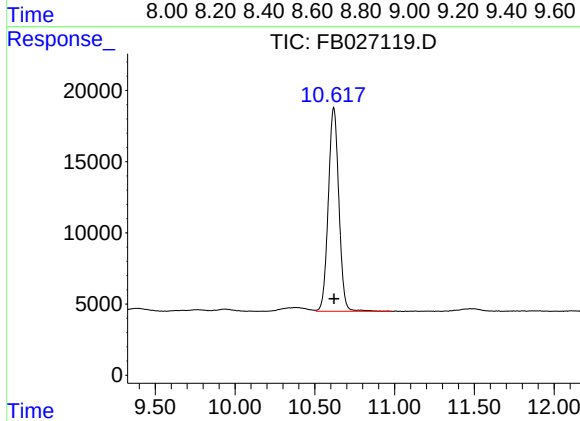


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 661257
Conc: 32.07 ng/ml

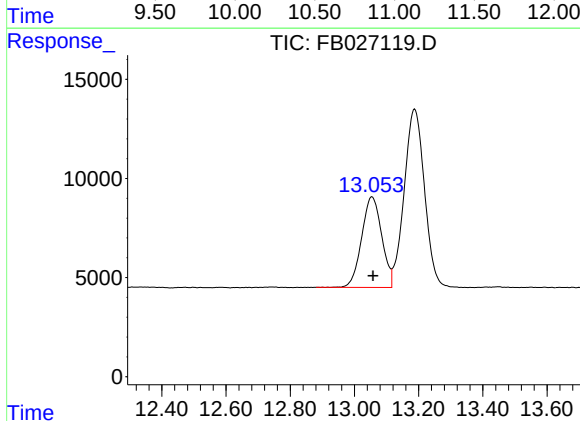


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.003 min
Response: 198617
Conc: 10.40 ng/ml

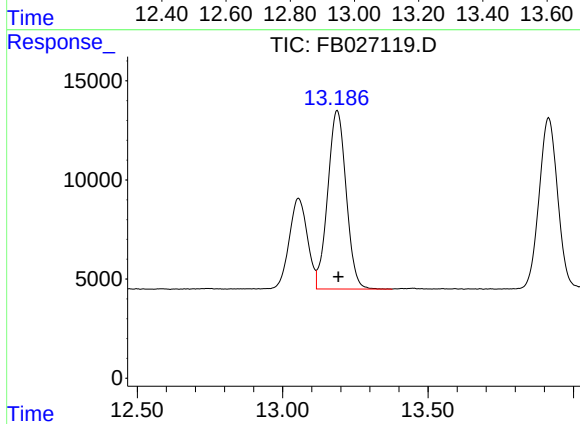

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.004 min
Response: 396619
Conc: 21.00 ng/ml

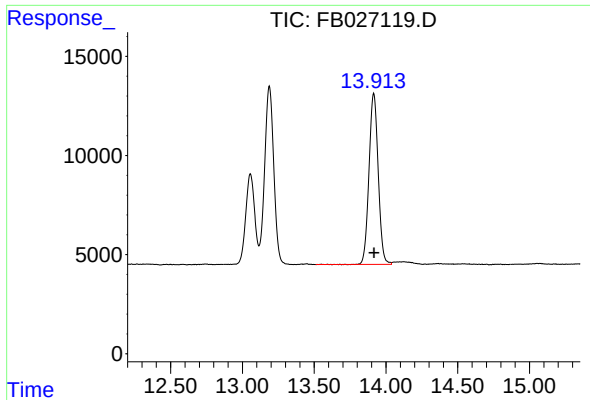

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.003 min
Response: 383499
Conc: 21.17 ng/ml

Instrument :
FID_B
ClientSampleId :

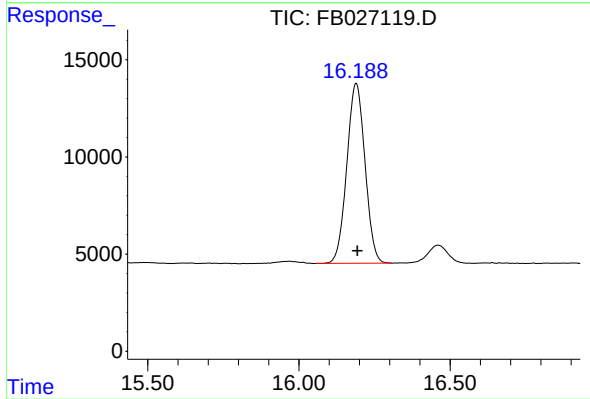

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 387071
Conc: 21.00 ng/ml